

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062022AL\
Data File : FC060367.D
Signal(s) : FID1A.CH
Acq On : 21 Jun 2022 1:27
Operator : UA/NP
Sample : N3213-06DL2 50X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 05:07:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052722.M
Quant Title : GC Extractables
QLast Update : Sat May 28 08:22:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
5) T	A~2-methylnaphthalene...	6.264f	182491	1.243 ug/ml
22) T	n-Tetracontane (C40)	20.330	391035	4.156 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062022AL\
Data File : FC060367.D
Signal(s) : FID1A.CH
Acq On : 21 Jun 2022 1:27
Operator : UA/NP
Sample : N3213-06DL2 50X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 05:07:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052722.M
Quant Title : GC Extractables
QLast Update : Sat May 28 08:22:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

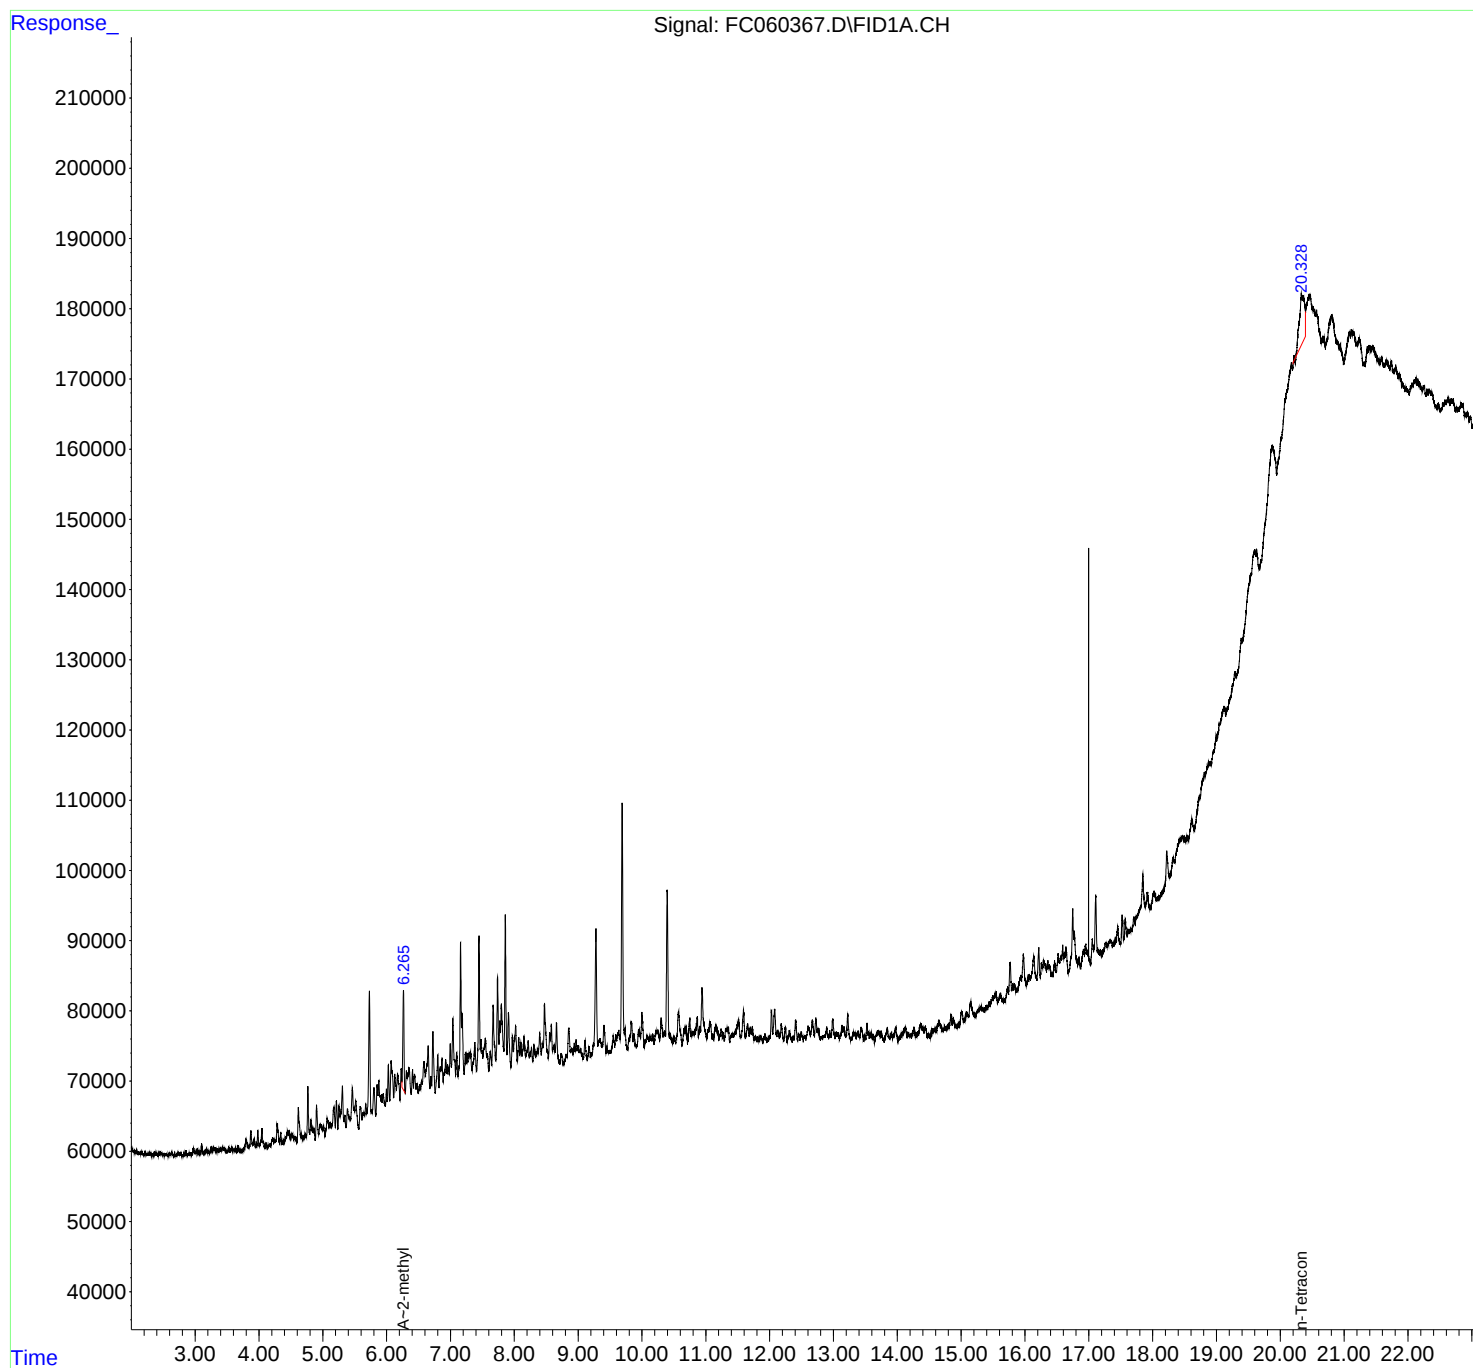


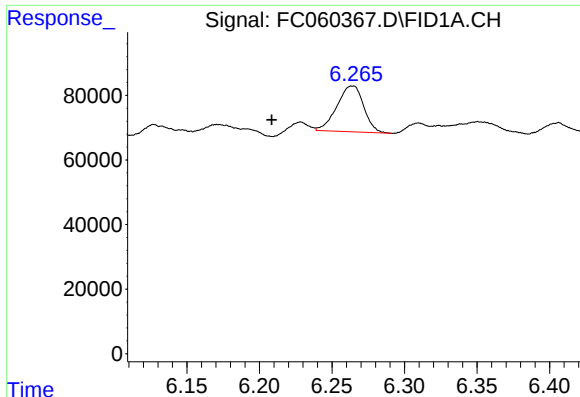

#5 A~2-methylnaphthalene (C12.89)


R.T.: 6.264 min
Delta R.T.: 0.055 min
Response: 182491
Conc: 1.24 ug/ml

Instrument :
FID_C
ClientSampleId :

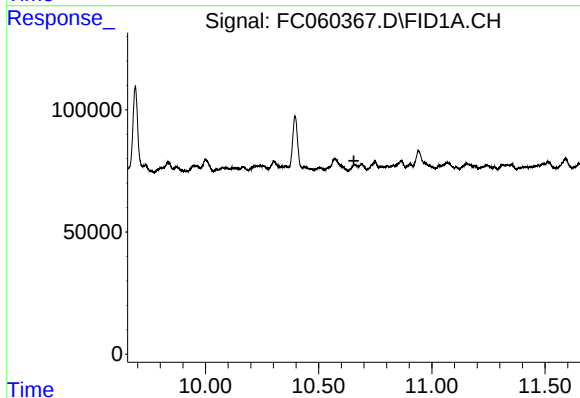


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 10.656 min
Response: 0
Conc: N.D.

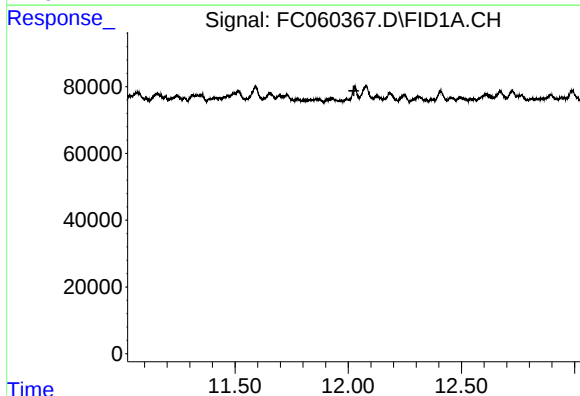

#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 12.025 min
Response: 0
Conc: N.D.

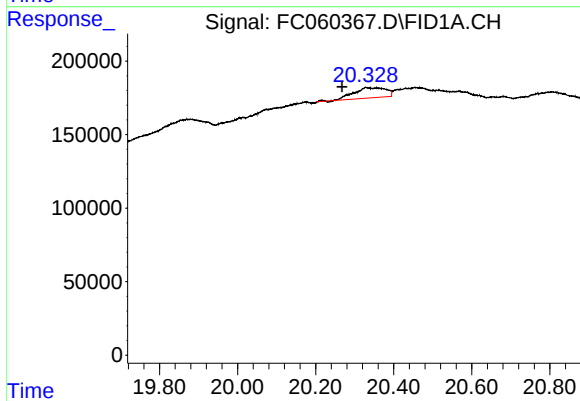

#22 n-Tetracontane (C40)

R.T.: 20.330 min
Delta R.T.: 0.062 min
Response: 391035
Conc: 4.16 ug/ml