

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062022AL\
 Data File : FC060377.D
 Signal(s) : FID1A.CH
 Acq On : 21 Jun 2022 8:24
 Operator : UA/NP
 Sample : N3404-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 14A-TP-7-(14.5-15.0)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/21/2022
 Supervised By :Ankita Jodhani 06/22/2022

Integration File: autoint1.e
 Quant Time: Jun 21 09:32:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052722.M
 Quant Title : GC Extractables
 QLast Update : Sat May 28 08:22:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.664	3521439	22.628 ug/mlm
Spiked Amount 50.000		Recovery =	45.26%
12) S 1-chlorooctadecane (S...	12.025	162959	1.314 ug/mlm
Spiked Amount 50.000		Recovery =	2.63%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062022AL\
Data File : FC060377.D
Signal(s) : FID1A.CH
Acq On : 21 Jun 2022 8:24
Operator : UA/NP
Sample : N3404-01
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
14A-TP-7-(14.5-15.0)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/21/2022
Supervised By :Ankita Jodhani 06/22/2022

Integration File: autoint1.e
Quant Time: Jun 21 09:32:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052722.M
Quant Title : GC Extractables
QLast Update : Sat May 28 08:22:04 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

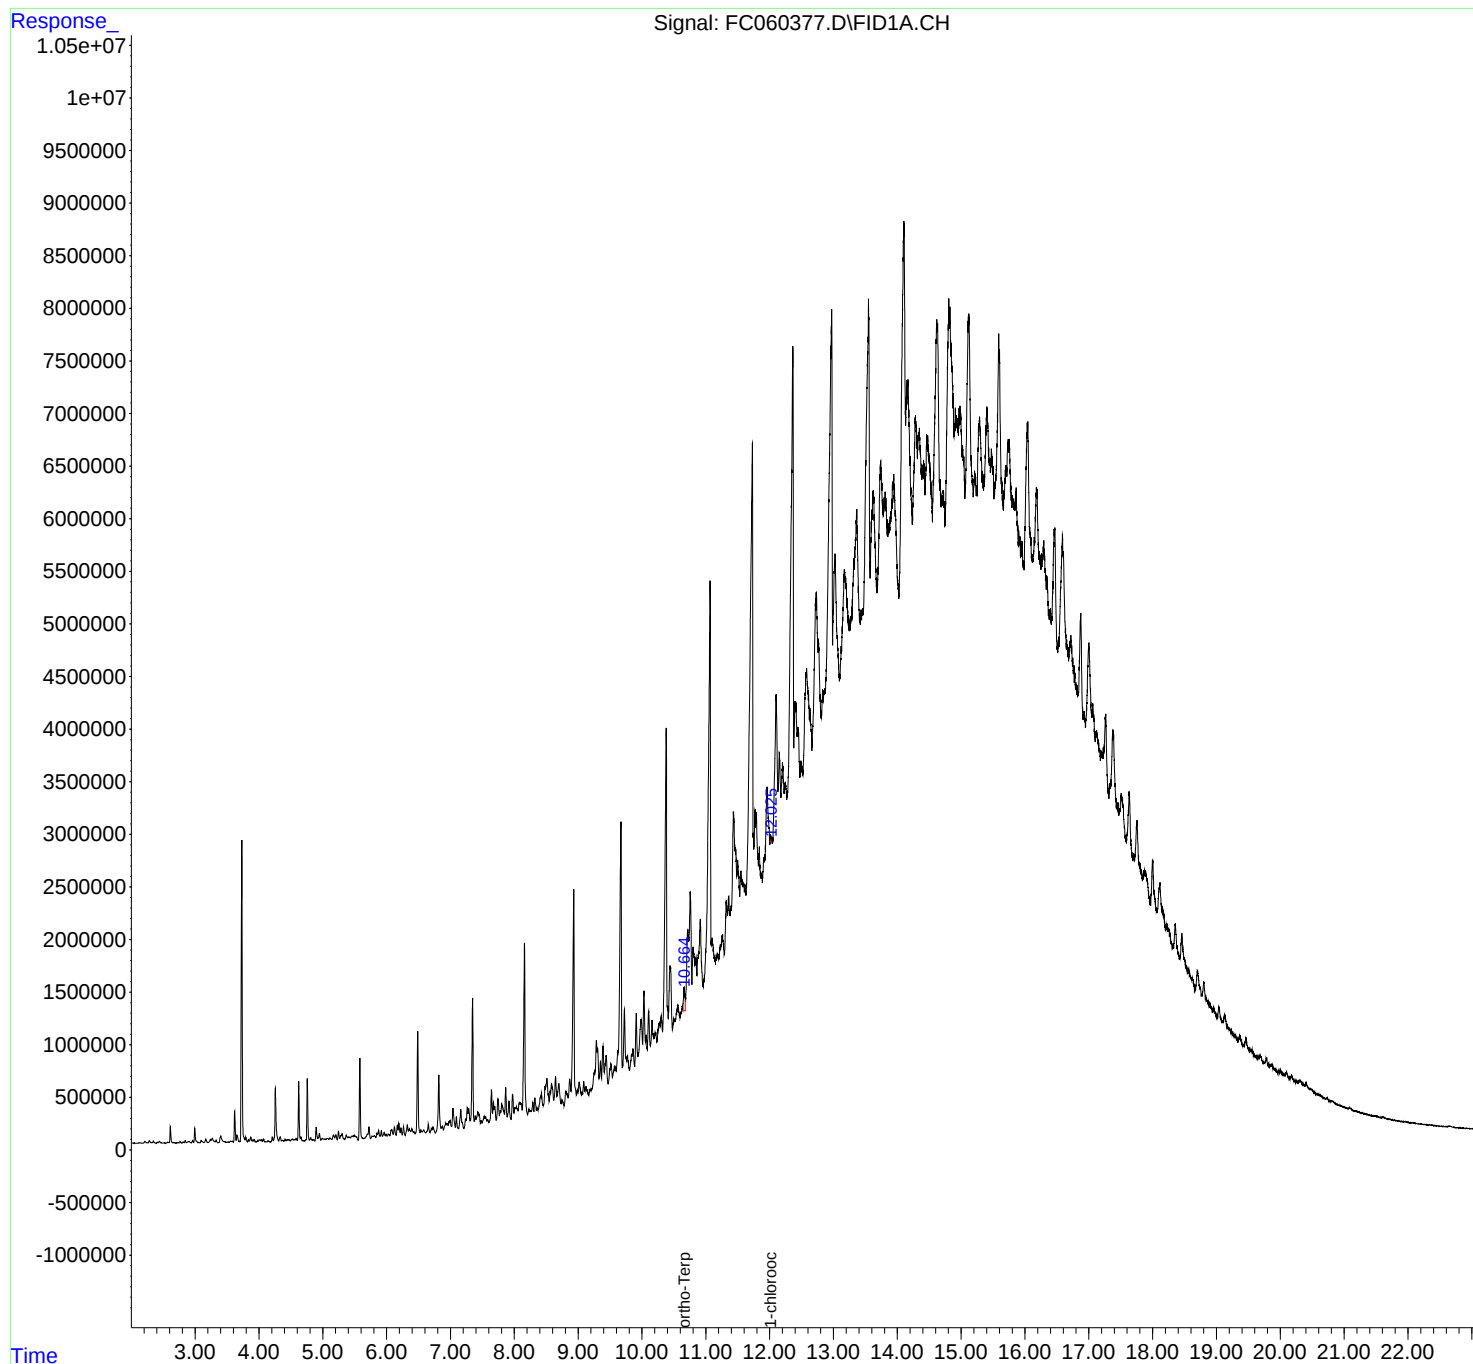

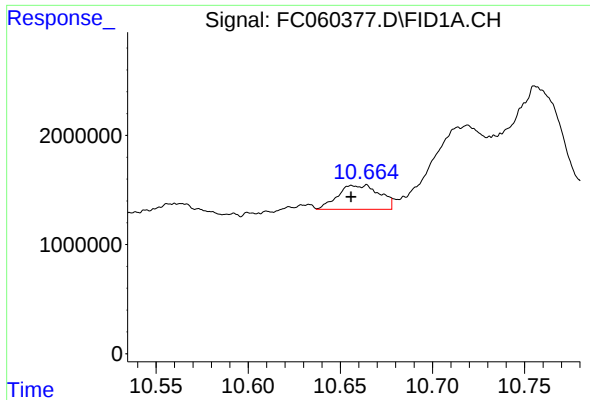


#9 ortho-Terphenyl (SURR)

R.T.: 10.664 min
Delta R.T.: 0.008 min
Response: 3521439
Conc: 22.63 ug/ml

Instrument :
FID_C
ClientSampleId :
14A-TP-7-(14.5-15.0)

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/21/2022
Supervised By :Ankita Jodhani 06/22/2022

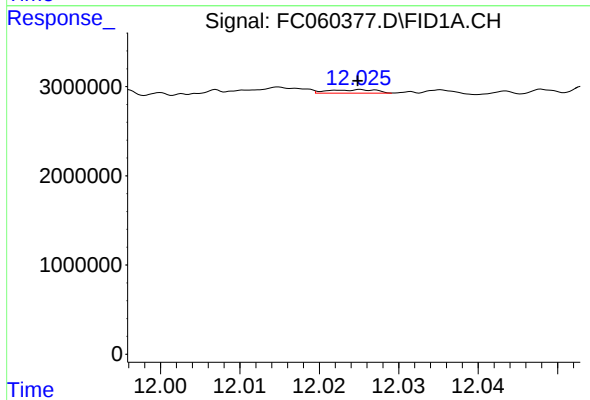

#12 1-chlorooctadecane (SURR)

R.T.: 12.025 min
Delta R.T.: 0.000 min
Response: 162959
Conc: 1.31 ug/ml m