

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062124AL\
 Data File : FC066668.D
 Signal(s) : FID1A.ch
 Acq On : 21 Jun 2024 17:47
 Operator : YP/AJ
 Sample : P2915-01D
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 22 02:58:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 17 13:44:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.970	3769734	27.321 ug/ml
Spiked Amount 50.000		Recovery =	54.64%
Target Compounds			
4) T n-Dodecane (C12)	6.378	141532	0.934 ug/ml
6) T n-Tetradecane (C14)	8.173	77343	0.510 ug/ml
14) T n-Tetracosane (C24)	14.824	59392	0.374 ug/ml
15) T n-Hexacosane (C26)	15.845	55690	0.365 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062124AL\
Data File : FC066668.D
Signal(s) : FID1A.ch
Acq On : 21 Jun 2024 17:47
Operator : YP/AJ
Sample : P2915-01D
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 22 02:58:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
Quant Title : GC Extractables
QLast Update : Mon Jun 17 13:44:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

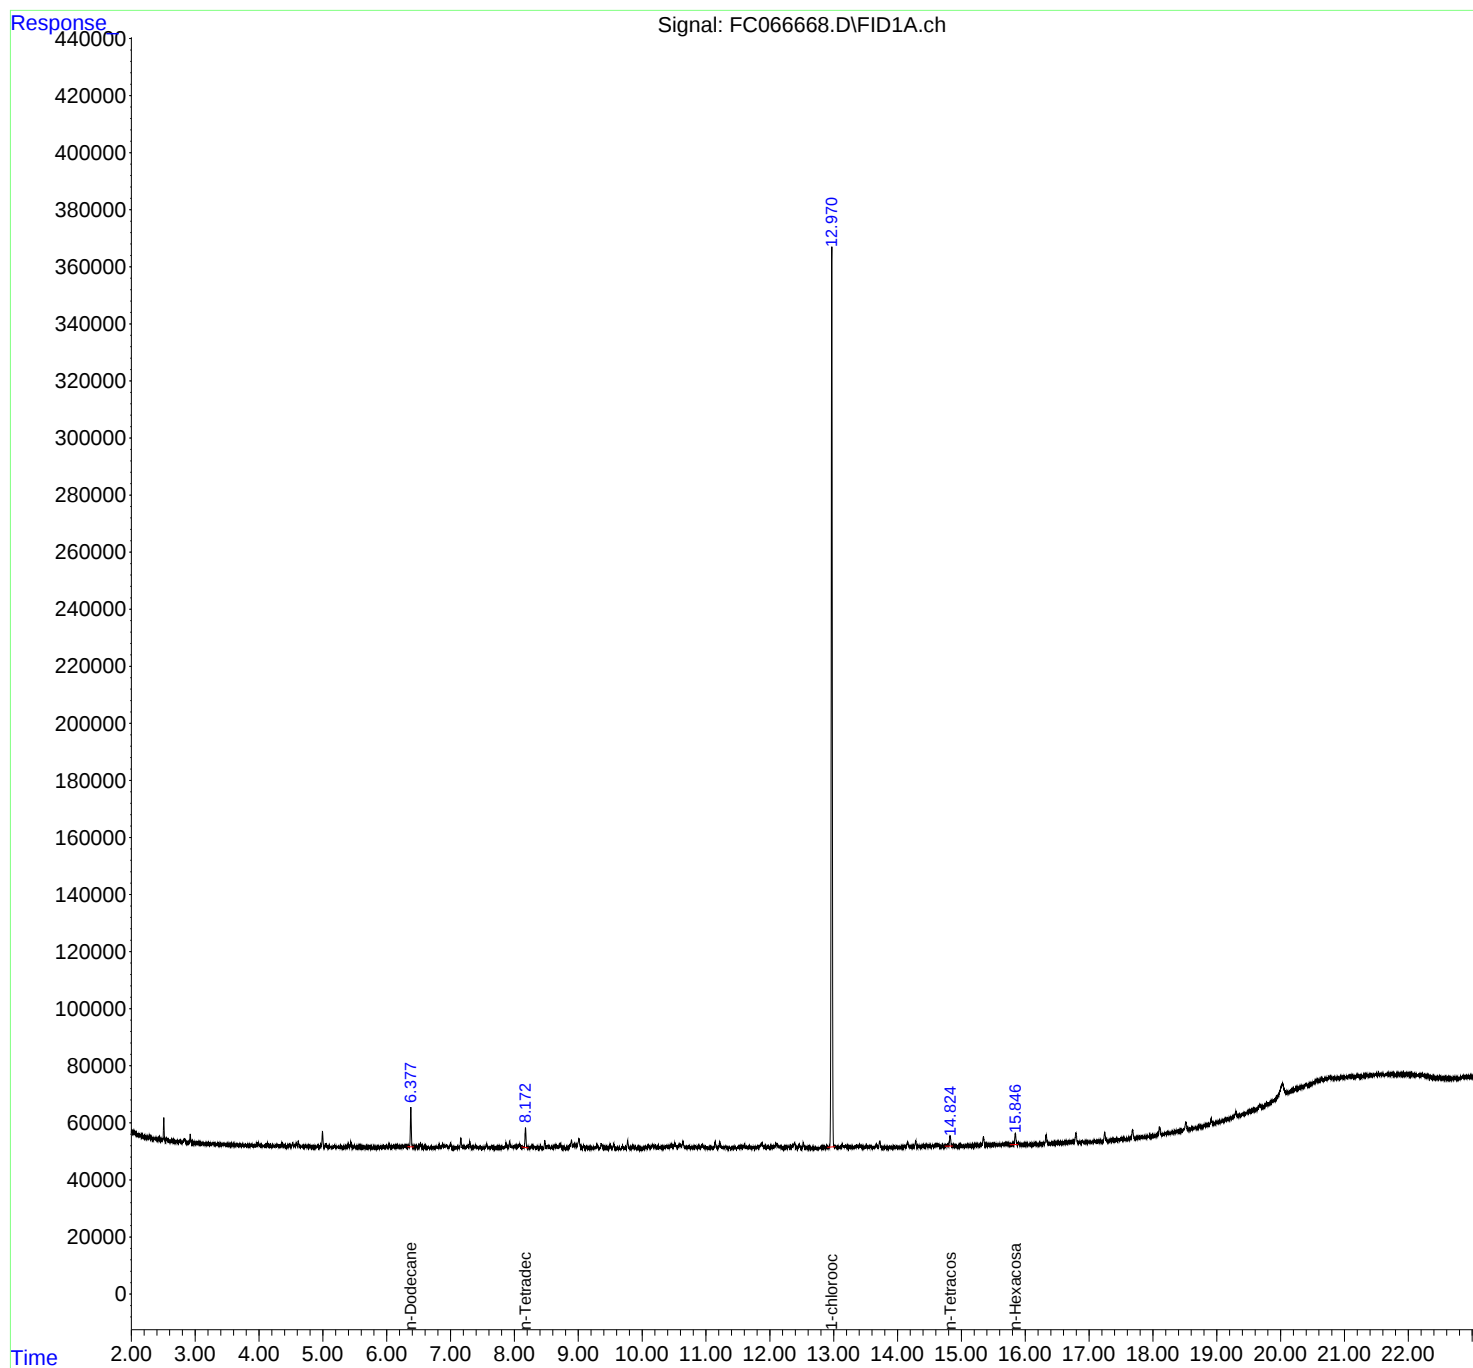


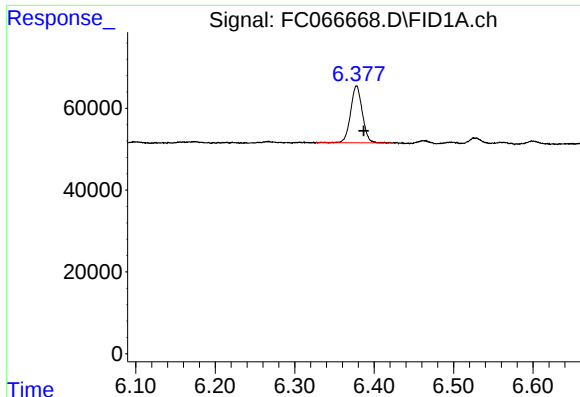

#4 n-Dodecane (C12)


R.T.: 6.378 min
Delta R.T.: -0.009 min
Response: 141532
Conc: 0.93 ug/ml

Instrument :
FID_C
ClientSampleId :

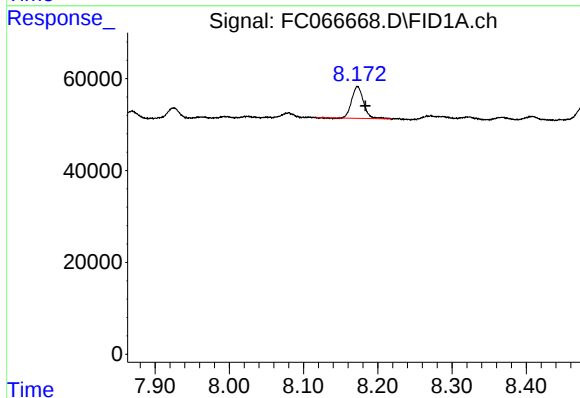


#6 n-Tetradecane (C14)

R.T.: 8.173 min
Delta R.T.: -0.011 min
Response: 77343
Conc: 0.51 ug/ml

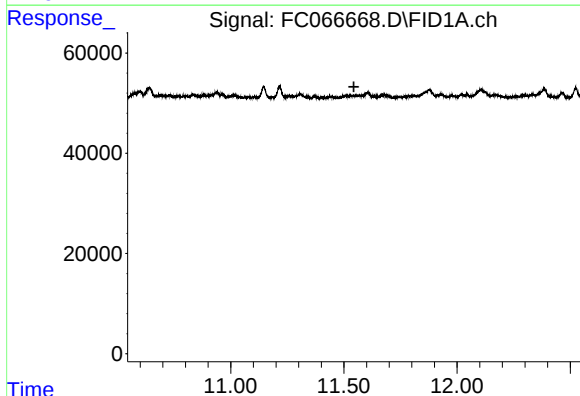


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.544 min
Response: 0
Conc: N.D.

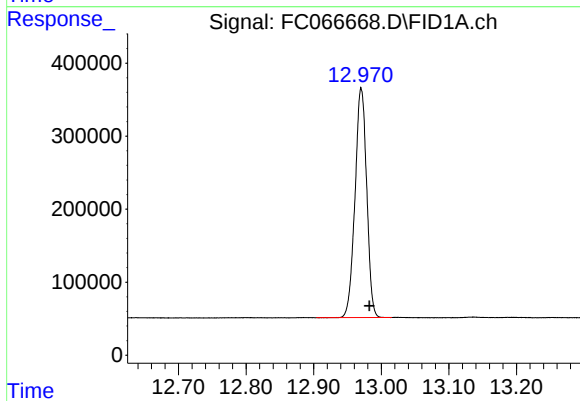

#12 1-chlorooctadecane (SURR)


R.T.: 12.970 min
Delta R.T.: -0.012 min
Response: 3769734
Conc: 27.32 ug/ml

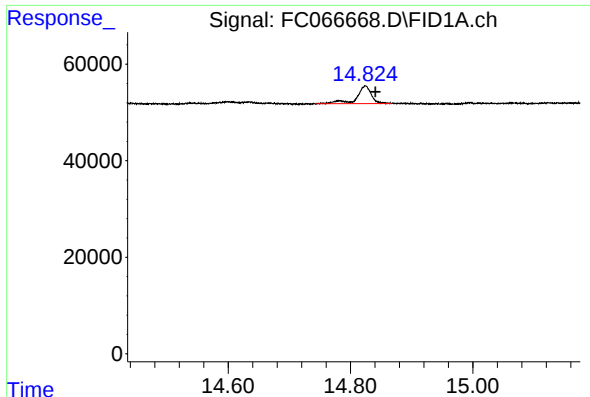

#14 n-Tetracosane (C24)

R.T.: 14.824 min
Delta R.T.: -0.016 min
Response: 59392
Conc: 0.37 ug/ml

Instrument :
FID_C
ClientSampleId :

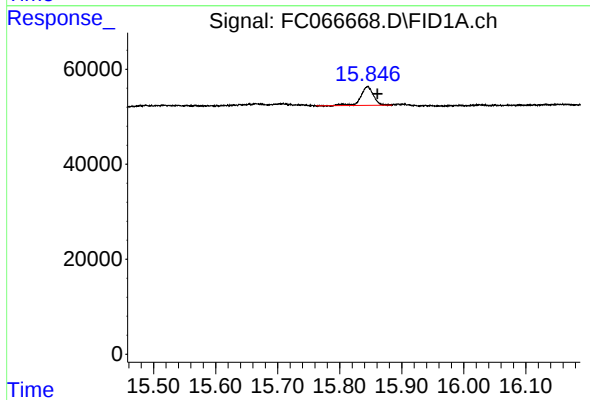

#15 n-Hexacosane (C26)

R.T.: 15.845 min
Delta R.T.: -0.016 min
Response: 55690
Conc: 0.36 ug/ml