

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062221AL\
 Data File : FC054370.D
 Signal(s) : FID1A.CH
 Acq On : 22 Jun 2021 19:45
 Operator : DD\AJ
 Sample : M2801-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 23 00:57:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 061021.M
 Quant Title : GC Extractables
 Qlast Update : Fri Jun 11 04:43:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Instrument :
 FID_C
 ClientSampleId :
 S-1

Manual Integrations
 APPROVED

Ankita
 6/23/2021 2:21:15 PM

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.349	6112558	40.251 ug/ml
Spiked Amount 50.000		Recovery =	80.50%
12) S 1-chlorooctadecane (S...	12.793	4906041	41.648 ug/mlm
Spiked Amount 50.000		Recovery =	83.30%
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062221AL\
Data File : FC054370.D
Signal(s) : FID1A.CH
Acq On : 22 Jun 2021 19:45
Operator : DD\AJ
Sample : M2801-01
Misc :
ALS Vial : 7 Sample Multiplier: 1


Integration File: autoint1.e
Quant Time: Jun 23 00:57:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 04:43:57 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Instrument :
FID_C
ClientSampleId :
S-1

Manual Integrations
APPROVED

Ankita
6/23/2021 2:21:15 PM


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

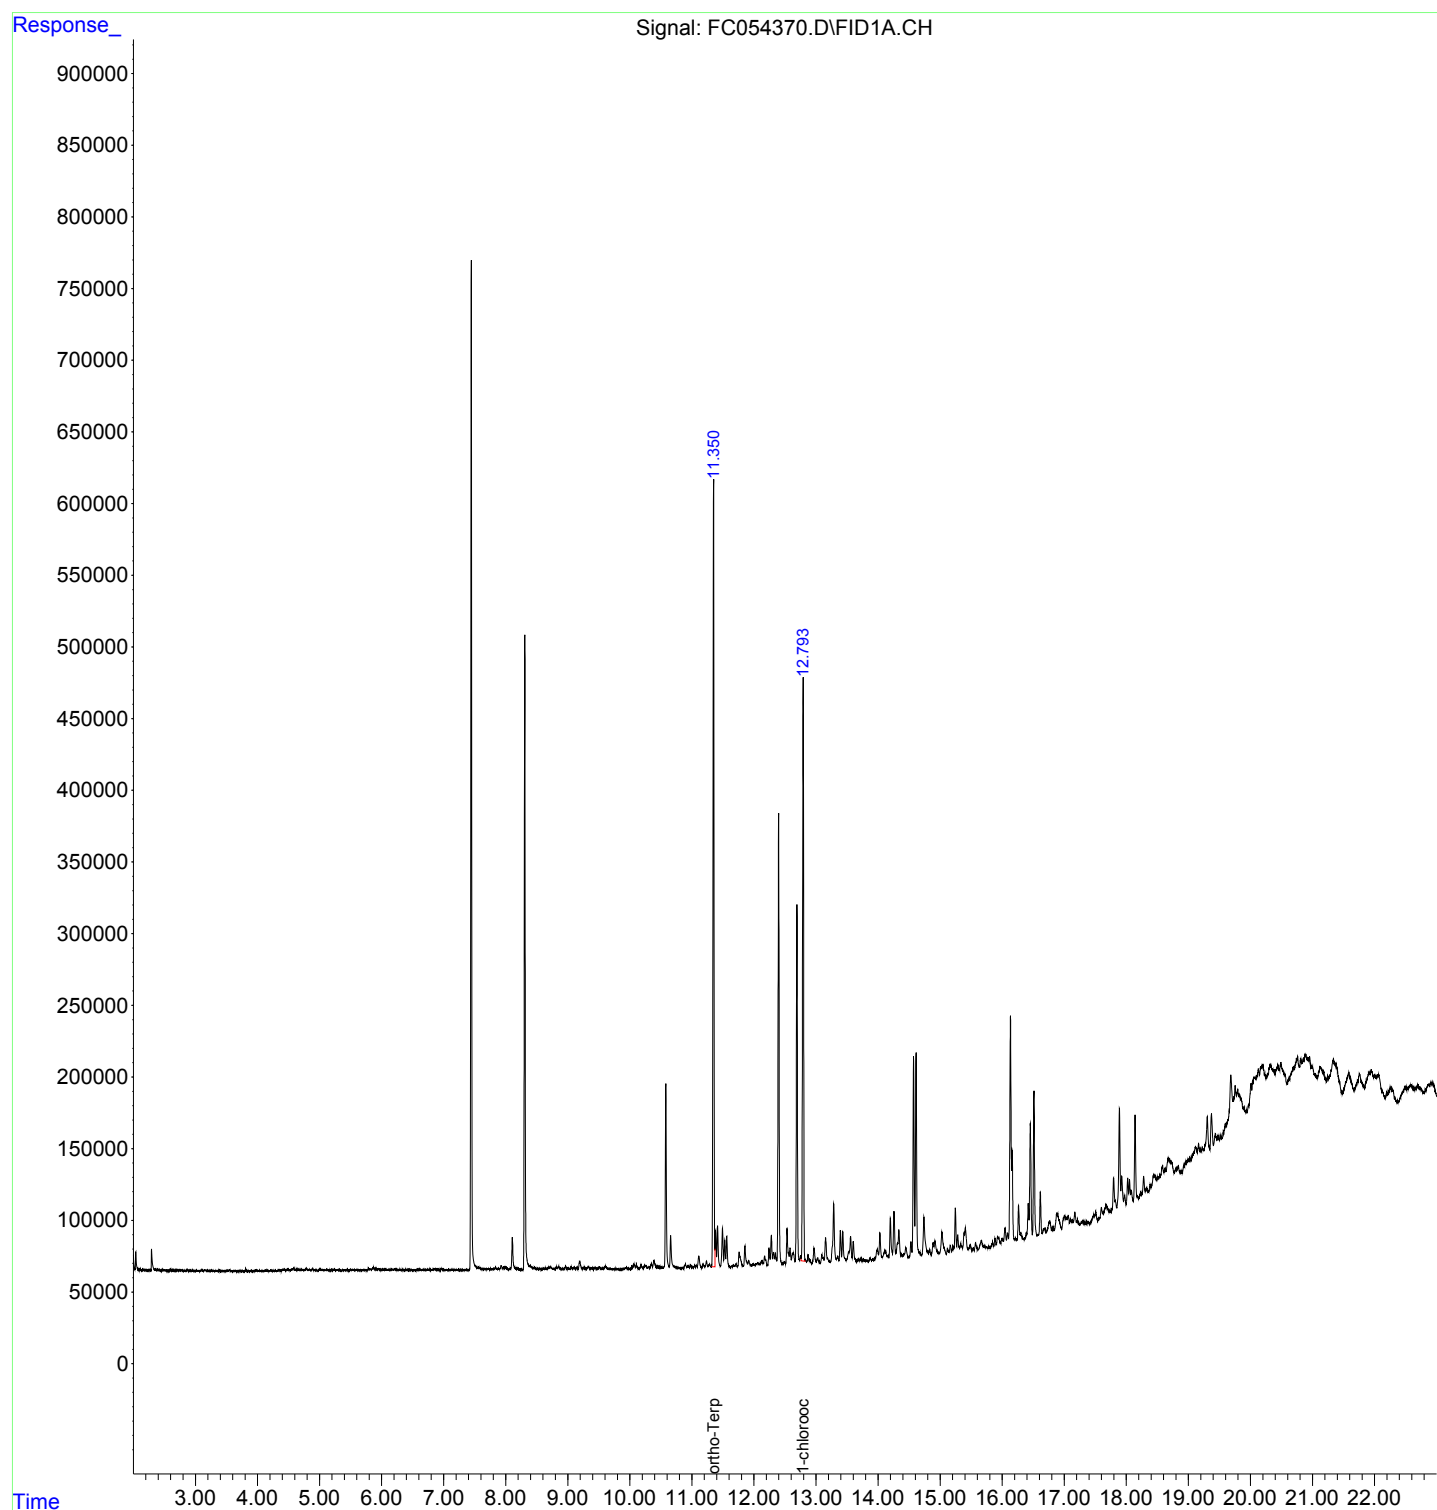

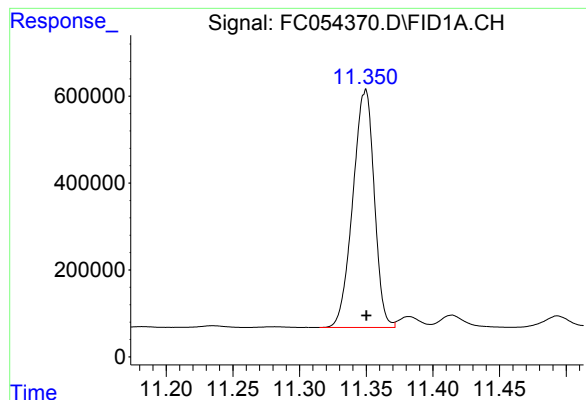

#9 ortho-Terphenyl (SURR)

R.T.: 11.349 min
Delta R.T.: -0.001 min
Response: 6112558
Conc: 40.25 ug/ml

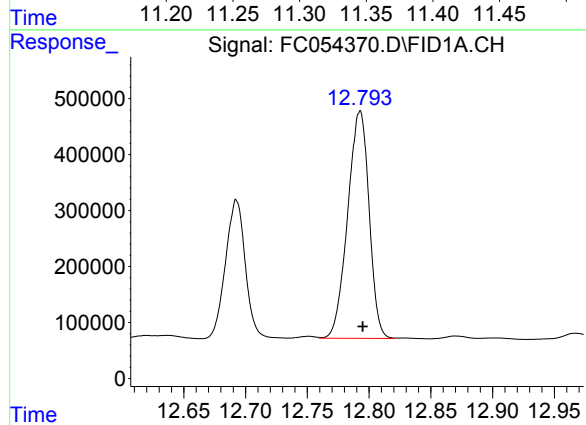

#12 1-chlorooctadecane (SURR)

R.T.: 12.793 min
Delta R.T.: -0.002 min
Response: 4906041
Conc: 41.65 ug/ml m

Instrument :
FID_C
ClientSampleId :
S-1

Manual Integrations
APPROVED

Ankita
6/23/2021 2:21:15 PM