

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062222\
 Data File : PS019766.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2022 00:04
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 01:06:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.195	6.780	1074.1E6	407.8E6	447.716	526.240
Target Compounds							
1) T	Dalapon	3.018	0.000	758727	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.440	0.000	84709	0	<MDL	N.D. #
5) T	DICAMBA	0.000	6.945	0	1448090	N.D.	<MDL
6) T	MCP	0.000	6.968f	0	2104972	N.D.	<MDL
7) T	MCPA	7.676	0.000	8022405	0	<MDL	N.D. #
8) T	DICHLORPROP	8.085	7.611f	442734	3197076	<MDL	3.619 #
9) T	2,4-D	0.000	7.819f	0	1952824	N.D.	1.831
10) T	Pentachlo...	8.613	8.281	543483	2579181	<MDL	<MDL #
11) T	2,4,5-TP ...	9.185	8.641	5266452	254698	<MDL	<MDL #
13) T	2,4-DB	10.016	0.000	2222096	0	<MDL	N.D. #
15) T	Picloram	11.009	10.863	9560144	3558225	<MDL	<MDL #
16) T	DCPA	11.444	10.776	801023	3705705	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062222\
Data File : PS019766.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2022 00:04
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 01:06:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

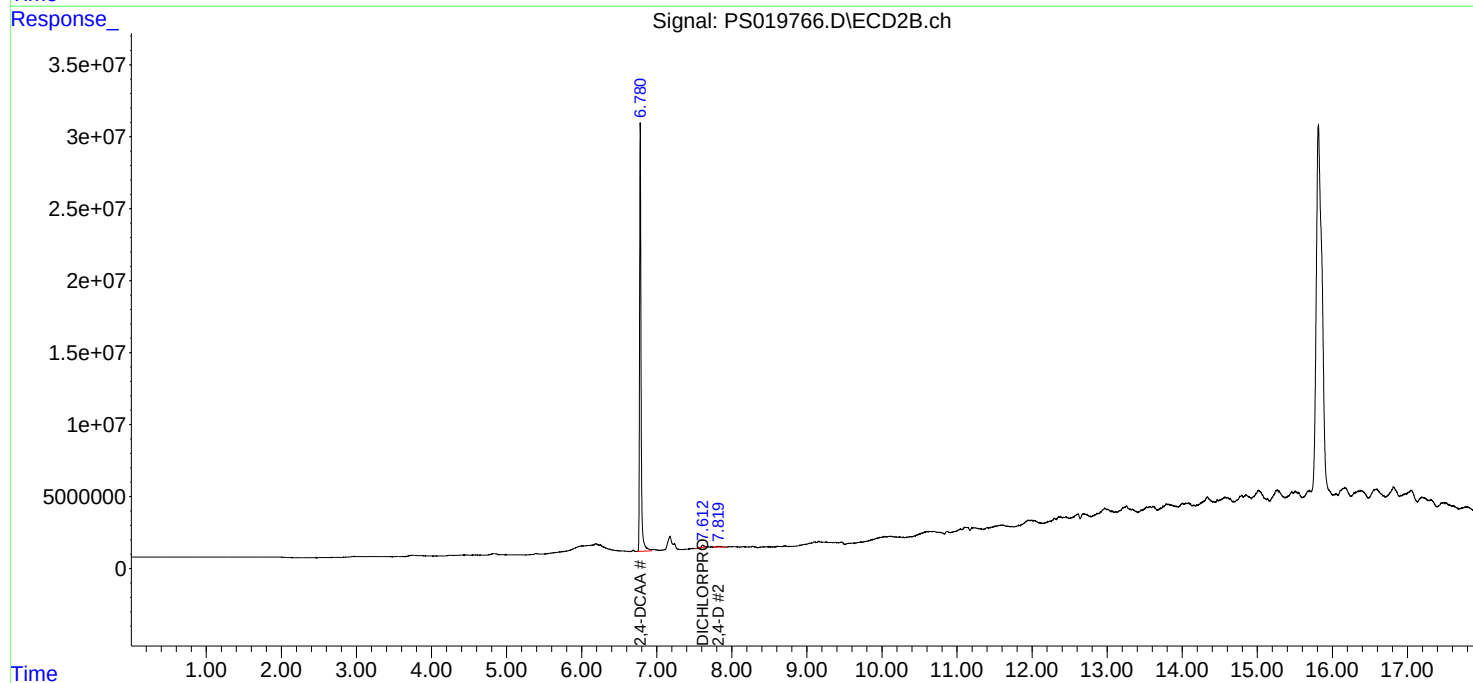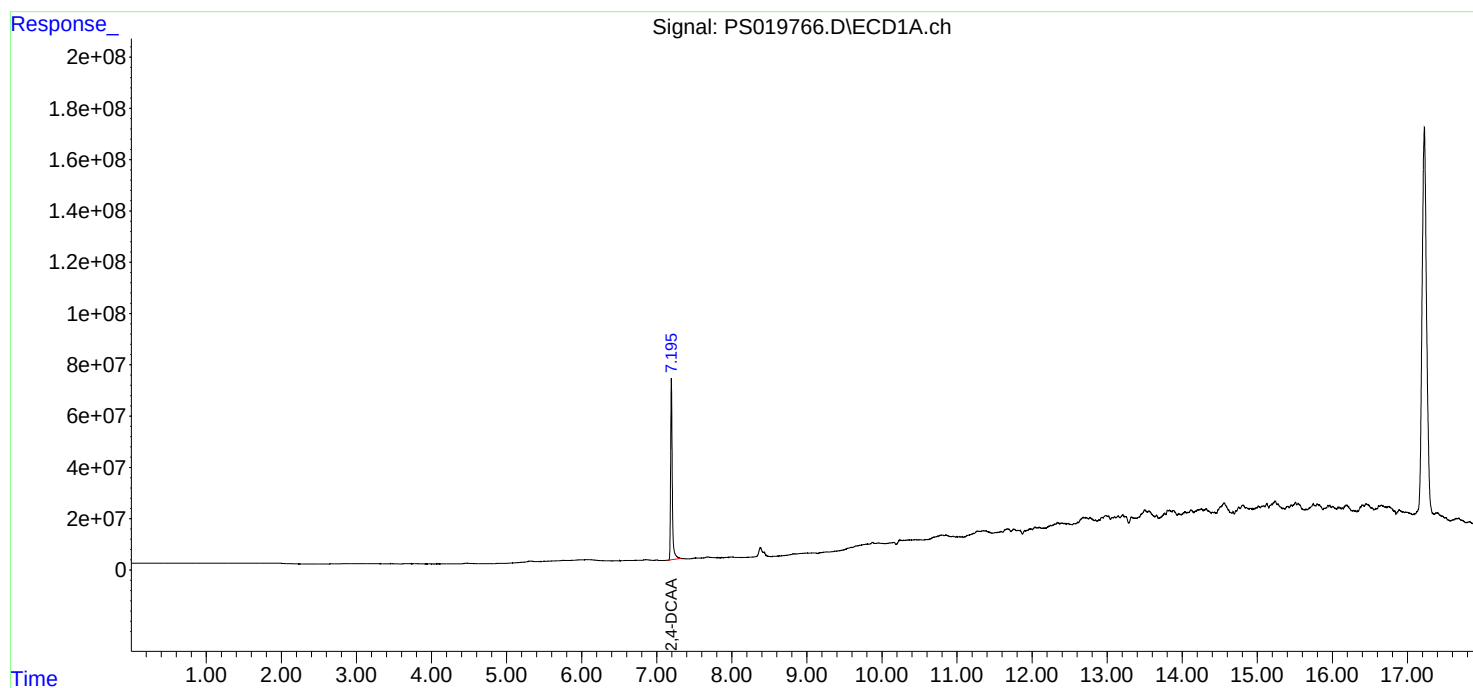

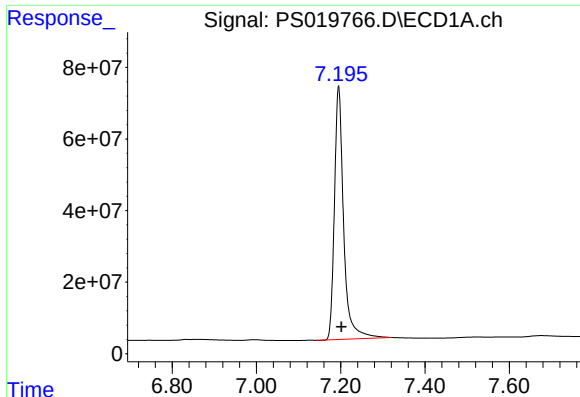


#4 2,4-DCAA

R.T.: 7.195 min
Delta R.T.: -0.007 min
Response: 1074145027
Conc: 447.72 ng/ml

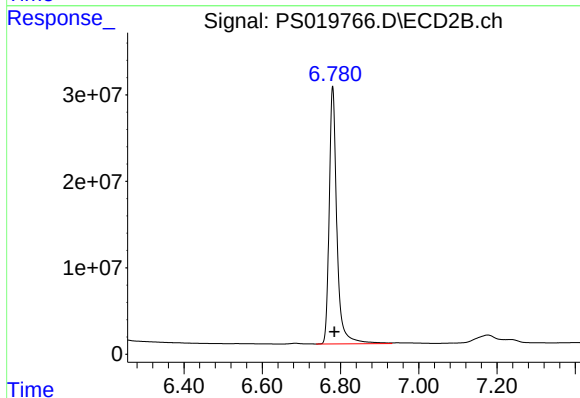


#4 2,4-DCAA

R.T.: 6.780 min
Delta R.T.: -0.005 min
Response: 407767466
Conc: 526.24 ng/ml

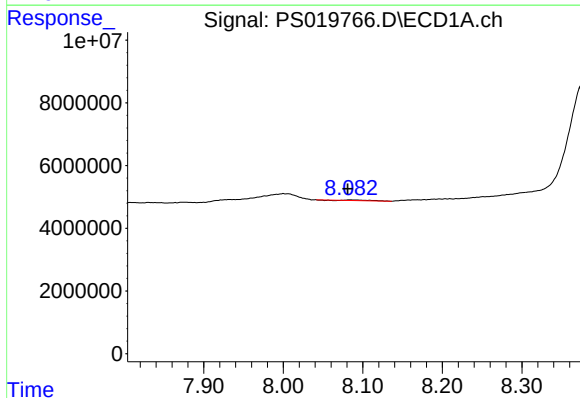


#8 DICHLORPROP

R.T.: 8.085 min
Delta R.T.: 0.004 min
Response: 442734
Conc: N.D.

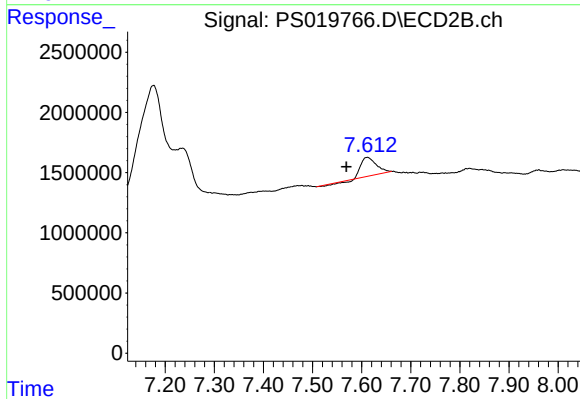


#8 DICHLORPROP

R.T.: 7.611 min
Delta R.T.: 0.042 min
Response: 3197076
Conc: 3.62 ng/ml

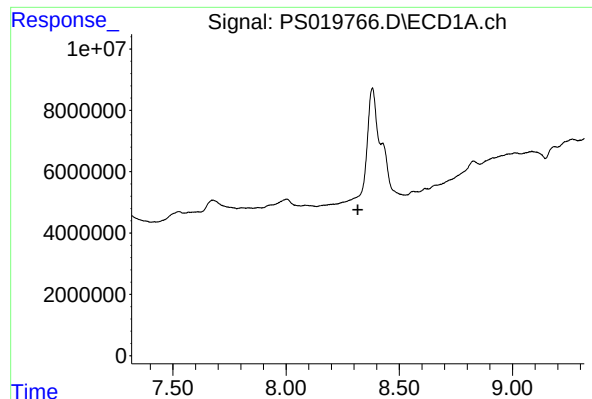

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.317 min
Response: 0
Conc: N.D.

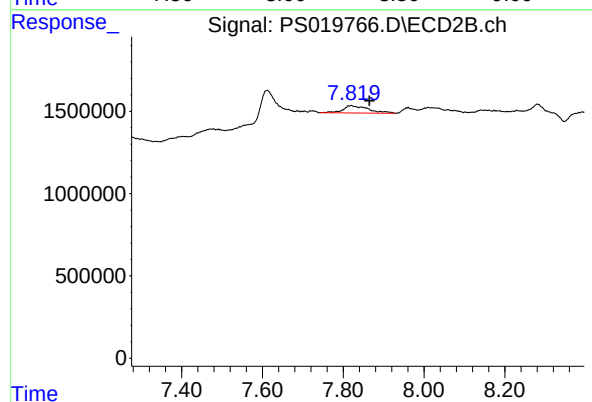

#9 2,4-D

R.T.: 7.819 min
Delta R.T.: -0.045 min
Response: 1952824
Conc: 1.83 ng/ml