

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062323AL\
Data File : FC063955.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2023 07:09
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 23 13:14:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052723.M
Quant Title : GC Extractables
QLast Update : Sat May 27 06:12:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
11) T	n-Heneicosane (C21)	13.125	62141	0.432 ug/ml
13) T	n-Docosane (C22)	13.710	112446	0.798 ug/ml
14) T	n-Tetracosane (C24)	14.784	79694	0.581 ug/ml
18) T	n-Dotriacontane (C32)	18.486	230729	1.854 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062323AL\
Data File : FC063955.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2023 07:09
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 23 13:14:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052723.M
Quant Title : GC Extractables
QLast Update : Sat May 27 06:12:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

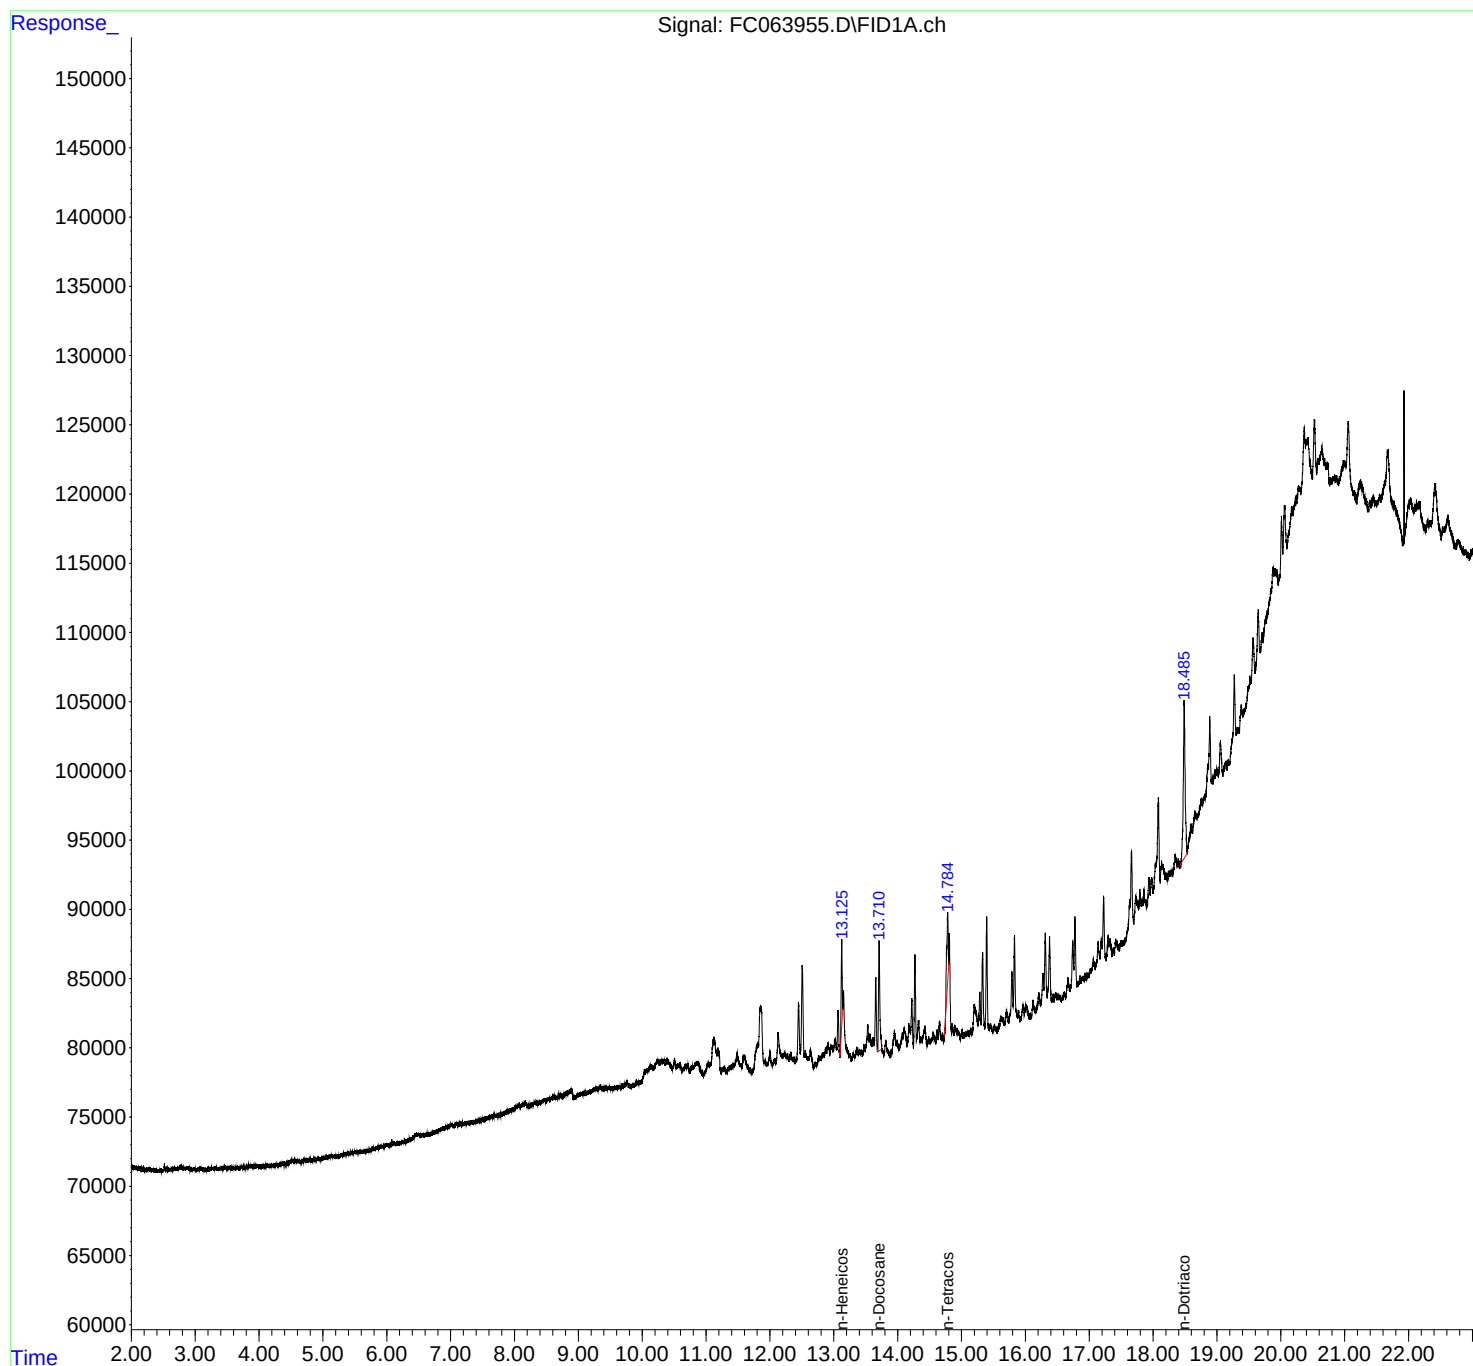


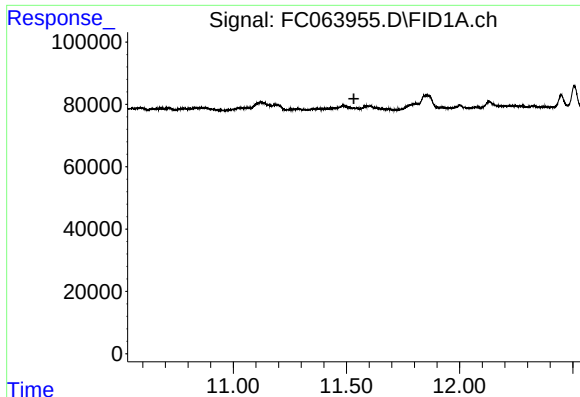

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.533 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

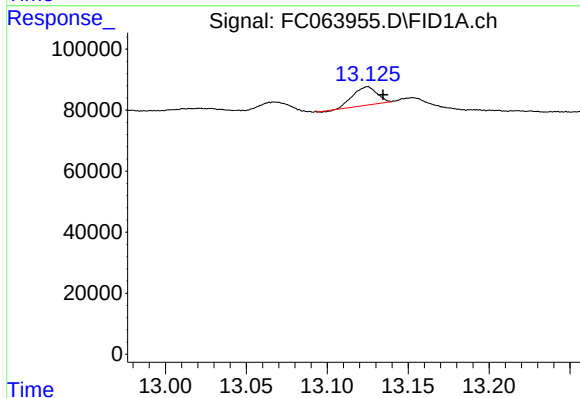


#11 n-Heneicosane (C21)

R.T.: 13.125 min
Delta R.T.: -0.010 min
Response: 62141
Conc: 0.43 ug/ml

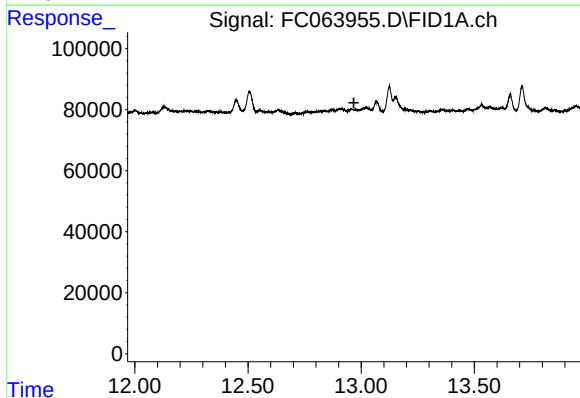


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.968 min
Response: 0
Conc: N.D.

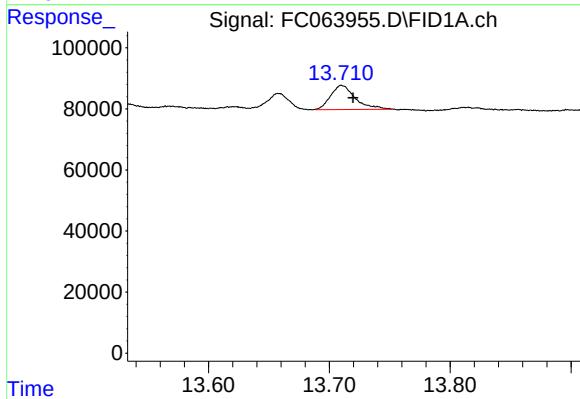

#13 n-Docosane (C22)


R.T.: 13.710 min
Delta R.T.: -0.009 min
Response: 112446
Conc: 0.80 ug/ml

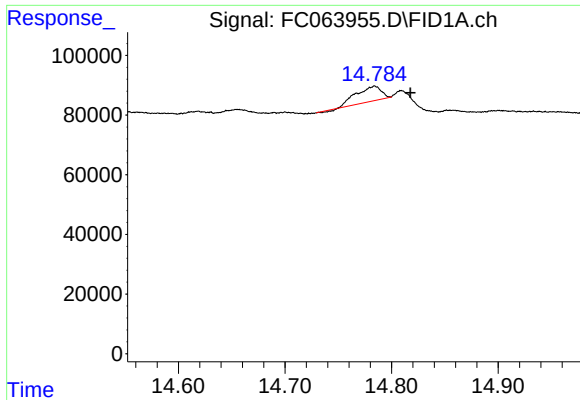

#14 n-Tetracosane (C24)

R.T.: 14.784 min
Delta R.T.: -0.033 min
Response: 79694
Conc: 0.58 ug/ml

Instrument :
FID_C
ClientSampleId :

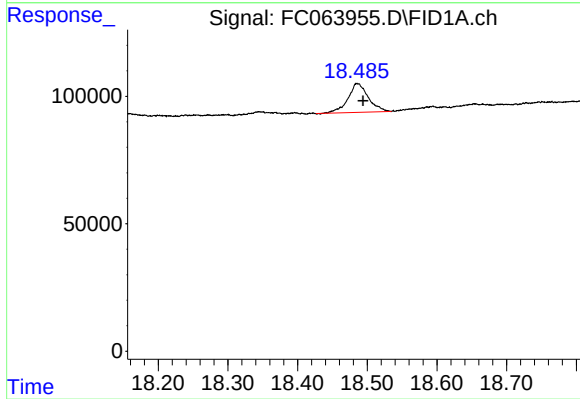

#18 n-Dotriacontane (C32)

R.T.: 18.486 min
Delta R.T.: -0.008 min
Response: 230729
Conc: 1.85 ug/ml