

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062323AL\
 Data File : FC063961.D
 Signal(s) : FID1A.ch
 Acq On : 23 Jun 2023 13:53
 Operator : YP/AJ
 Sample : 03329-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 23 14:57:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052723.M
 Quant Title : GC Extractables
 QLast Update : Sat May 27 06:12:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.962	5104680	39.951 ug/ml
Spiked Amount 50.000		Recovery =	79.90%
Target Compounds			
4) T n-Dodecane (C12)	6.383	203500	1.245 ug/ml
6) T n-Tetradecane (C14)	8.175	93117	0.592 ug/ml
15) T n-Hexacosane (C26)	15.830	93660	0.706 ug/ml
16) T n-Octacosane (C28)	16.779	141564	1.115 ug/ml
17) T n-Tricontane (C30)	17.659	159422	1.248 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062323AL\
Data File : FC063961.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2023 13:53
Operator : YP/AJ
Sample : 03329-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 23 14:57:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 052723.M
Quant Title : GC Extractables
QLast Update : Sat May 27 06:12:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

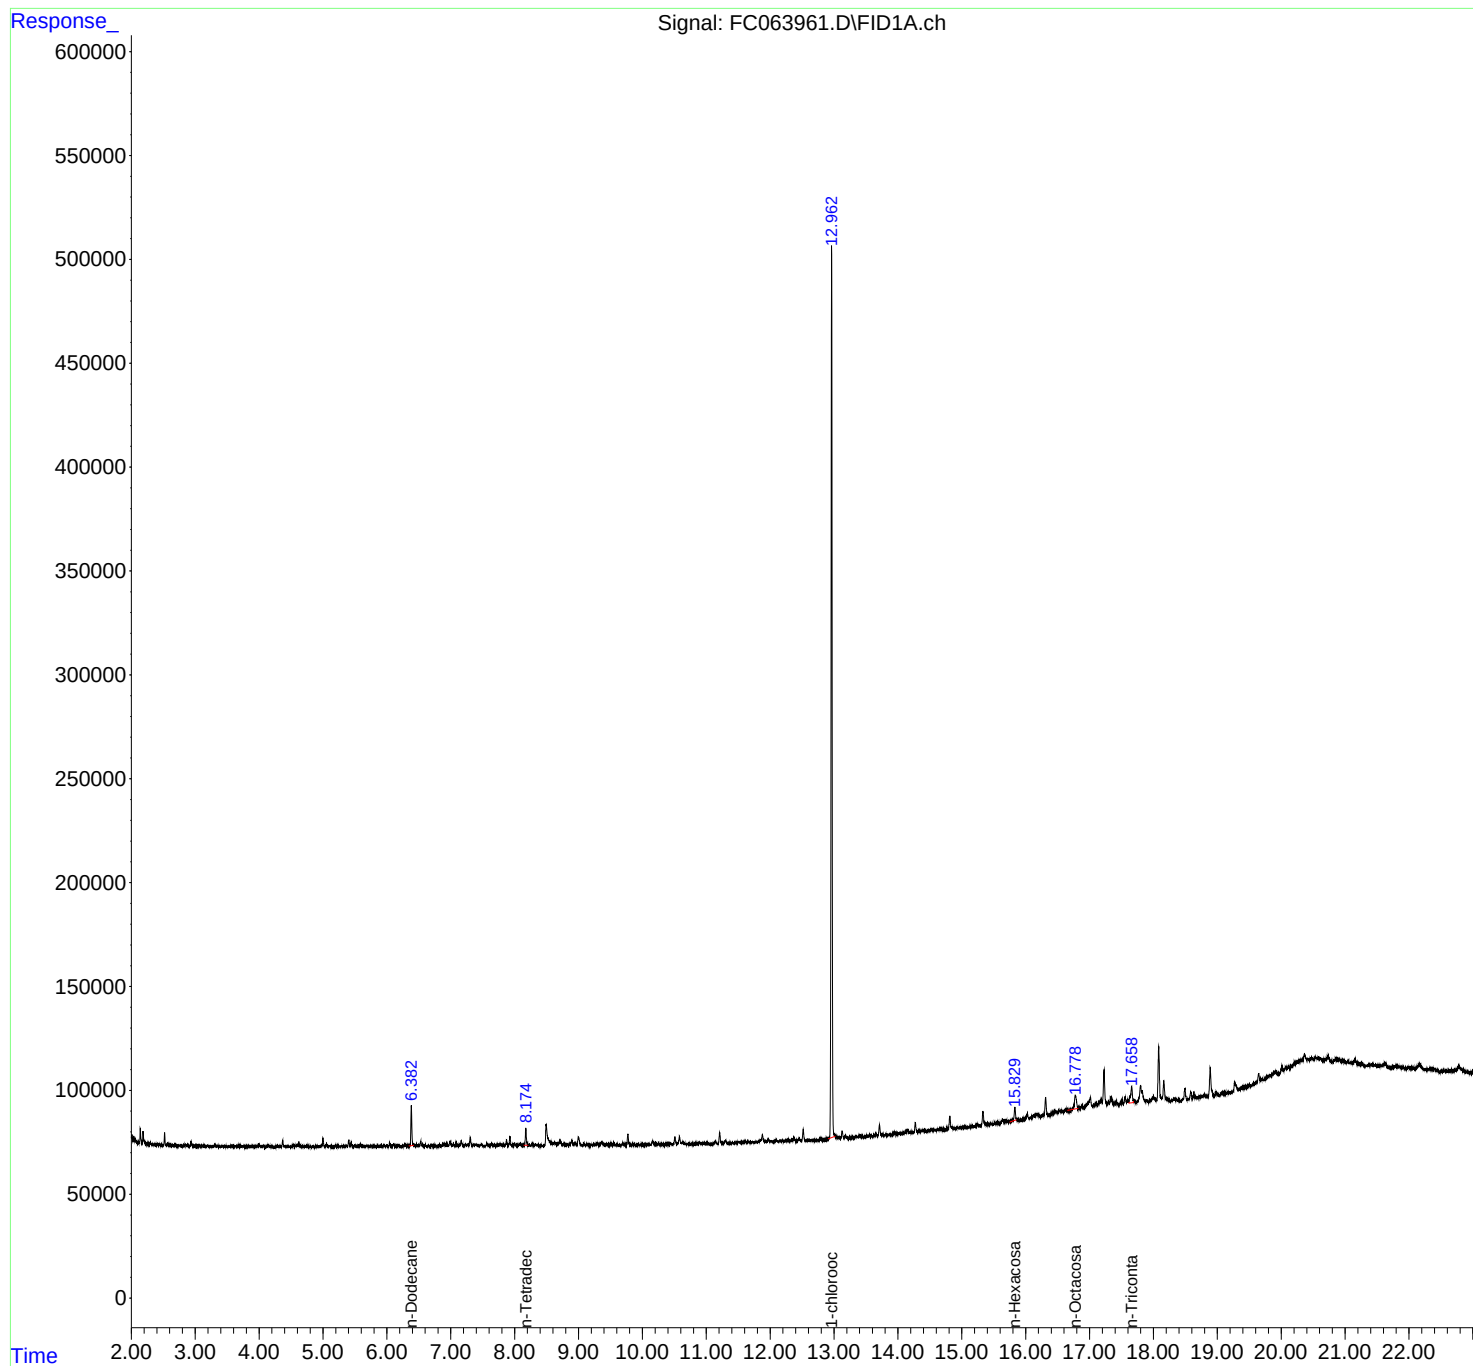


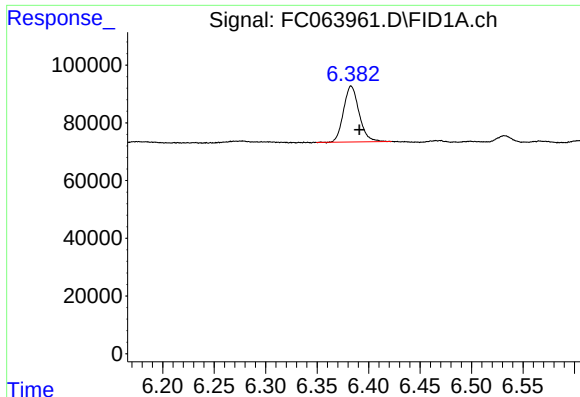

#4 n-Dodecane (C12)


R.T.: 6.383 min
Delta R.T.: -0.008 min
Response: 203500
Conc: 1.24 ug/ml

Instrument :
FID_C
ClientSampleId :

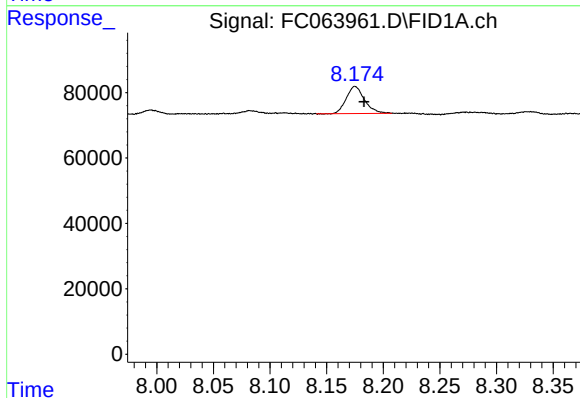


#6 n-Tetradecane (C14)

R.T.: 8.175 min
Delta R.T.: -0.008 min
Response: 93117
Conc: 0.59 ug/ml

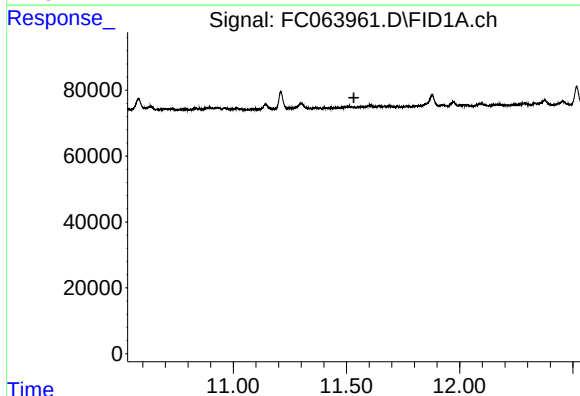


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.533 min
Response: 0
Conc: N.D.

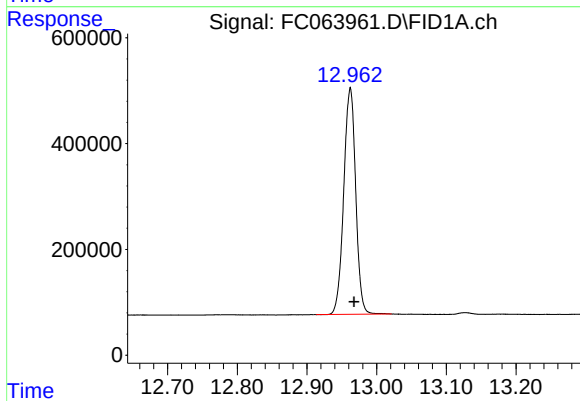

#12 1-chlorooctadecane (SURR)


R.T.: 12.962 min
Delta R.T.: -0.005 min
Response: 5104680
Conc: 39.95 ug/ml

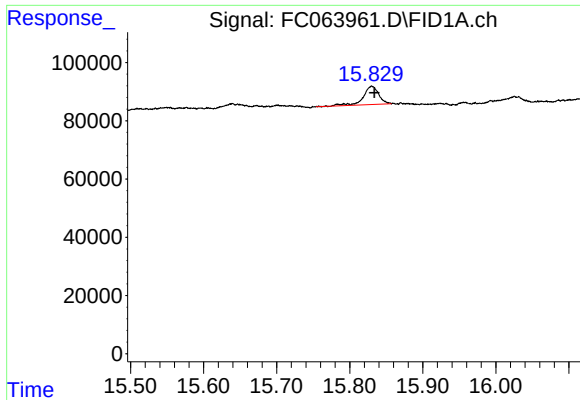

#15 n-Hexacosane (C26)


R.T.: 15.830 min
Delta R.T.: -0.004 min
Response: 93660
Conc: 0.71 ug/ml

Instrument :
FID_C
ClientSampleId :

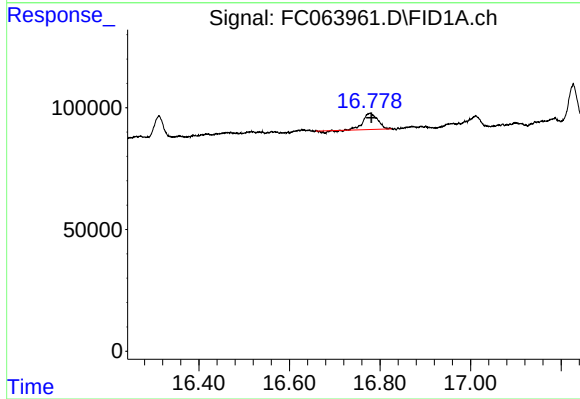

#16 n-Octacosane (C28)

R.T.: 16.779 min
Delta R.T.: -0.002 min
Response: 141564
Conc: 1.11 ug/ml

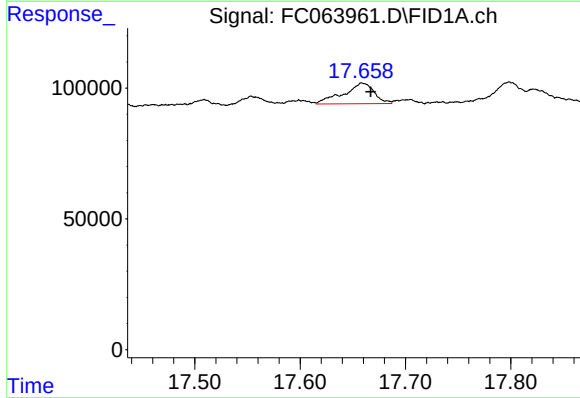

#17 n-Tricontane (C30)

R.T.: 17.659 min
Delta R.T.: -0.008 min
Response: 159422
Conc: 1.25 ug/ml