

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062325AL\
 Data File : FC069242.D
 Signal(s) : FID1A.ch
 Acq On : 23 Jun 2025 09:54
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 MECL2

Integration File: autoint1.e
 Quant Time: Jun 24 01:25:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061825.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 18 14:24:27 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.835	49804	0.419 ug/ml
18) T	n-Dotriacontane (C32)	18.669	63192	0.578 ug/ml
19) T	n-Tetratriacontane (C34)	19.454	43925	0.455 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062325AL\
Data File : FC069242.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2025 09:54
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Jun 24 01:25:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061825.M
Quant Title : GC Extractables
QLast Update : Wed Jun 18 14:24:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

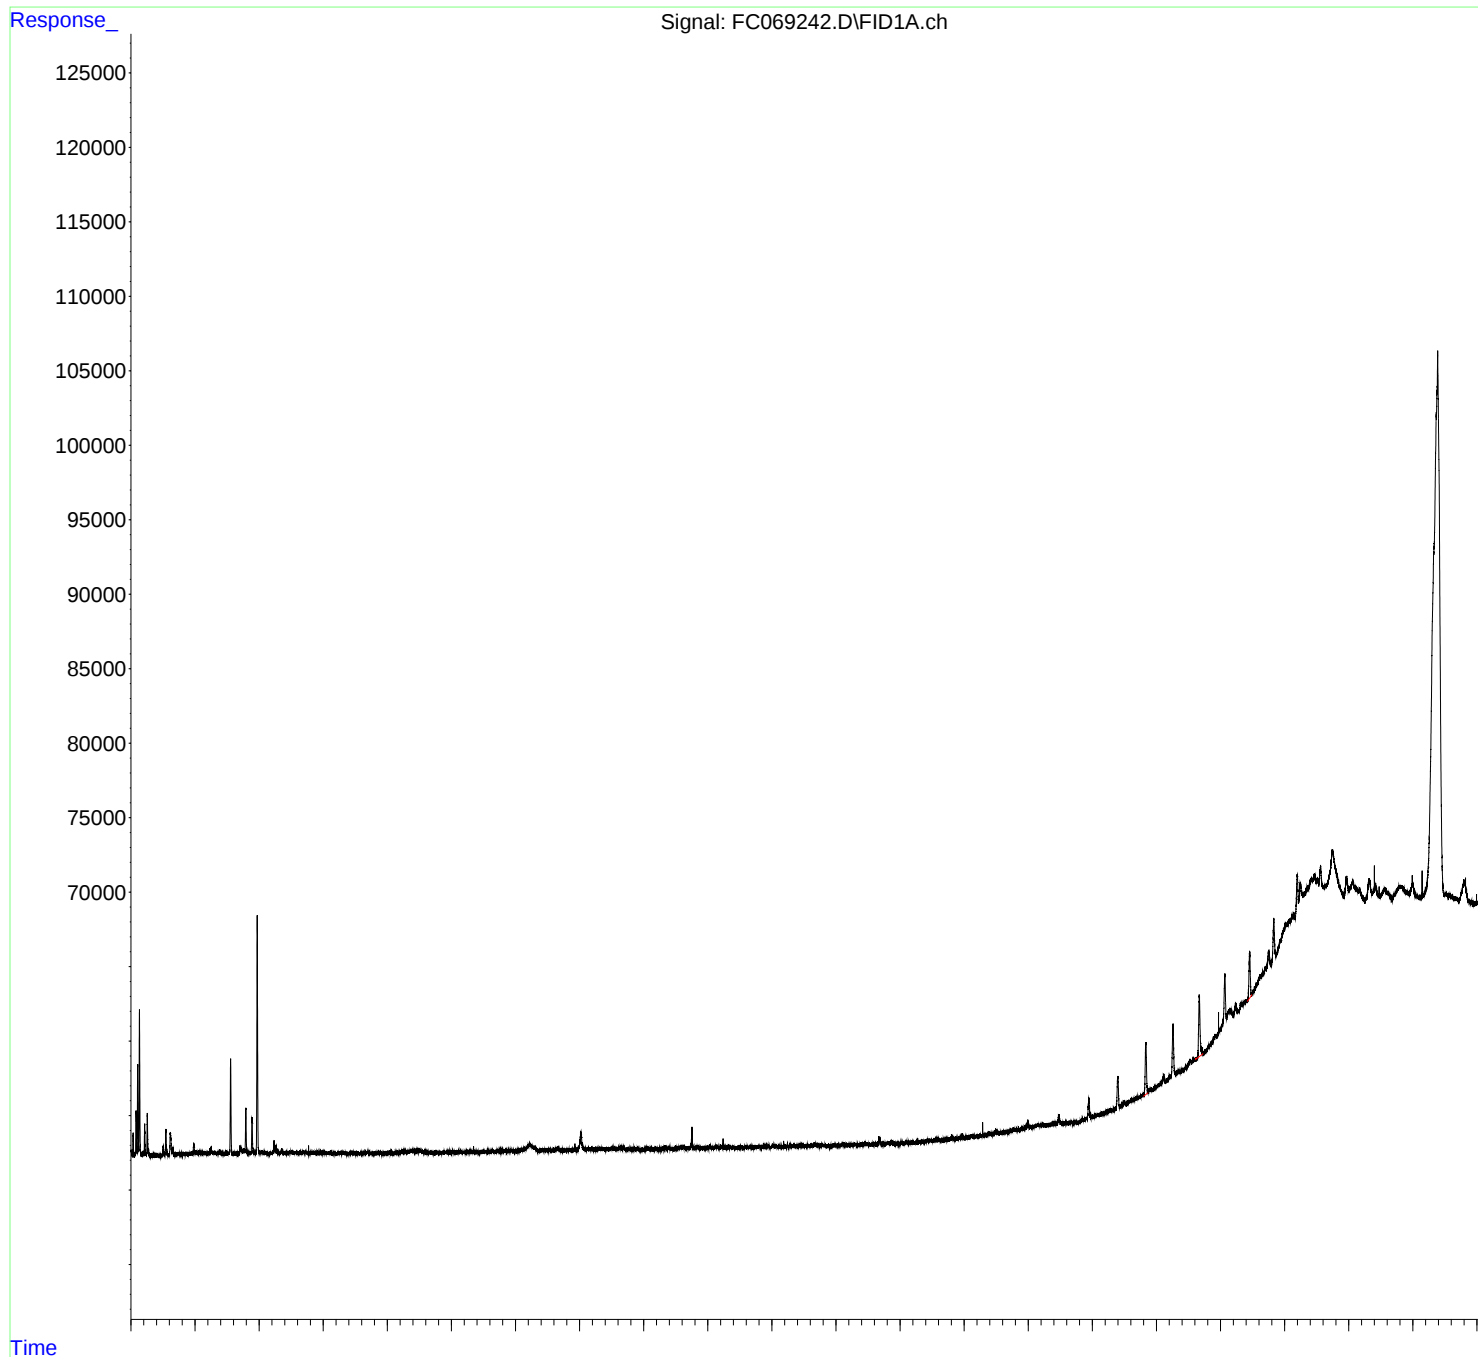


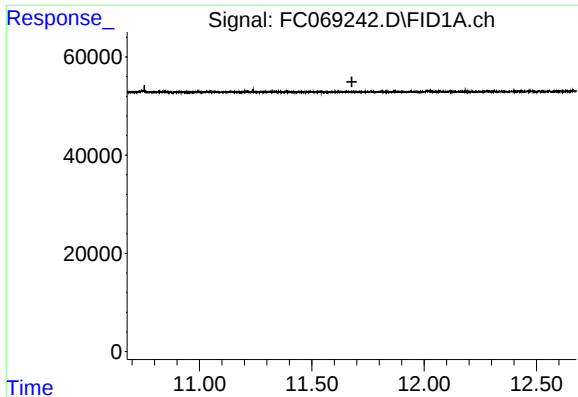

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.678 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
MECL2

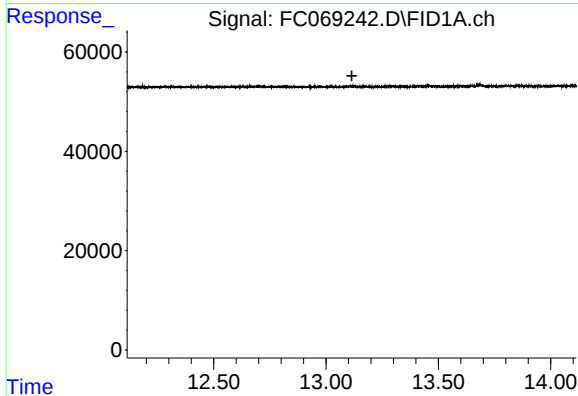


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.114 min
Response: 0
Conc: N.D.

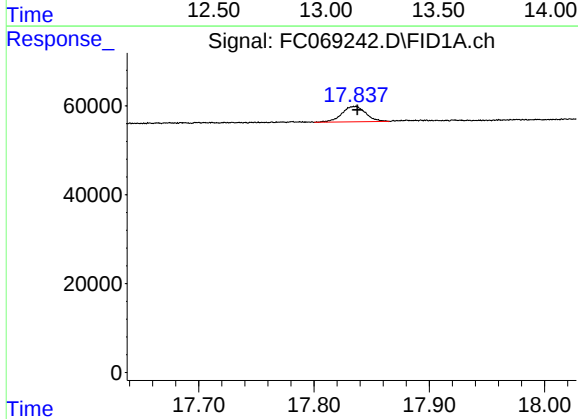


#17 n-Tricontane (C30)

R.T.: 17.835 min
Delta R.T.: -0.003 min
Response: 49804
Conc: 0.42 ug/ml

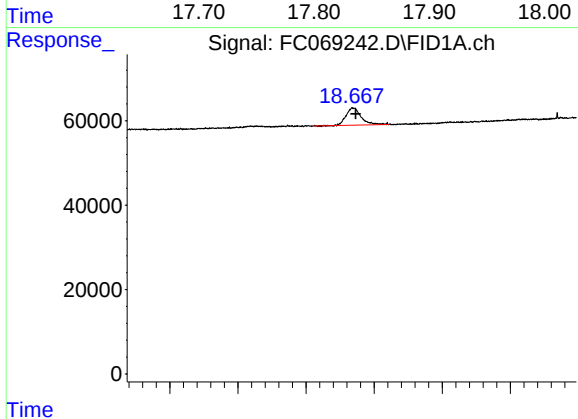

#18 n-Dotriacontane (C32)

R.T.: 18.669 min
Delta R.T.: -0.004 min
Response: 63192
Conc: 0.58 ug/ml

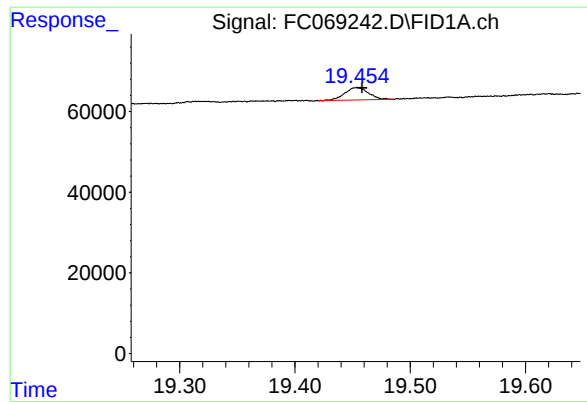

#19 n-Tetratriacontane (C34)

R.T.: 19.454 min
Delta R.T.: -0.004 min
Response: 43925
Conc: 0.45 ug/ml

Instrument :
FID_C
ClientSampleId :
MECL2