

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062623AL\
 Data File : FC063987.D
 Signal(s) : FID1A.ch
 Acq On : 26 Jun 2023 07:46
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 27 03:54:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 062423.M
 Quant Title : GC Extractables
 QLast Update : Sun Jun 25 04:03:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) T n-Heneicosane (C21)	13.121	70501	0.440 ug/ml
13) T n-Docosane (C22)	13.708	99245	0.632 ug/ml
14) T n-Tetracosane (C24)	14.782	115761	0.734 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062623AL\
Data File : FC063987.D
Signal(s) : FID1A.ch
Acq On : 26 Jun 2023 07:46
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 27 03:54:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 062423.M
Quant Title : GC Extractables
QLast Update : Sun Jun 25 04:03:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

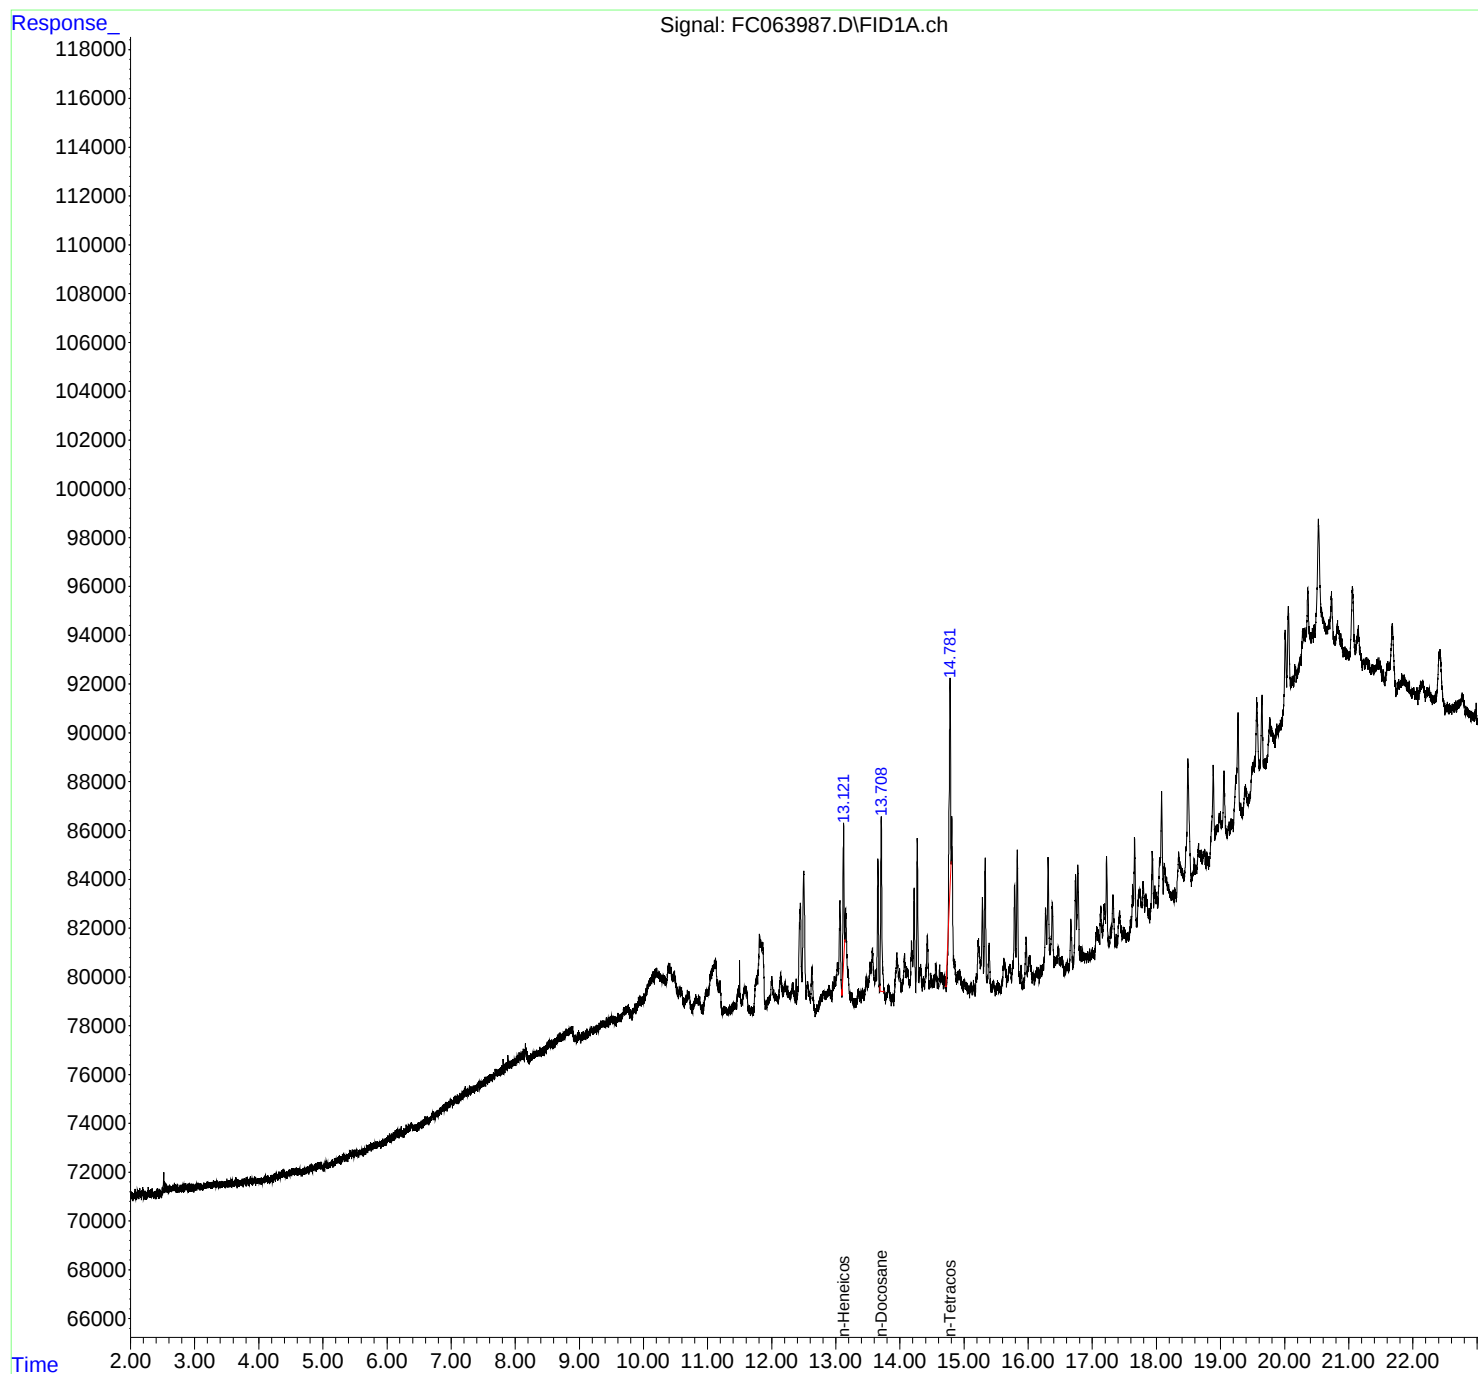


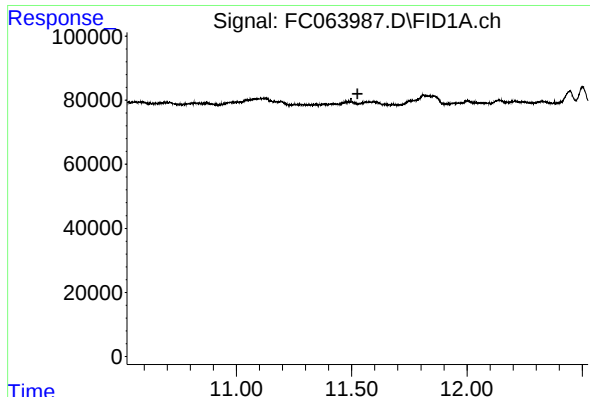

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.525 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

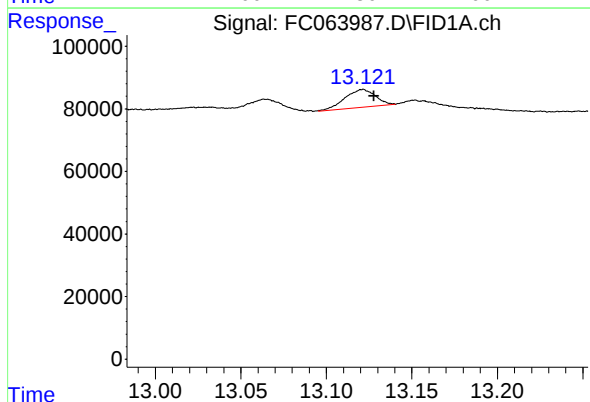


#11 n-Heneicosane (C21)

R.T.: 13.121 min
Delta R.T.: -0.007 min
Response: 70501
Conc: 0.44 ug/ml

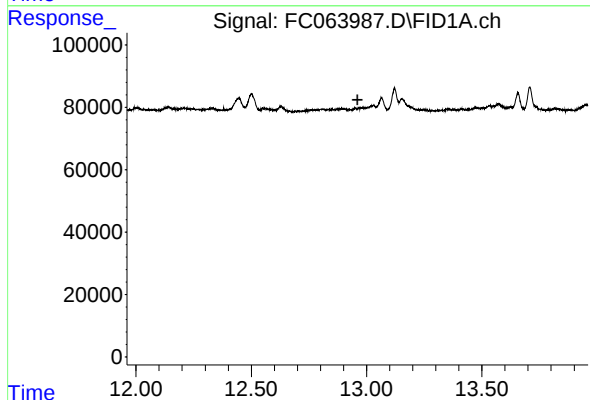


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.961 min
Response: 0
Conc: N.D.

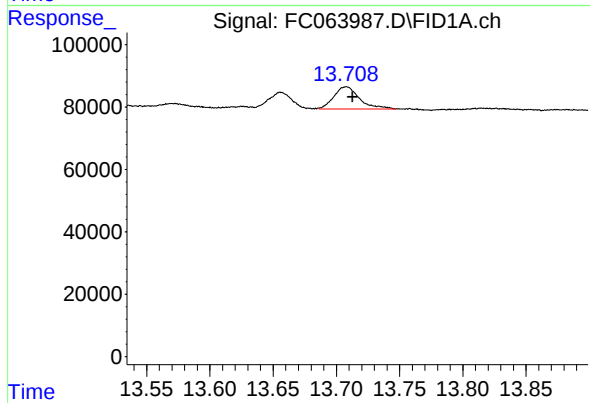

#13 n-Docosane (C22)

R.T.: 13.708 min
Delta R.T.: -0.005 min
Response: 99245
Conc: 0.63 ug/ml

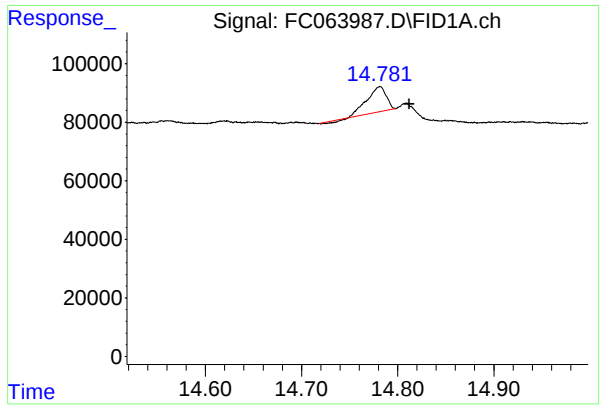

#14 n-Tetracosane (C24)

R.T.: 14.782 min
Delta R.T.: -0.031 min
Response: 115761
Conc: 0.73 ug/ml

Instrument :

FID_C

ClientSampleId :