

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062623AL\
 Data File : FC063994.D
 Signal(s) : FID1A.ch
 Acq On : 26 Jun 2023 17:16
 Operator : YP/AJ
 Sample : PB153788BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 27 03:55:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 062423.M
 Quant Title : GC Extractables
 QLast Update : Sun Jun 25 04:03:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.531	10490559	54.030 ug/ml
Spiked Amount 50.000		Recovery =	108.06%
12) S 1-chlorooctadecane (S...	12.961	2416765	17.370 ug/ml
Spiked Amount 50.000		Recovery =	34.74%
Target Compounds			
10) T n-Eicosane (C20)	12.517	91633	0.561 ug/ml
14) T n-Tetracosane (C24)	14.804	403458	2.560 ug/ml
17) T n-Tricontane (C30)	17.662	112460	0.720 ug/ml
18) T n-Dotriacontane (C32)	18.491	127799	0.809 ug/ml
19) T n-Tetratriacontane (C34)	19.273	116548	0.757 ug/ml
20) T n-Hexatriacontane (C36)	20.008	99145	0.672 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062623AL\
Data File : FC063994.D
Signal(s) : FID1A.ch
Acq On : 26 Jun 2023 17:16
Operator : YP/AJ
Sample : PB153788BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 27 03:55:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 062423.M
Quant Title : GC Extractables
QLast Update : Sun Jun 25 04:03:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

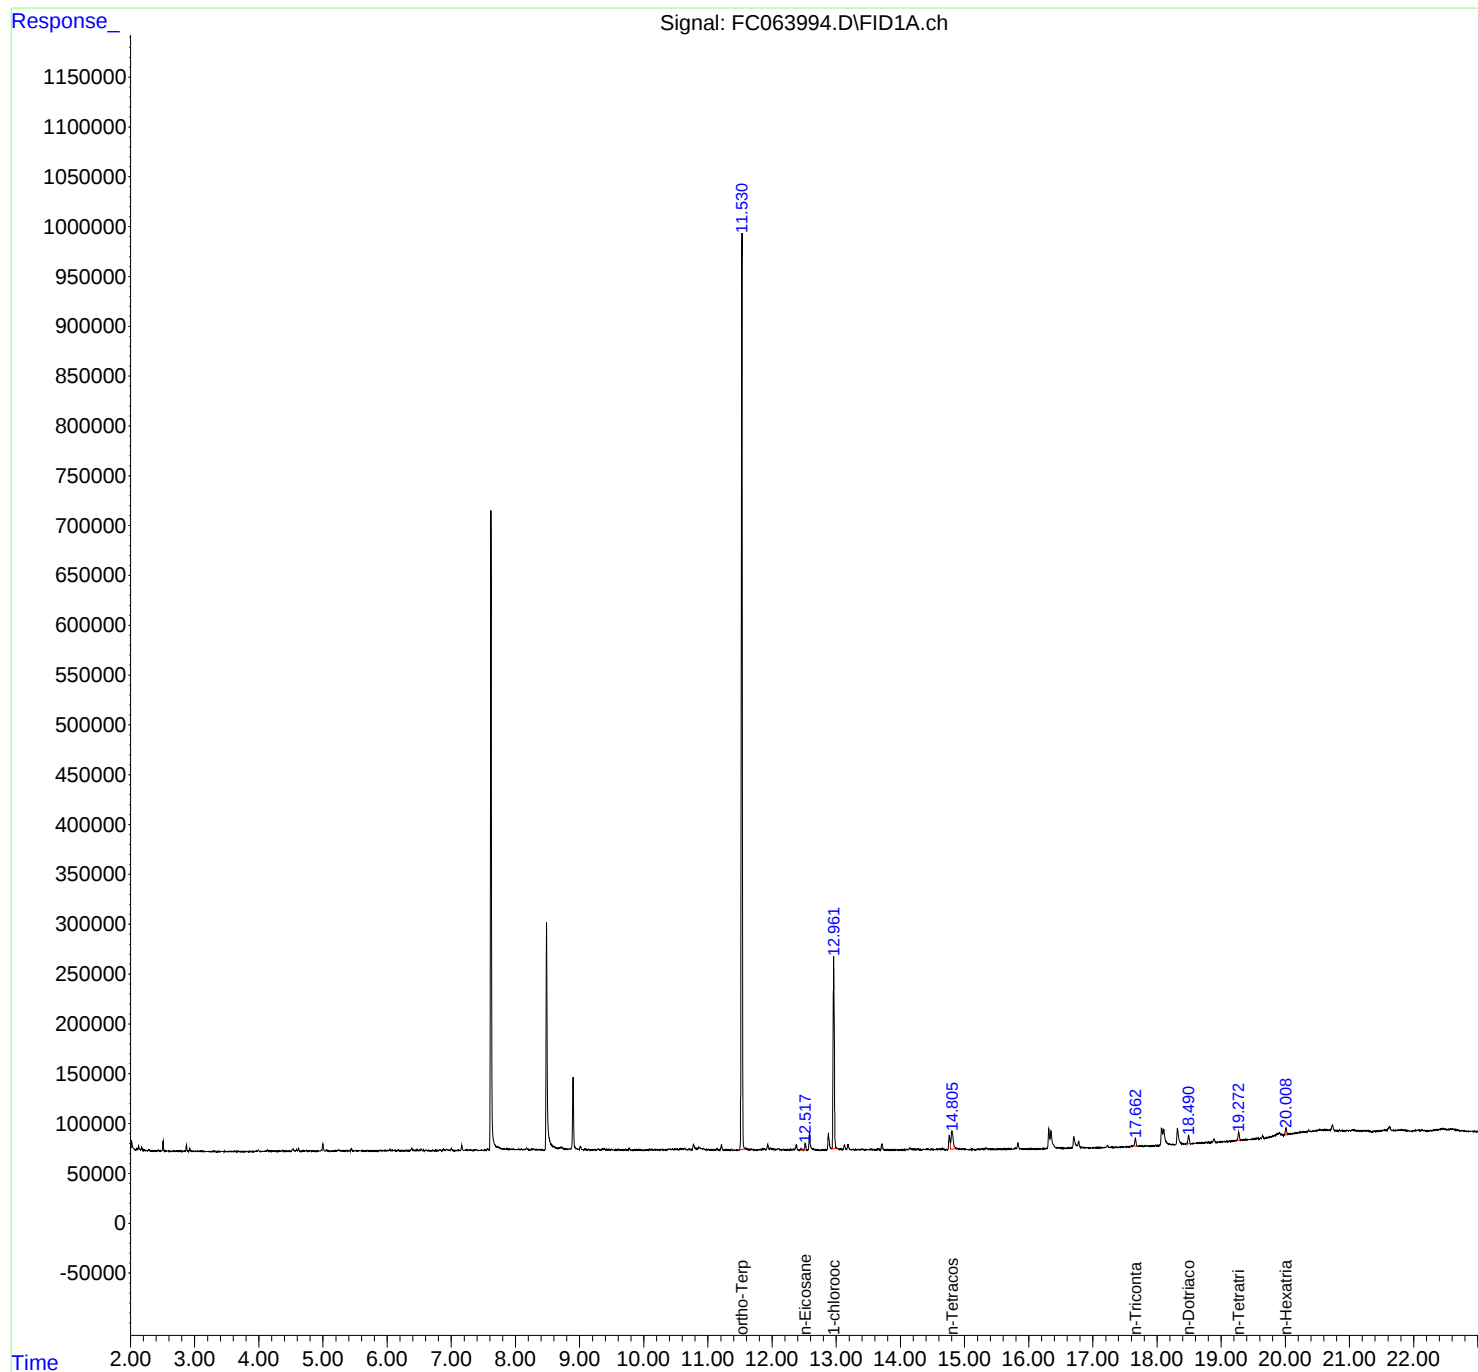


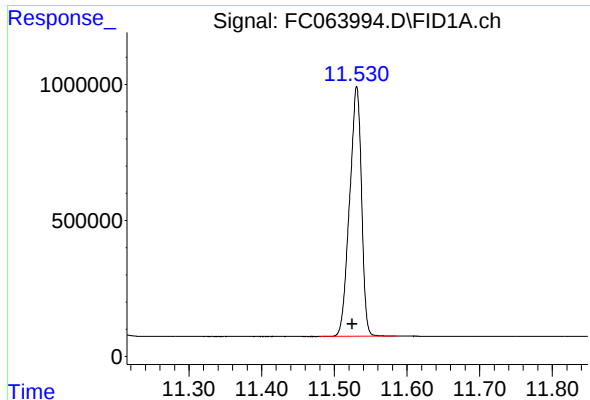

#9 ortho-Terphenyl (SURR)


R.T.: 11.531 min
Delta R.T.: 0.006 min
Response: 10490559
Conc: 54.03 ug/ml

Instrument :
FID_C
ClientSampleId :

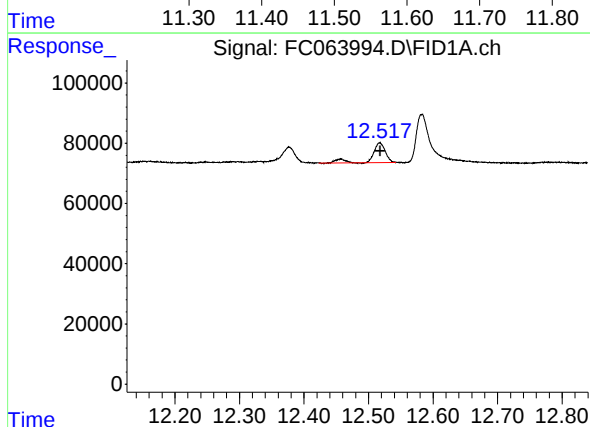


#10 n-Eicosane (C20)

R.T.: 12.517 min
Delta R.T.: 0.000 min
Response: 91633
Conc: 0.56 ug/ml

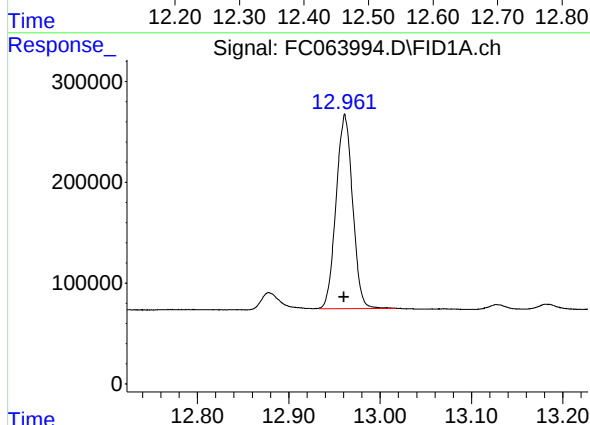


#12 1-chlorooctadecane (SURR)

R.T.: 12.961 min
Delta R.T.: 0.000 min
Response: 2416765
Conc: 17.37 ug/ml

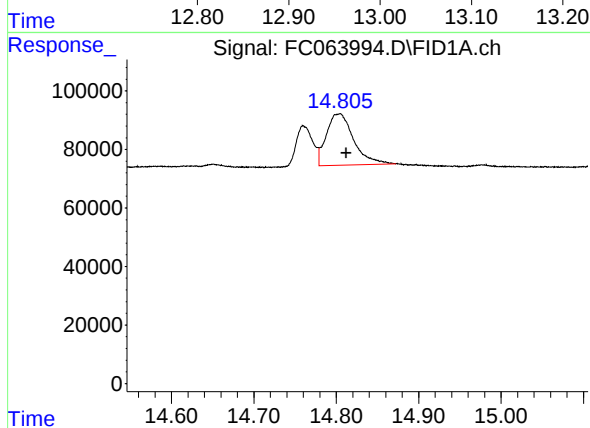

#14 n-Tetracosane (C24)


R.T.: 14.804 min
Delta R.T.: -0.008 min
Response: 403458
Conc: 2.56 ug/ml

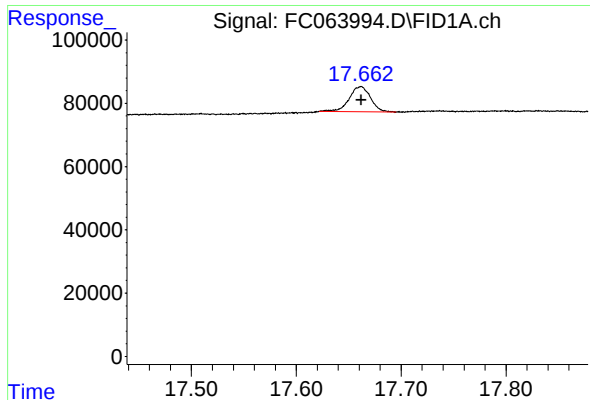

#17 n-Tricontane (C30)


R.T.: 17.662 min
Delta R.T.: 0.000 min
Response: 112460
Conc: 0.72 ug/ml

Instrument :
FID_C
ClientSampleId :

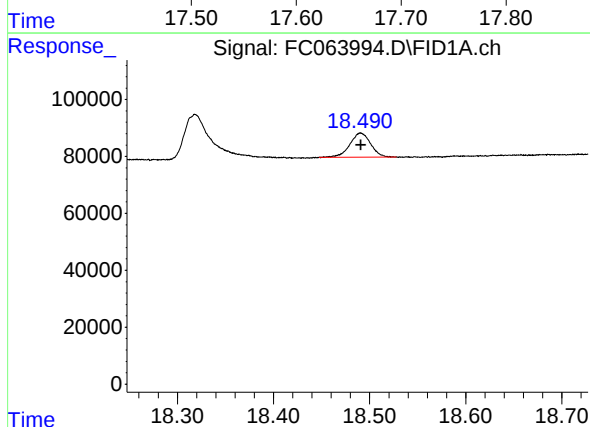


#18 n-Dotriacontane (C32)

R.T.: 18.491 min
Delta R.T.: 0.000 min
Response: 127799
Conc: 0.81 ug/ml

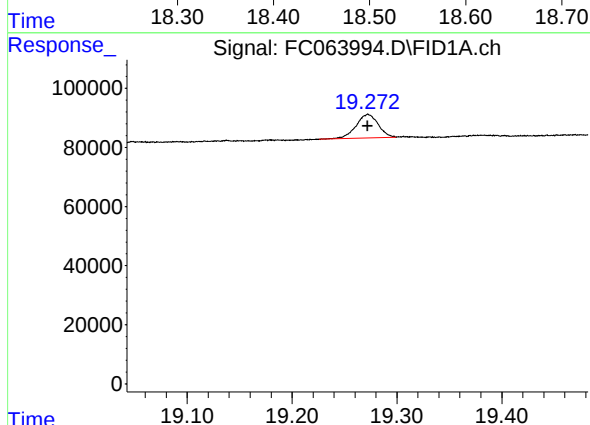

#19 n-Tetatriacontane (C34)

R.T.: 19.273 min
Delta R.T.: 0.000 min
Response: 116548
Conc: 0.76 ug/ml

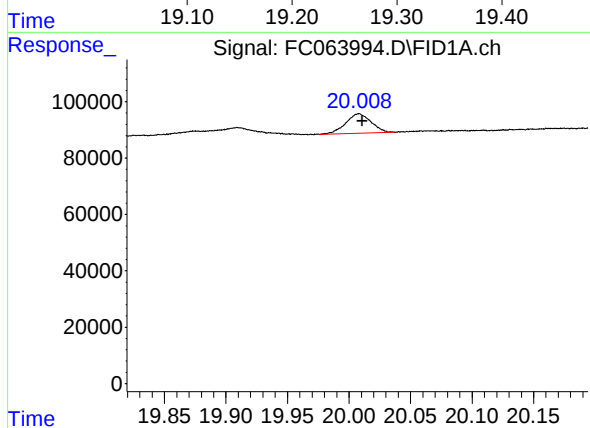

#20 n-Hexatriacontane (C36)

R.T.: 20.008 min
Delta R.T.: -0.003 min
Response: 99145
Conc: 0.67 ug/ml