

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC062722AL\  
 Data File : FC060479.D  
 Signal(s) : FID1A.ch  
 Acq On : 28 Jun 2022 06:13  
 Operator : YP/AJ  
 Sample : N3494-34  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 FID\_C  
 ClientSampleId :  
 SP-EXC-1-1-GR

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 06/28/2022  
 Supervised By :Ankita Jodhani 06/28/2022

Integration File: sample.E  
 Quant Time: Jun 28 06:49:33 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 062422.M  
 Quant Title : GC Extractables  
 QLast Update : Sat Jun 25 04:15:44 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units    |
|--------------------------------|--------|------------|---------------|
| -----                          |        |            |               |
| System Monitoring Compounds    |        |            |               |
| 12) S 1-chlorooctadecane (S... | 12.009 | 3969264    | 26.929 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 53.86%        |
| Target Compounds               |        |            |               |
| -----                          |        |            |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC062722AL\  
Data File : FC060479.D  
Signal(s) : FID1A.ch  
Acq On : 28 Jun 2022 06:13  
Operator : YP/AJ  
Sample : N3494-34  
Misc :  
ALS Vial : 19 Sample Multiplier: 1


Instrument :  
FID\_C  
ClientSampleId :  
SP-EXC-1-1-GR


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/28/2022  
Supervised By :Ankita Jodhani 06/28/2022

Integration File: sample.E  
Quant Time: Jun 28 06:49:33 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 062422.M  
Quant Title : GC Extractables  
QLast Update : Sat Jun 25 04:15:44 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

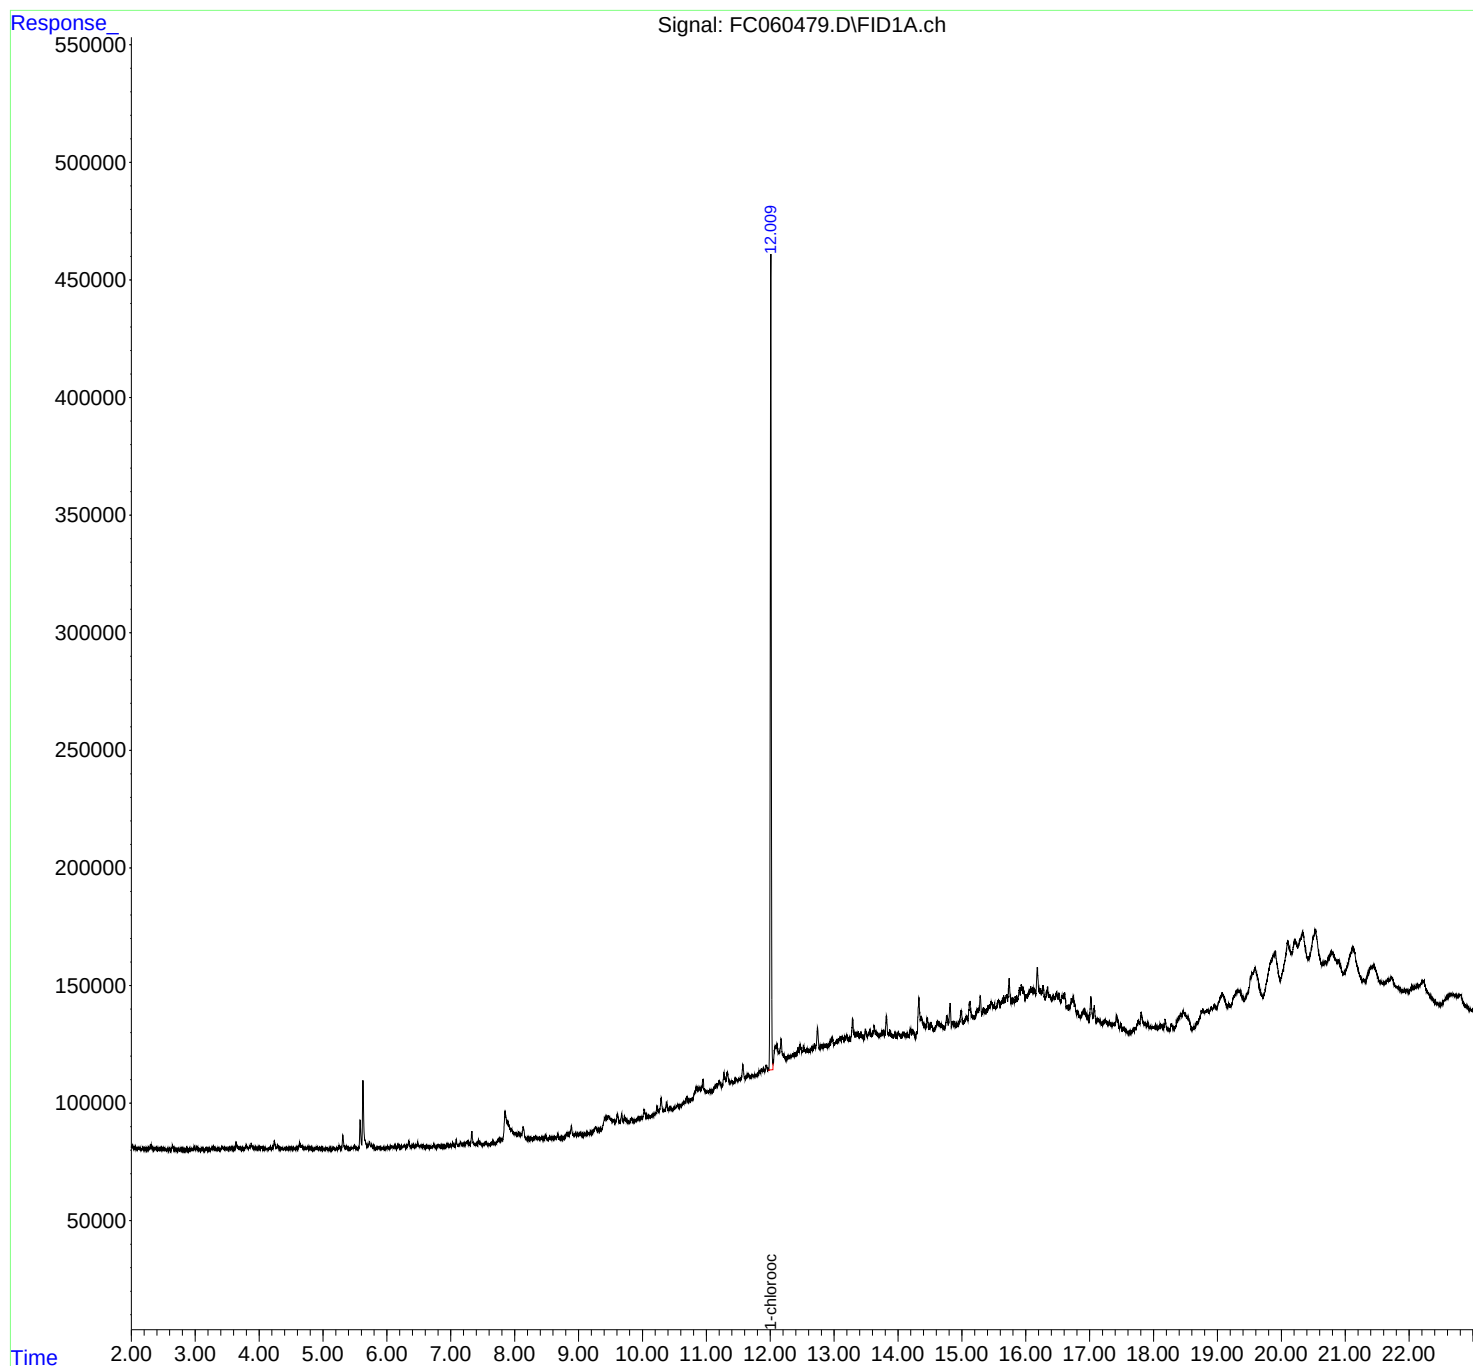

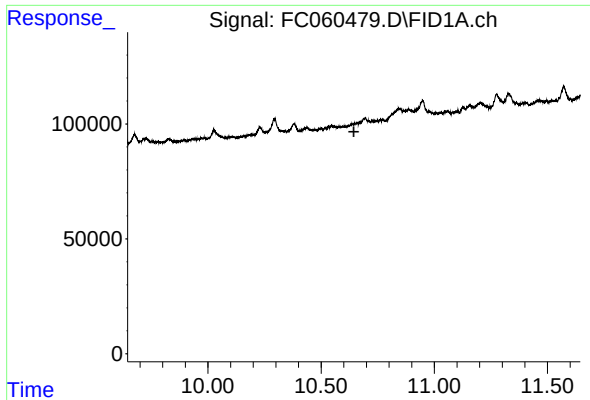


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T.: 10.645 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_C  
ClientSampleId :  
SP-EXC-1-1-GR

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/28/2022  
Supervised By :Ankita Jodhani 06/28/2022

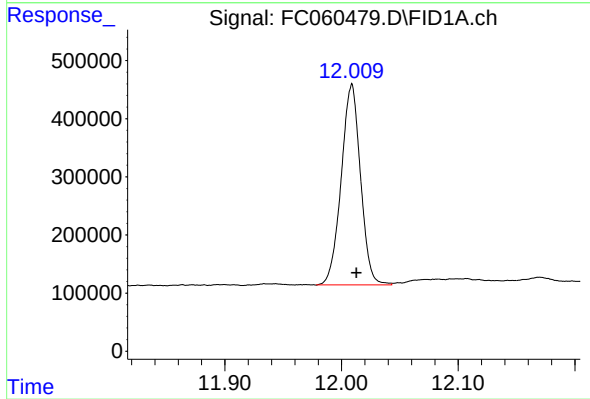

#12 1-chlorooctadecane (SURR)

R.T.: 12.009 min  
Delta R.T.: -0.004 min  
Response: 3969264  
Conc: 26.93 ug/ml m