

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062824AL\
 Data File : FC066680.D
 Signal(s) : FID1A.ch
 Acq On : 28 Jun 2024 09:57
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 29 02:17:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 17 13:44:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) T n-Heneicosane (C21)	13.133	68506	0.425 ug/ml
13) T n-Docosane (C22)	13.719	65905	0.411 ug/ml
14) T n-Tetracosane (C24)	14.823	47363	0.298 ug/ml
17) T n-Tricontane (C30)	17.683	115977	0.830 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062824AL\
Data File : FC066680.D
Signal(s) : FID1A.ch
Acq On : 28 Jun 2024 09:57
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 29 02:17:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
Quant Title : GC Extractables
QLast Update : Mon Jun 17 13:44:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

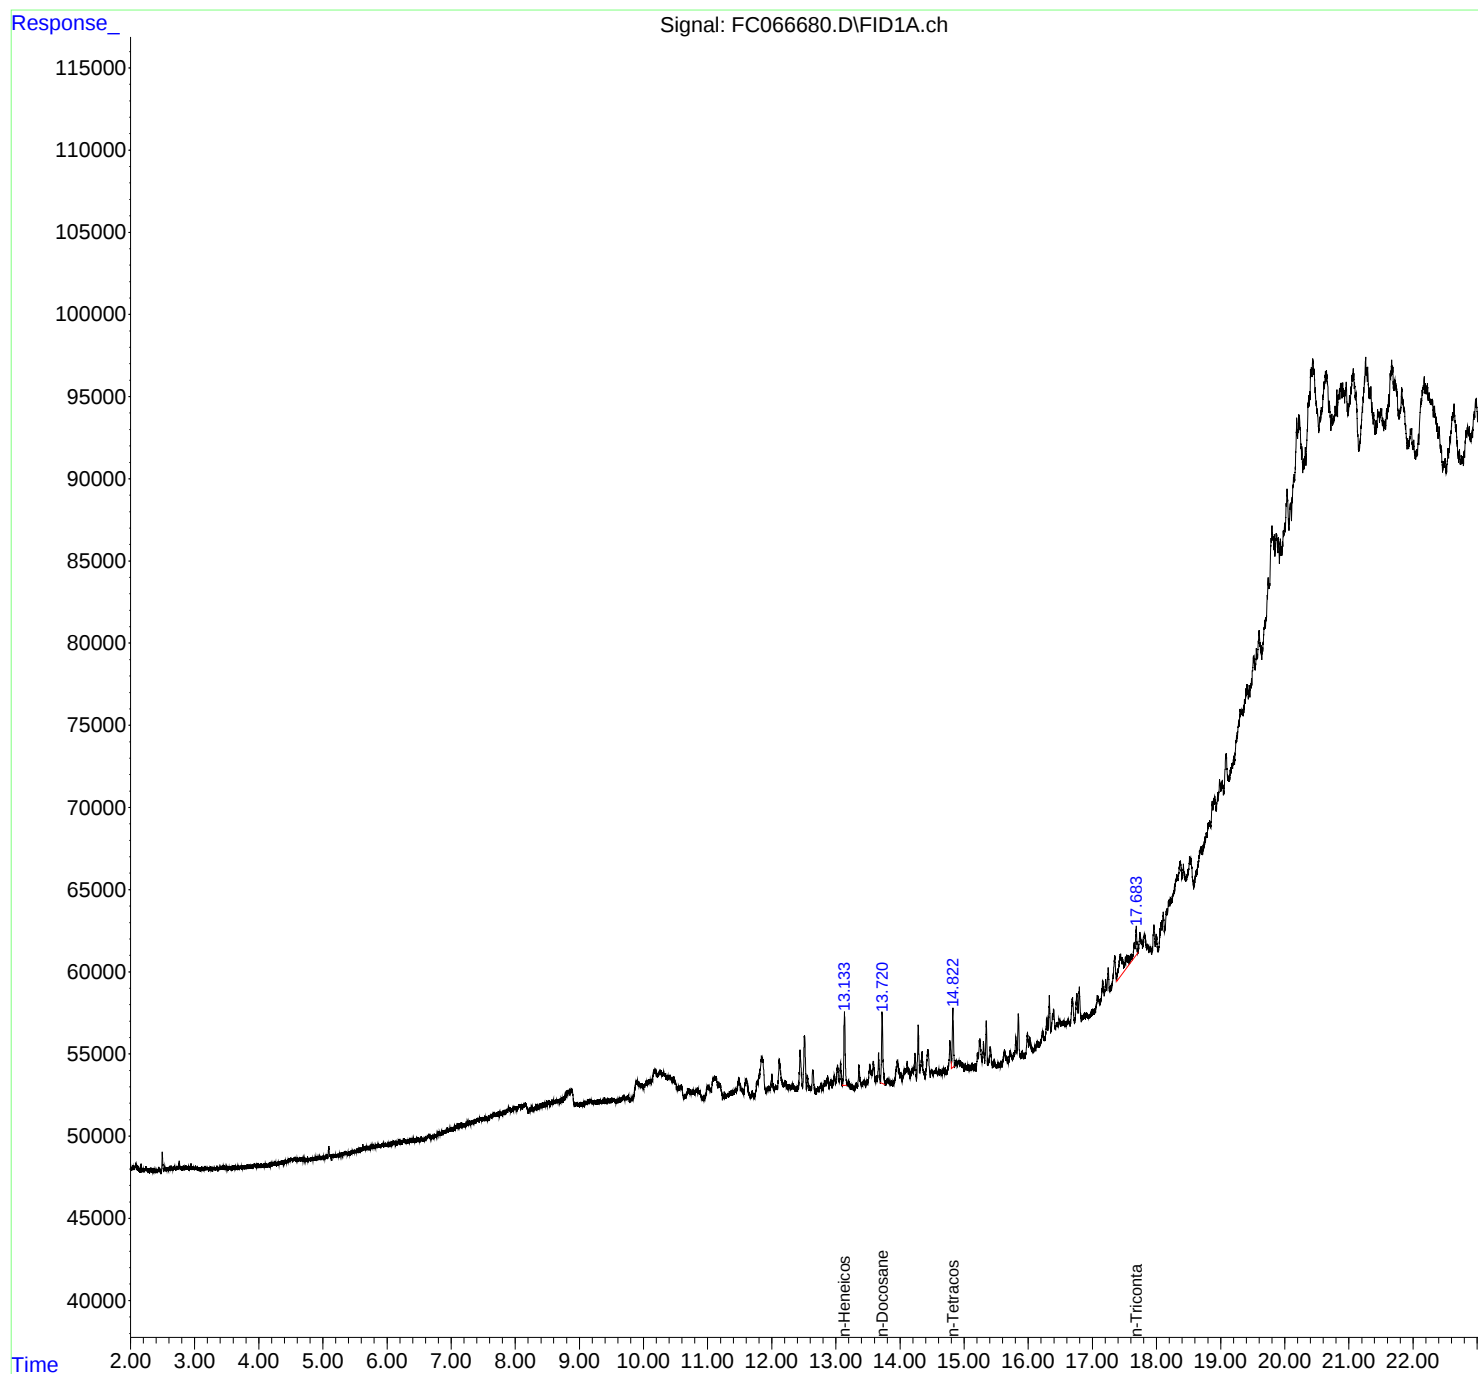


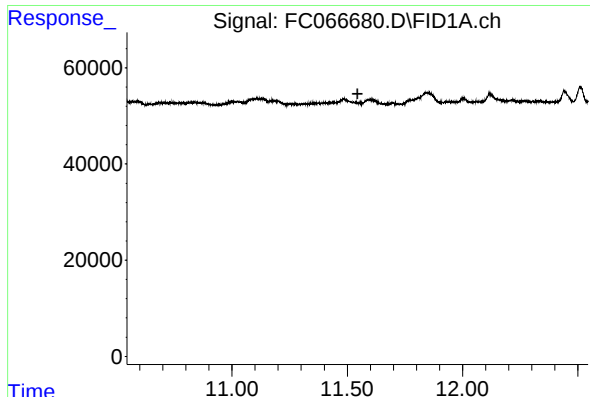

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.544 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

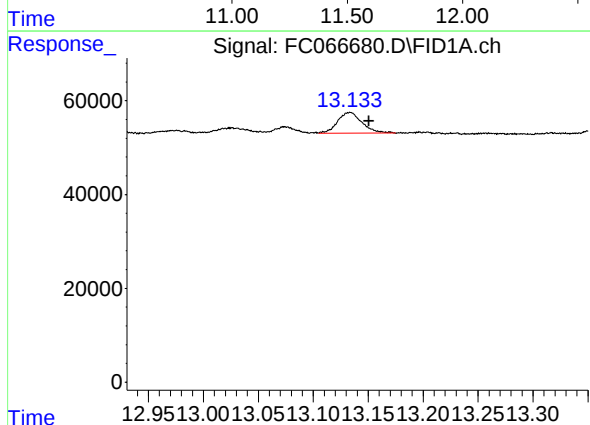


#11 n-Heneicosane (C21)

R.T.: 13.133 min
Delta R.T.: -0.018 min
Response: 68506
Conc: 0.43 ug/ml

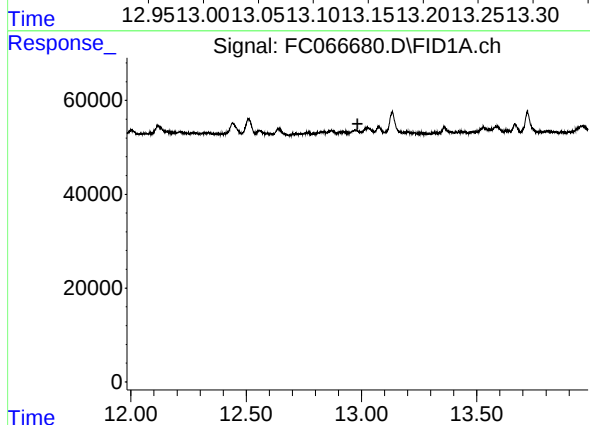


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.983 min
Response: 0
Conc: N.D.

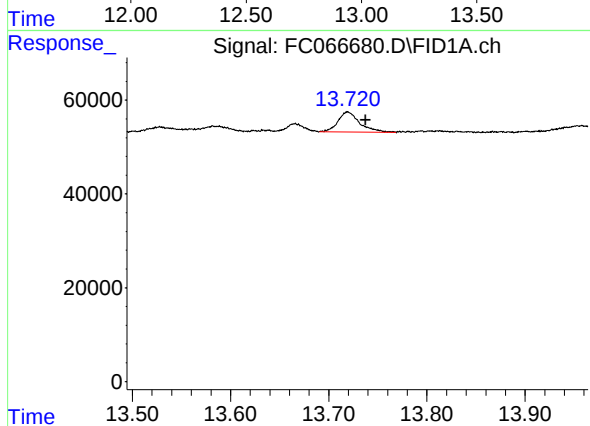

#13 n-Docosane (C22)


R.T.: 13.719 min
Delta R.T.: -0.018 min
Response: 65905
Conc: 0.41 ug/ml

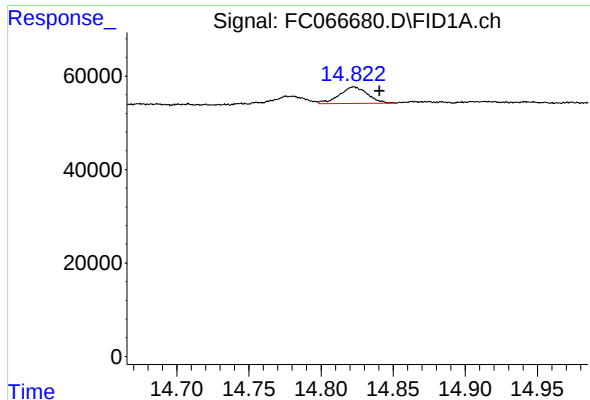

#14 n-Tetracosane (C24)

R.T.: 14.823 min
Delta R.T.: -0.017 min
Response: 47363
Conc: 0.30 ug/ml

Instrument :
FID_C
ClientSampleId :

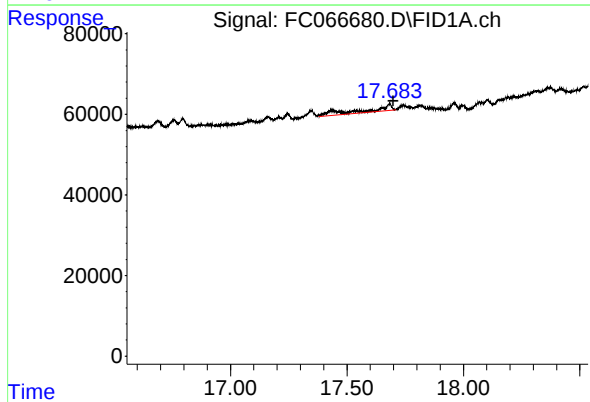

#17 n-Tricontane (C30)

R.T.: 17.683 min
Delta R.T.: -0.016 min
Response: 115977
Conc: 0.83 ug/ml