

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062824AL\
Data File : FC066694.D
Signal(s) : FID1A.ch
Acq On : 28 Jun 2024 23:06
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 29 02:19:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
Quant Title : GC Extractables
QLast Update : Mon Jun 17 13:44:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.686	44331	0.317 ug/ml
19) T	n-Tetratriacontane (C34)	19.310	45233	0.366 ug/ml
20) T	n-Hexatriacontane (C36)	20.117f	23046	0.191 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC062824AL\
Data File : FC066694.D
Signal(s) : FID1A.ch
Acq On : 28 Jun 2024 23:06
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 29 02:19:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
Quant Title : GC Extractables
QLast Update : Mon Jun 17 13:44:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

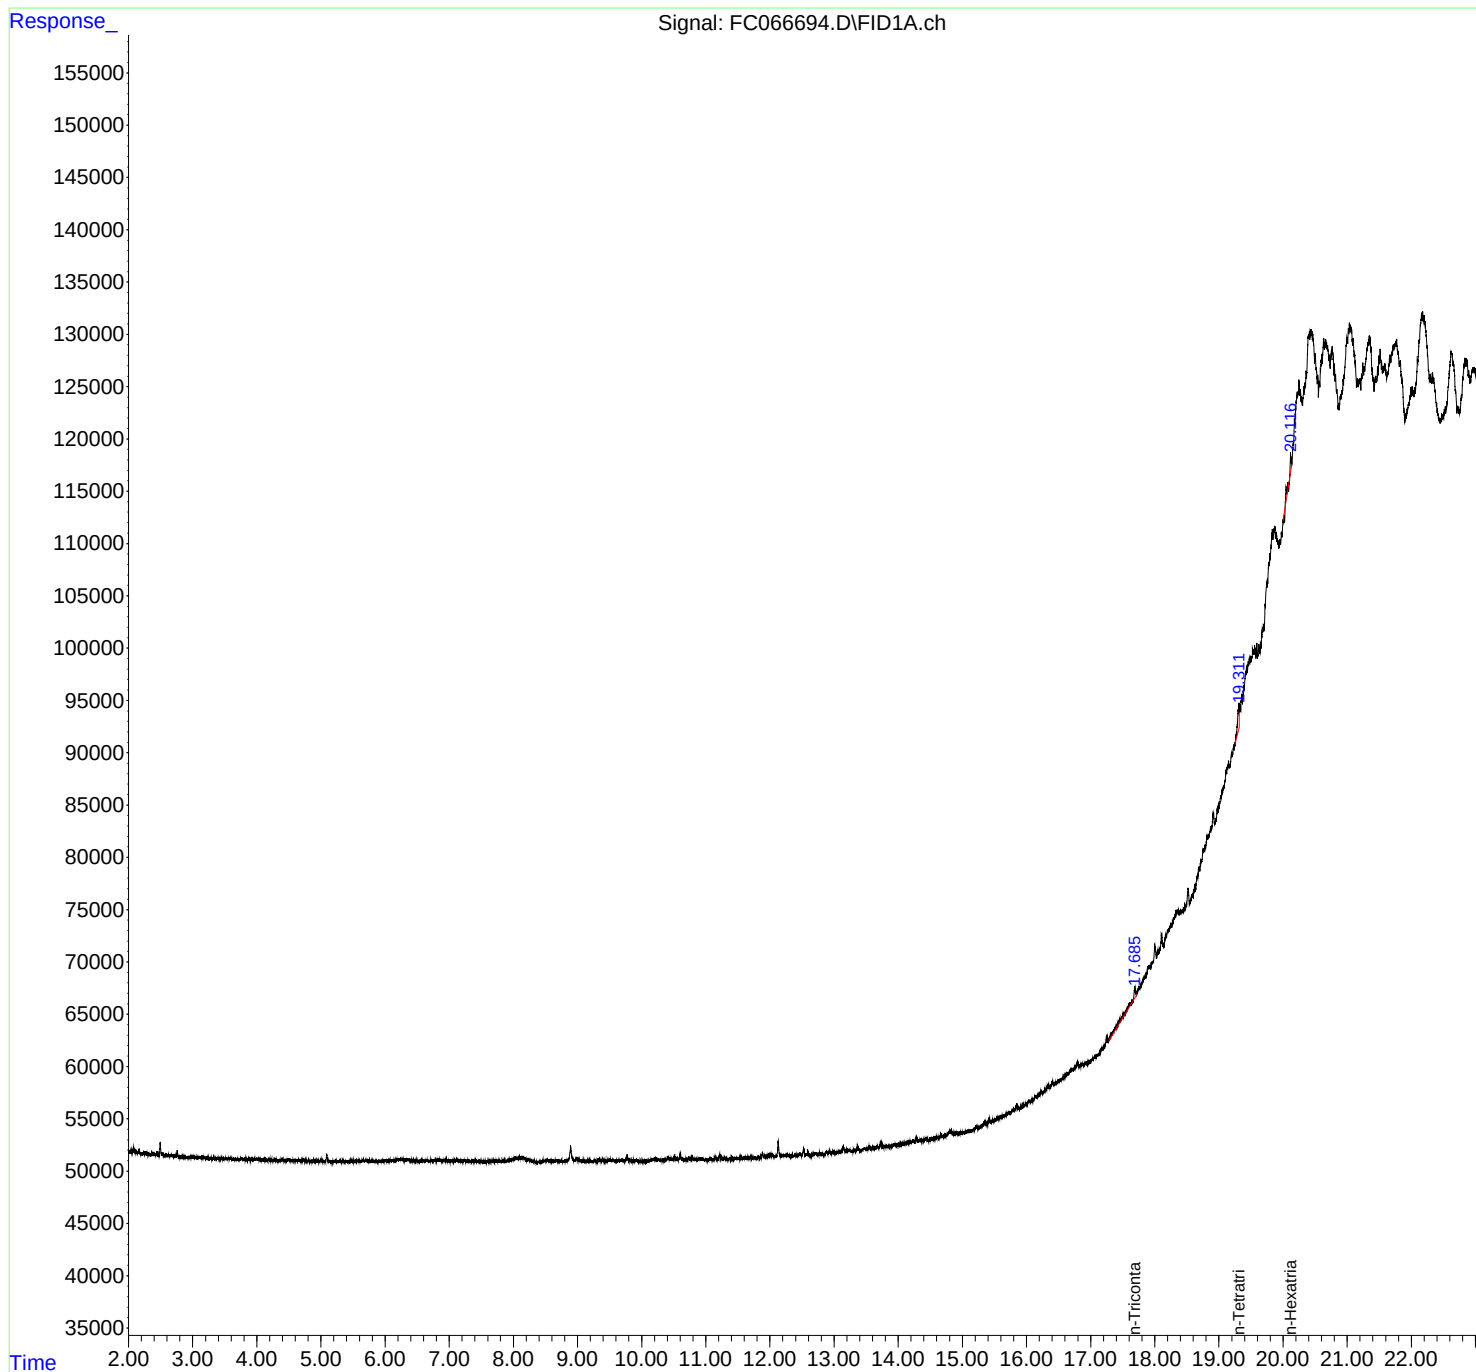


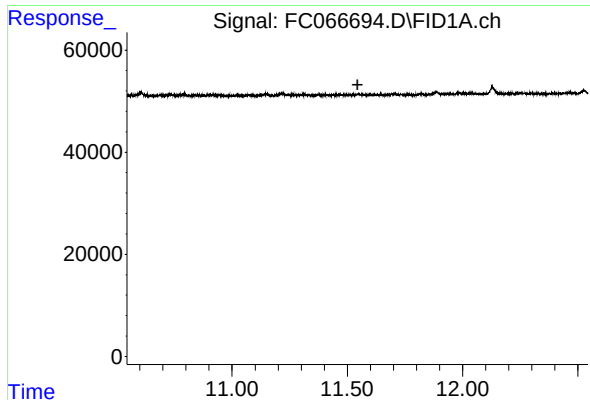

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.544 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

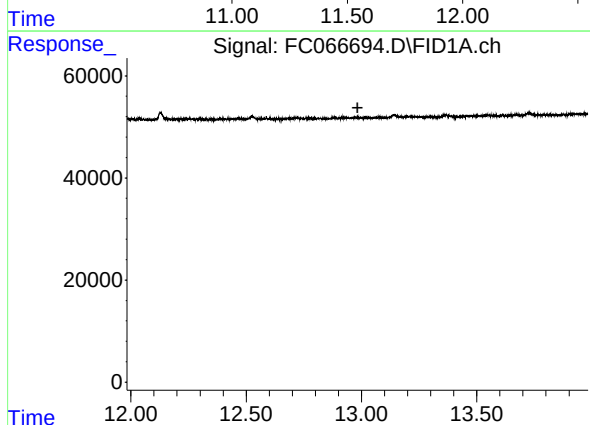


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.983 min
Response: 0
Conc: N.D.

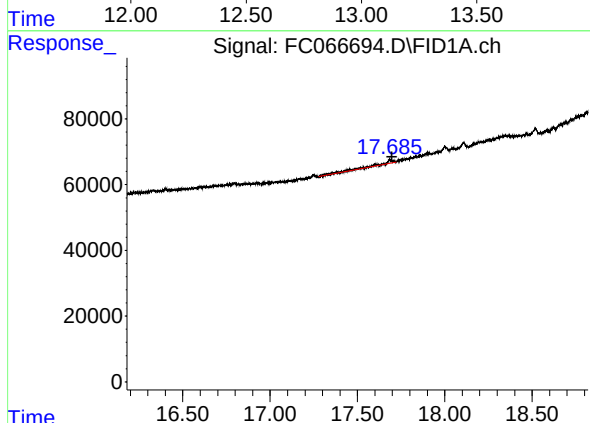


#17 n-Tricontane (C30)

R.T.: 17.686 min
Delta R.T.: -0.013 min
Response: 44331
Conc: 0.32 ug/ml

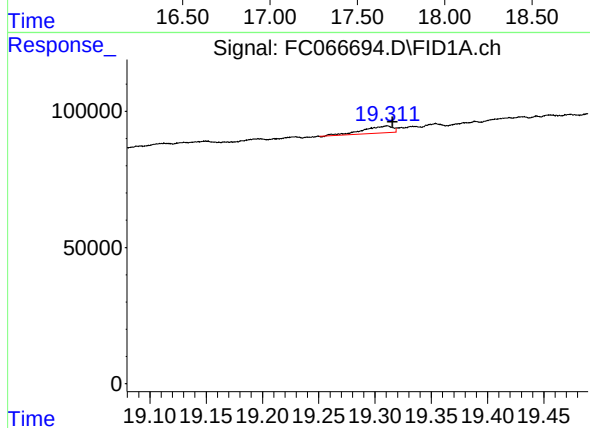

#19 n-Tetratriacontane (C34)

R.T.: 19.310 min
Delta R.T.: -0.005 min
Response: 45233
Conc: 0.37 ug/ml

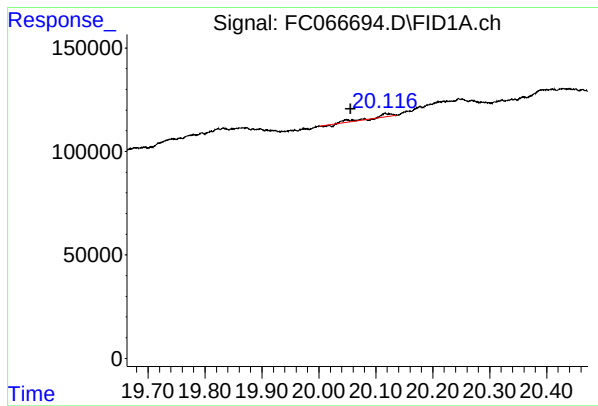

#20 n-Hexatriacontane (C36)

R.T.: 20.117 min
Delta R.T.: 0.061 min
Response: 23046
Conc: 0.19 ug/ml

Instrument :
FID_C
ClientSampleId :