

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC070124AL\
 Data File : FC066703.D
 Signal(s) : FID1A.ch
 Acq On : 01 Jul 2024 15:20
 Operator : YP/AJ
 Sample : P3134-01D
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 02 03:11:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 17 13:44:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.533	6683482	38.748 ug/ml
Spiked Amount 50.000		Recovery =	77.50%
12) S 1-chlorooctadecane (S...	12.972	5501248	39.870 ug/ml
Spiked Amount 50.000		Recovery =	79.74%
Target Compounds			
10) T n-Eicosane (C20)	12.546	57789	0.355 ug/ml
14) T n-Tetracosane (C24)	14.788f	74288	0.468 ug/ml
15) T n-Hexacosane (C26)	15.845	48973	0.321 ug/ml
16) T n-Octacosane (C28)	16.794	195761	1.357 ug/ml
17) T n-Tricontane (C30)	17.682	108877	0.779 ug/ml
18) T n-Dotriacontane (C32)	18.511	262394	1.988 ug/ml
19) T n-Tetratriacontane (C34)	19.310	102393	0.828 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC070124AL\
Data File : FC066703.D
Signal(s) : FID1A.ch
Acq On : 01 Jul 2024 15:20
Operator : YP/AJ
Sample : P3134-01D
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 02 03:11:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
Quant Title : GC Extractables
QLast Update : Mon Jun 17 13:44:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

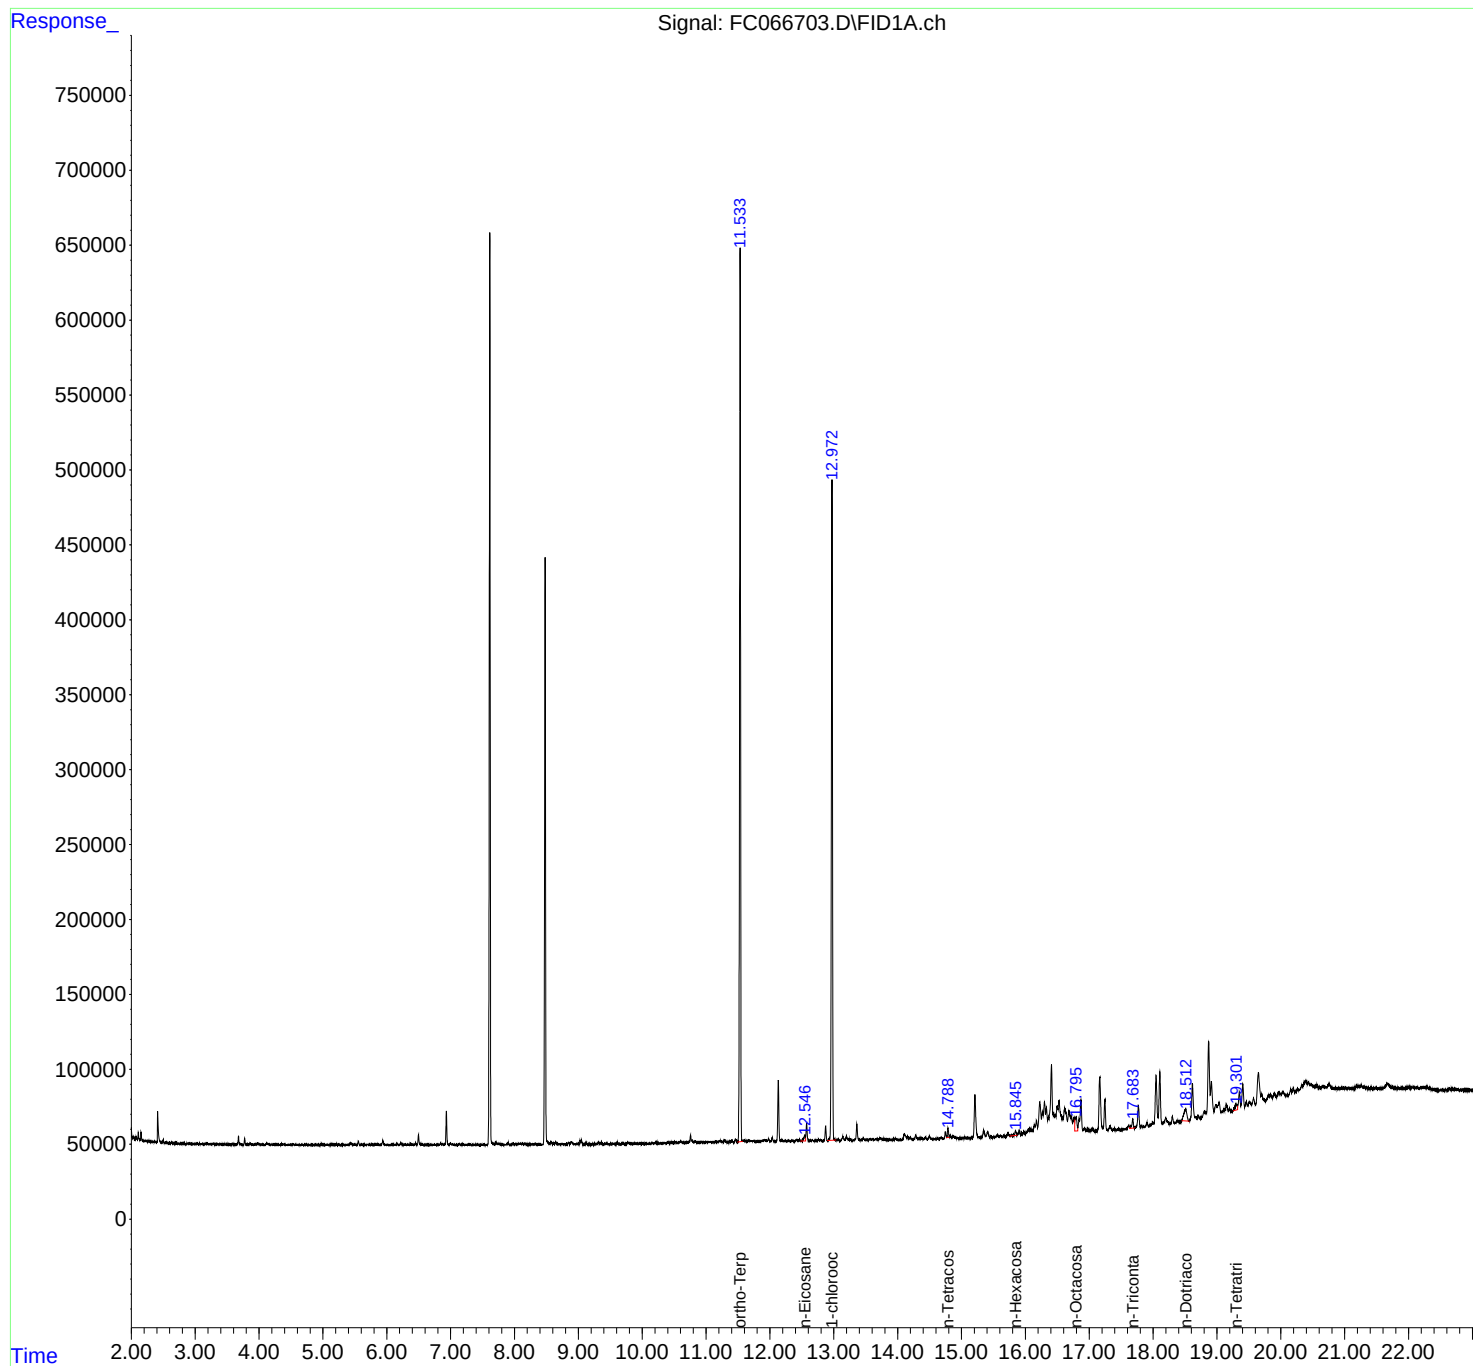


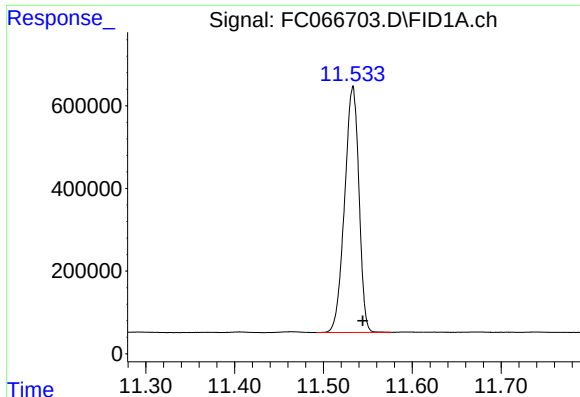

#9 ortho-Terphenyl (SURR)


R.T.: 11.533 min
Delta R.T.: -0.011 min
Response: 6683482
Conc: 38.75 ug/ml

Instrument :
FID_C
ClientSampleId :

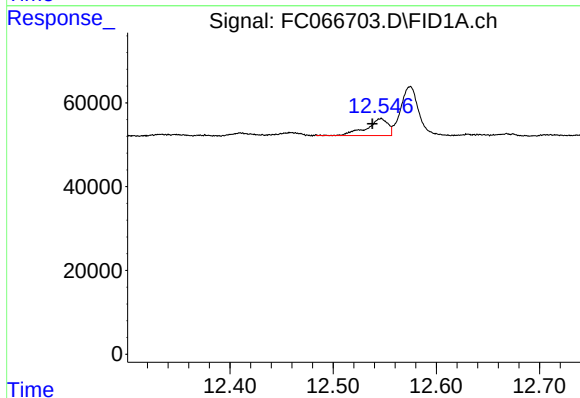


#10 n-Eicosane (C20)

R.T.: 12.546 min
Delta R.T.: 0.008 min
Response: 57789
Conc: 0.36 ug/ml

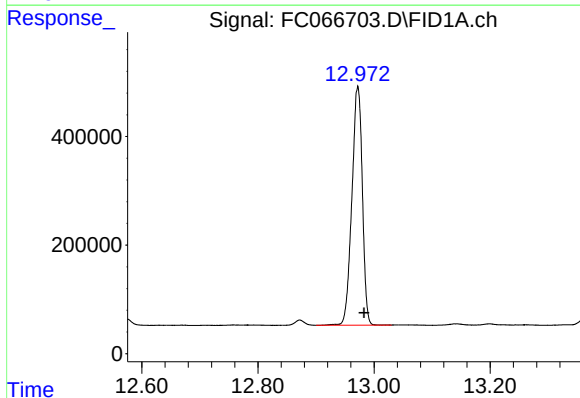


#12 1-chlorooctadecane (SURR)

R.T.: 12.972 min
Delta R.T.: -0.011 min
Response: 5501248
Conc: 39.87 ug/ml

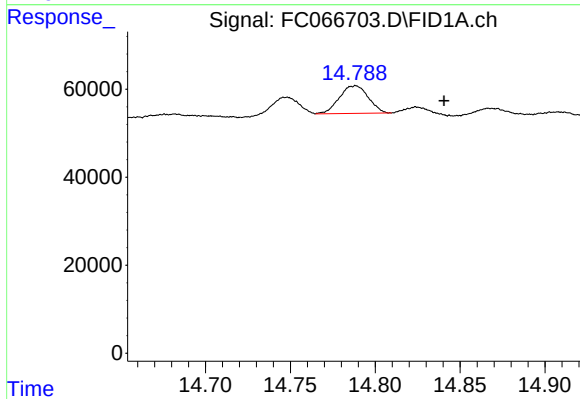

#14 n-Tetracosane (C24)


R.T.: 14.788 min
Delta R.T.: -0.053 min
Response: 74288
Conc: 0.47 ug/ml

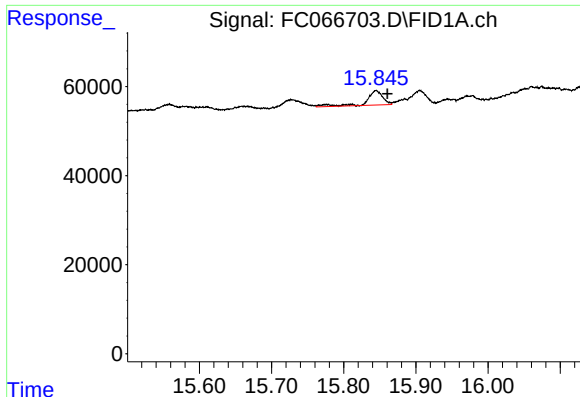

#15 n-Hexacosane (C26)


R.T.: 15.845 min
Delta R.T.: -0.016 min
Response: 48973
Conc: 0.32 ug/ml

Instrument :
FID_C
ClientSampleId :

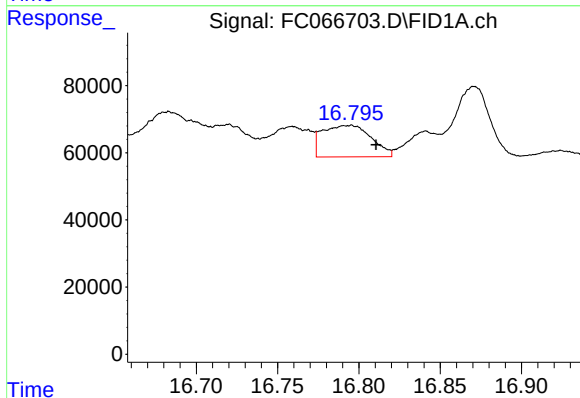


#16 n-Octacosane (C28)

R.T.: 16.794 min
Delta R.T.: -0.016 min
Response: 195761
Conc: 1.36 ug/ml

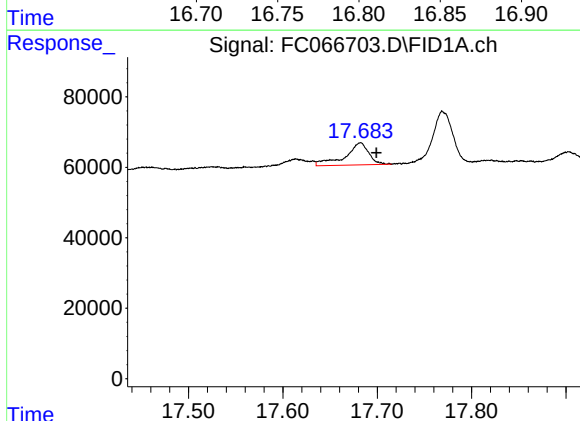


#17 n-Tricontane (C30)

R.T.: 17.682 min
Delta R.T.: -0.017 min
Response: 108877
Conc: 0.78 ug/ml

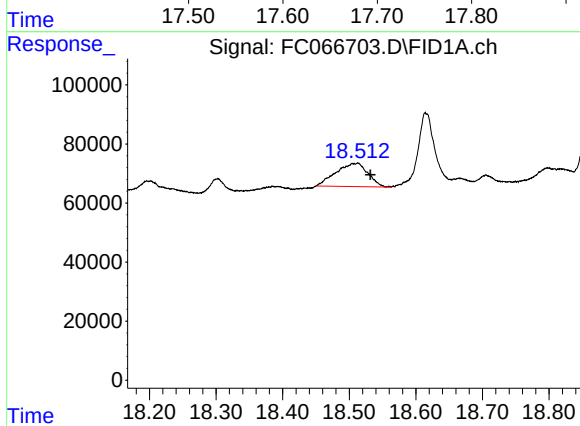

#18 n-Dotriacontane (C32)

R.T.: 18.511 min
Delta R.T.: -0.020 min
Response: 262394
Conc: 1.99 ug/ml

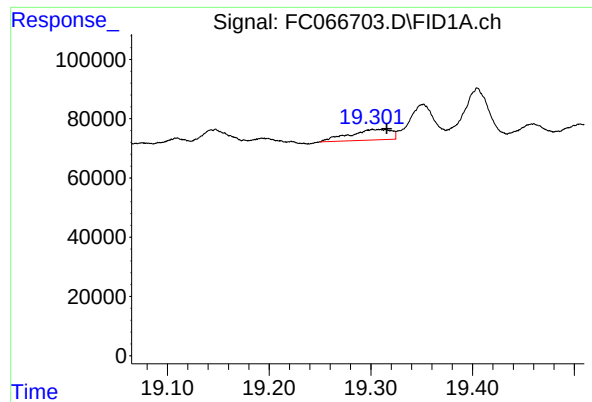

#19 n-Tetratriacontane (C34)

R.T.: 19.310 min
Delta R.T.: -0.006 min
Response: 102393
Conc: 0.83 ug/ml

Instrument :

FID_C

ClientSampleId :