

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC070224AL\
 Data File : FC066721.D
 Signal(s) : FID1A.ch
 Acq On : 02 Jul 2024 18:56
 Operator : YP/AJ
 Sample : P3141-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 03 03:02:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 17 13:44:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.965	4546908	32.953 ug/ml
Spiked Amount 50.000		Recovery =	65.91%
Target Compounds			
4) T n-Dodecane (C12)	6.374	86604	0.571 ug/ml
6) T n-Tetradecane (C14)	8.168	55507	0.366 ug/ml
14) T n-Tetracosane (C24)	14.861	115267	0.726 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC070224AL\
Data File : FC066721.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2024 18:56
Operator : YP/AJ
Sample : P3141-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 03:02:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
Quant Title : GC Extractables
QLast Update : Mon Jun 17 13:44:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

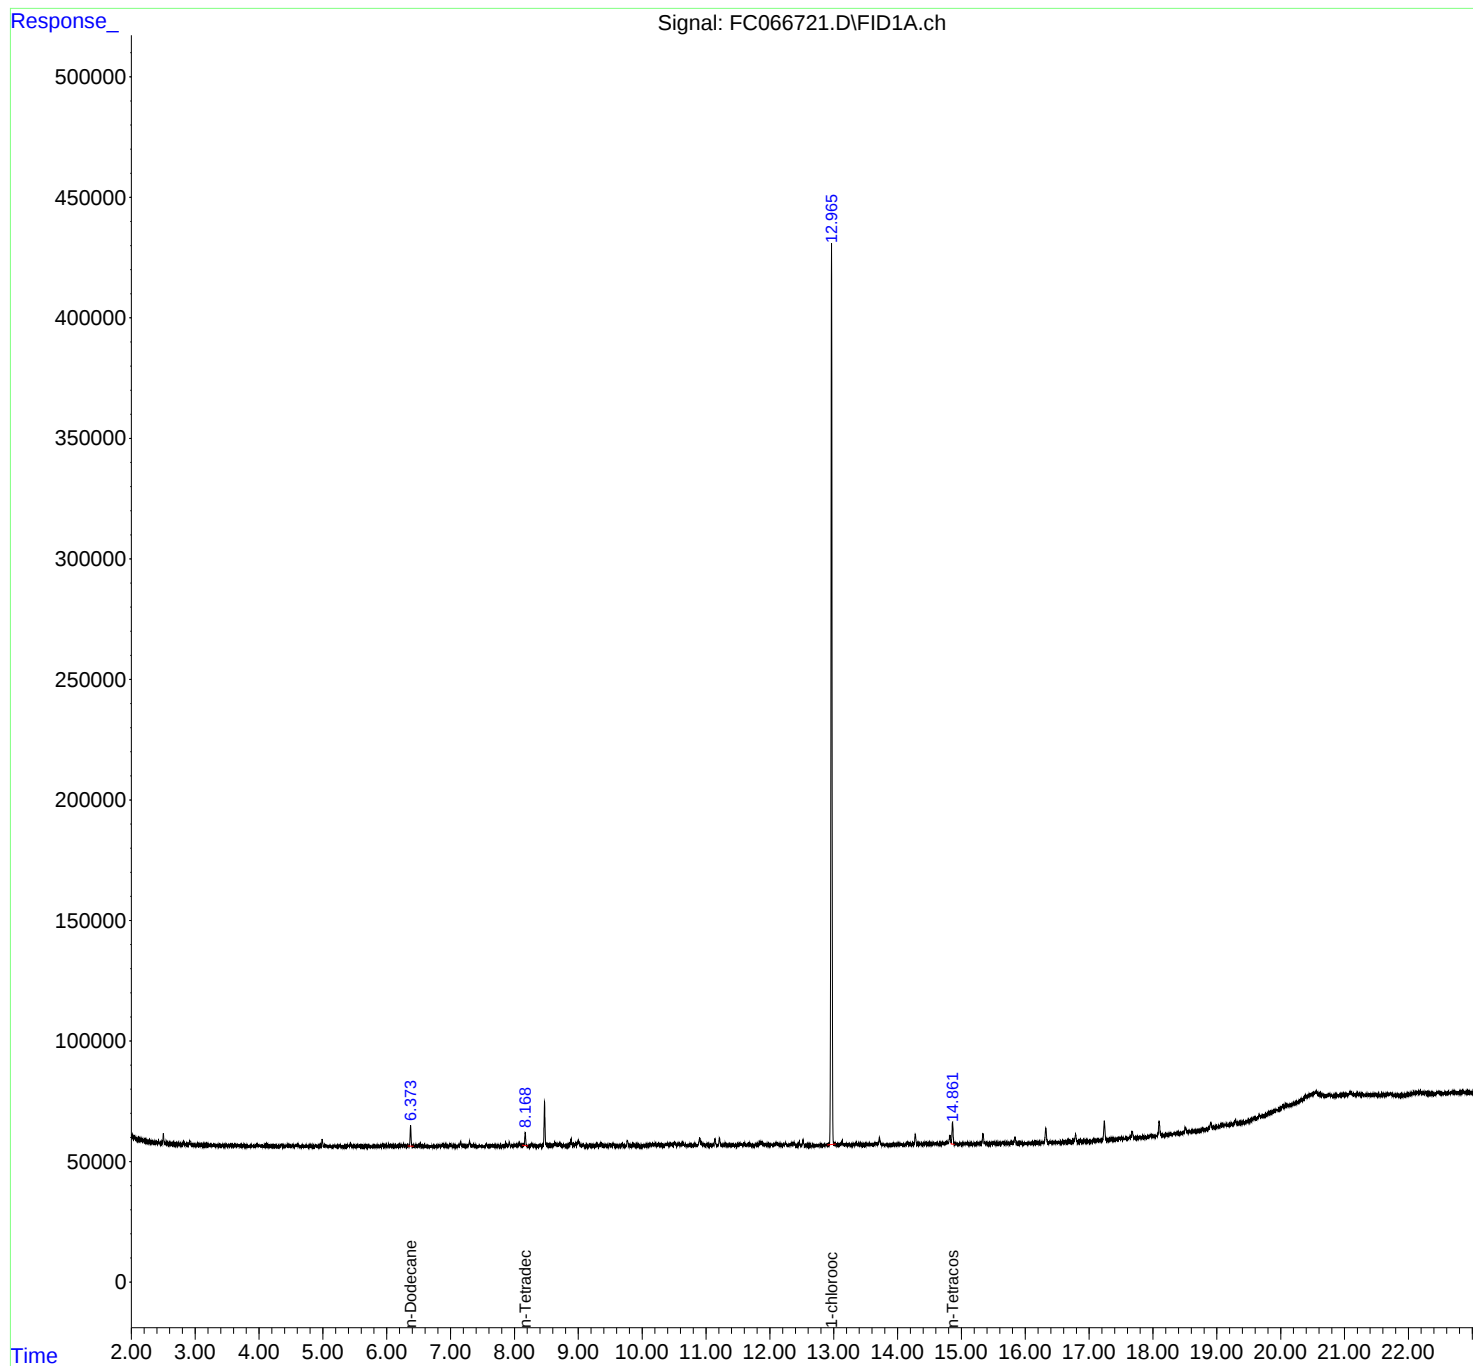


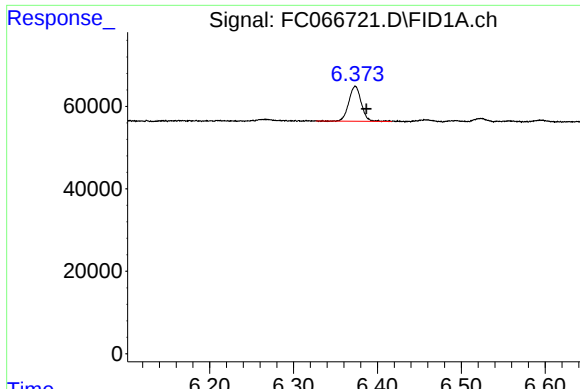

#4 n-Dodecane (C12)


R.T.: 6.374 min
Delta R.T.: -0.013 min
Response: 86604
Conc: 0.57 ug/ml

Instrument :
FID_C
ClientSampleId :

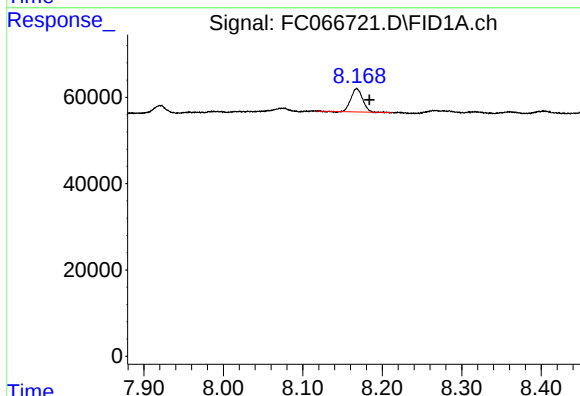


#6 n-Tetradecane (C14)

R.T.: 8.168 min
Delta R.T.: -0.016 min
Response: 55507
Conc: 0.37 ug/ml

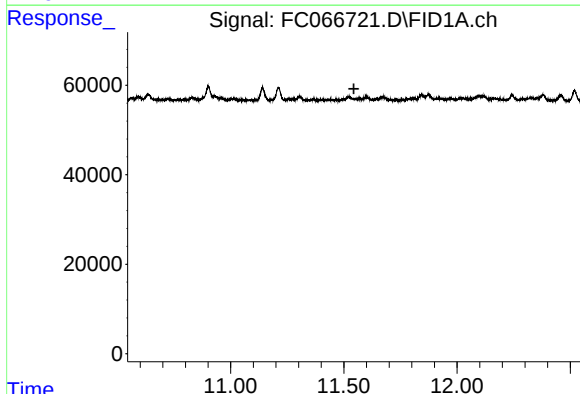


#9 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.544 min
Response: 0
Conc: N.D.

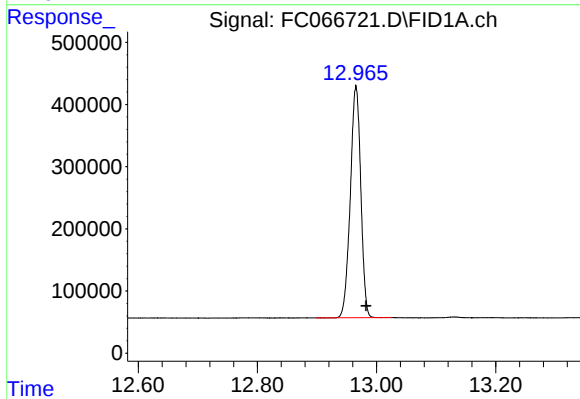

#12 1-chlorooctadecane (SURRE)

R.T.: 12.965 min
Delta R.T.: -0.017 min
Response: 4546908
Conc: 32.95 ug/ml

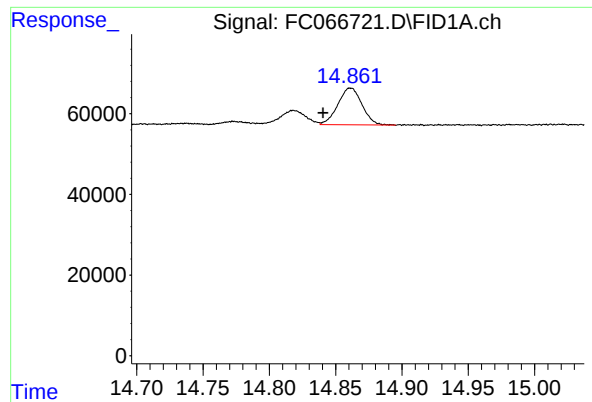

#14 n-Tetracosane (C24)

R.T.: 14.861 min
Delta R.T.: 0.021 min
Response: 115267
Conc: 0.73 ug/ml

Instrument :
FID_C
ClientSampleId :