

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC070224AL\
 Data File : FC066727.D
 Signal(s) : FID1A.ch
 Acq On : 02 Jul 2024 23:17
 Operator : YP/AJ
 Sample : P3141-05D
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 03 03:03:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 17 13:44:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.965	4798401	34.776 ug/ml
Spiked Amount 50.000		Recovery =	69.55%
Target Compounds			
4) T n-Dodecane (C12)	6.373	92834	0.613 ug/ml
6) T n-Tetradecane (C14)	8.167	64210	0.423 ug/ml
14) T n-Tetracosane (C24)	14.859	127421	0.803 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC070224AL\
Data File : FC066727.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2024 23:17
Operator : YP/AJ
Sample : P3141-05D
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 03:03:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
Quant Title : GC Extractables
QLast Update : Mon Jun 17 13:44:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

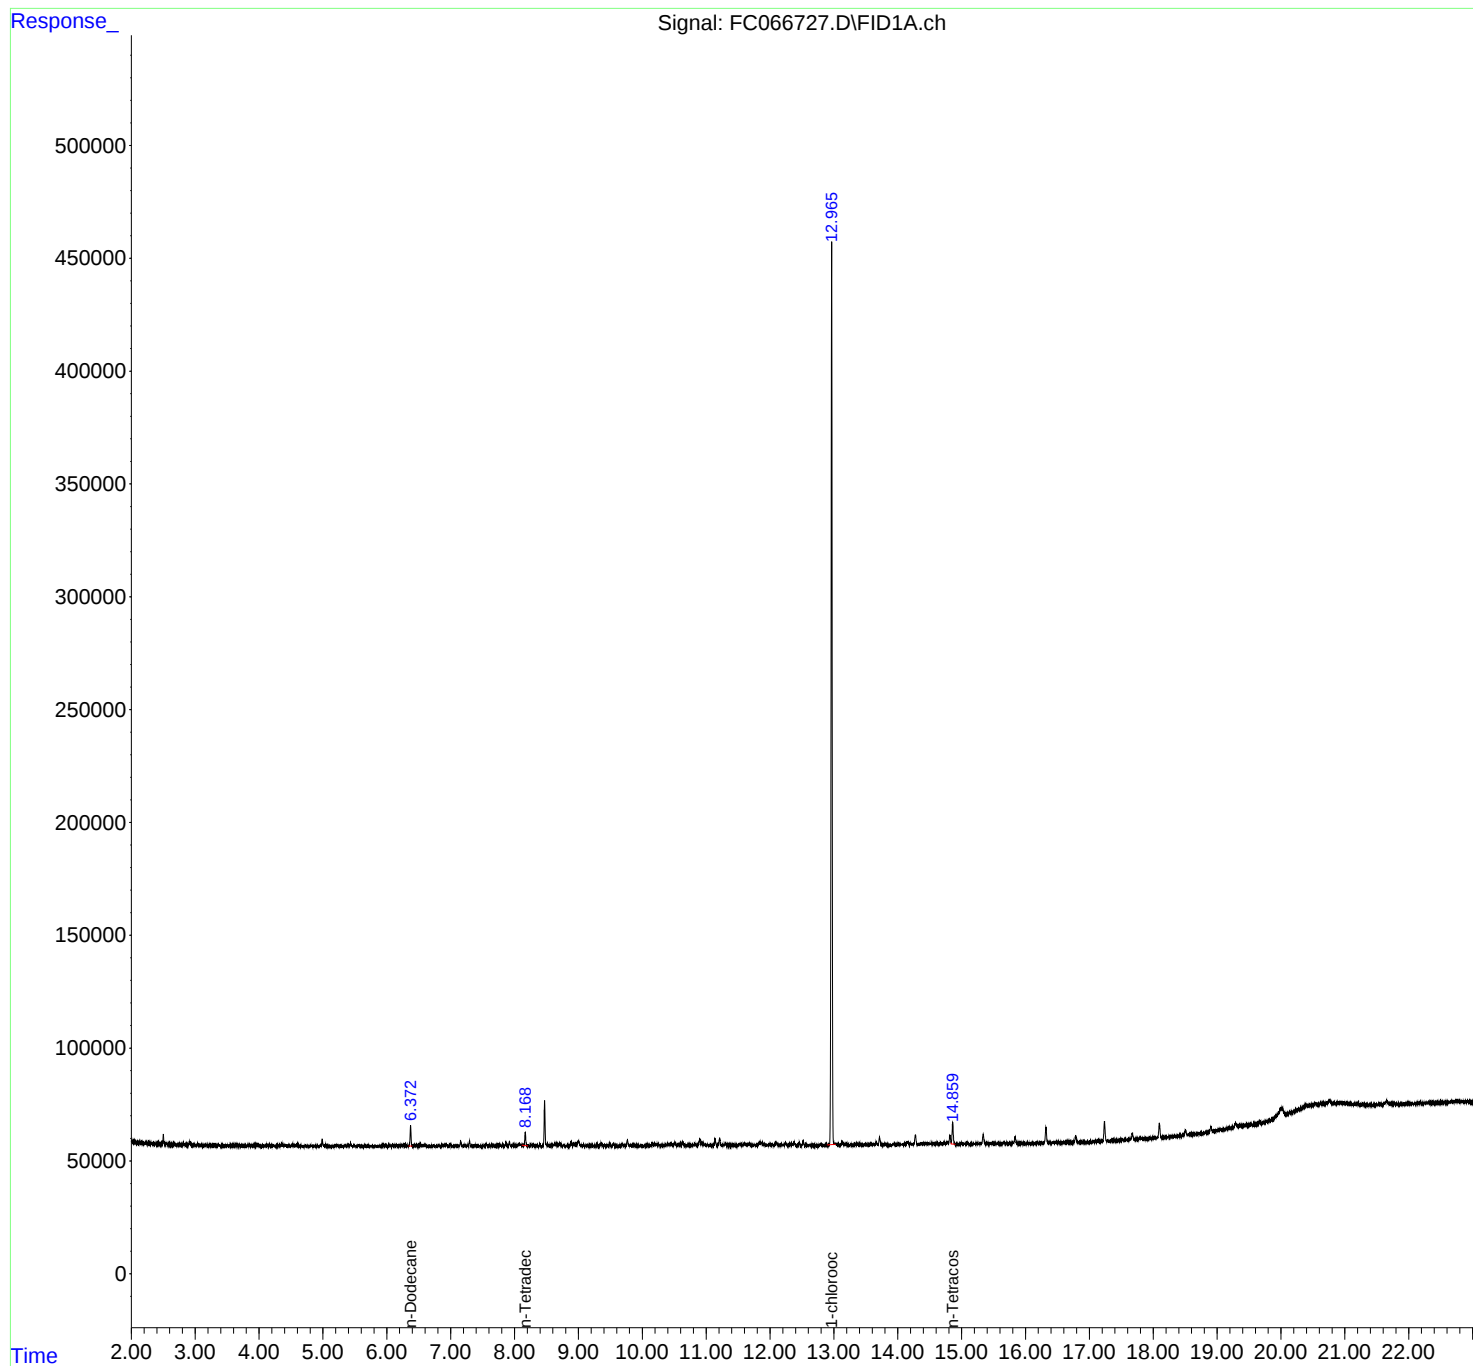


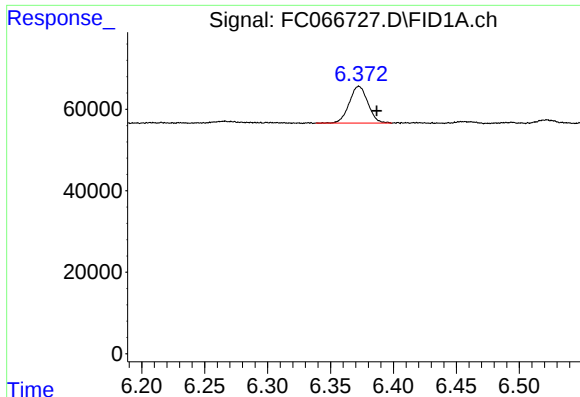

#4 n-Dodecane (C12)


R.T.: 6.373 min
Delta R.T.: -0.014 min
Response: 92834
Conc: 0.61 ug/ml

Instrument :
FID_C
ClientSampleId :

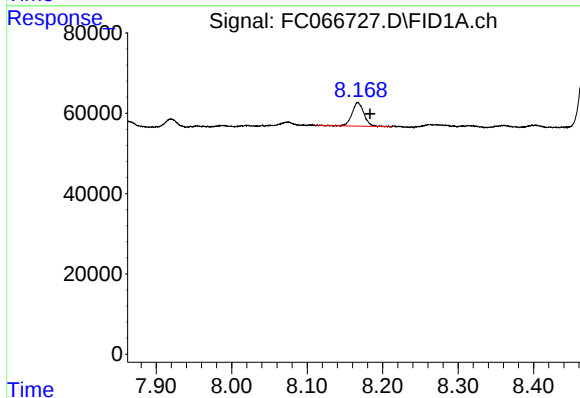


#6 n-Tetradecane (C14)

R.T.: 8.167 min
Delta R.T.: -0.016 min
Response: 64210
Conc: 0.42 ug/ml

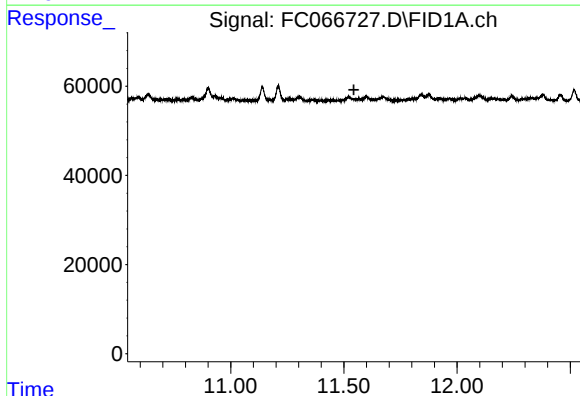


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.544 min
Response: 0
Conc: N.D.

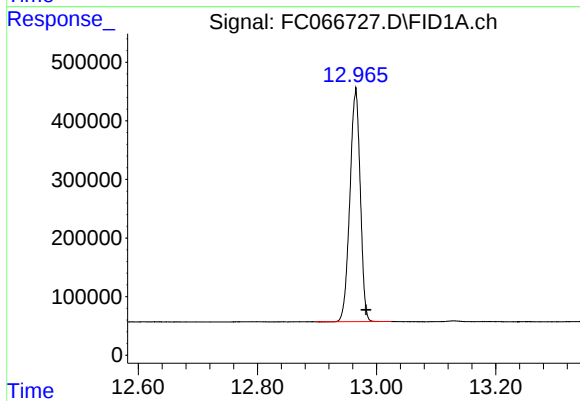

#12 1-chlorooctadecane (SURR)

R.T.: 12.965 min
Delta R.T.: -0.018 min
Response: 4798401
Conc: 34.78 ug/ml

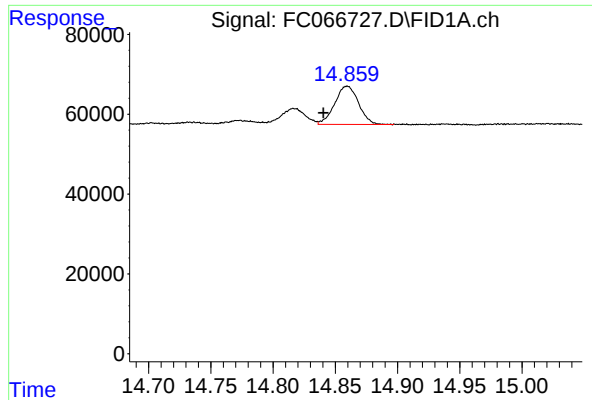

#14 n-Tetracosane (C24)

R.T.: 14.859 min
Delta R.T.: 0.019 min
Response: 127421
Conc: 0.80 ug/ml

Instrument :

FID_C

ClientSampleId :