

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC070323AL\
 Data File : FC064028.D
 Signal(s) : FID1A.ch
 Acq On : 03 Jul 2023 07:36
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 04 05:51:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 062423.M
 Quant Title : GC Extractables
 QLast Update : Sun Jun 25 04:03:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

11) T	n-Heneicosane (C21)	13.103	406199	2.535 ug/ml
13) T	n-Docosane (C22)	13.700	292968	1.864 ug/ml
14) T	n-Tetracosane (C24)	14.805	210860	1.338 ug/ml
15) T	n-Hexacosane (C26)	15.826	163137	1.080 ug/ml
16) T	n-Octacosane (C28)	16.772	154546	1.026 ug/ml
17) T	n-Tricontane (C30)	17.657	120238	0.770 ug/ml
18) T	n-Dotriacontane (C32)	18.487	301725	1.910 ug/ml
19) T	n-Tetratriacontane (C34)	19.268	270424	1.757 ug/ml
20) T	n-Hexatriacontane (C36)	20.007	113543	0.769 ug/ml
22) T	n-Tetracontane (C40)	21.677	335845	2.304 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC070323AL\
Data File : FC064028.D
Signal(s) : FID1A.ch
Acq On : 03 Jul 2023 07:36
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 04 05:51:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 062423.M
Quant Title : GC Extractables
QLast Update : Sun Jun 25 04:03:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

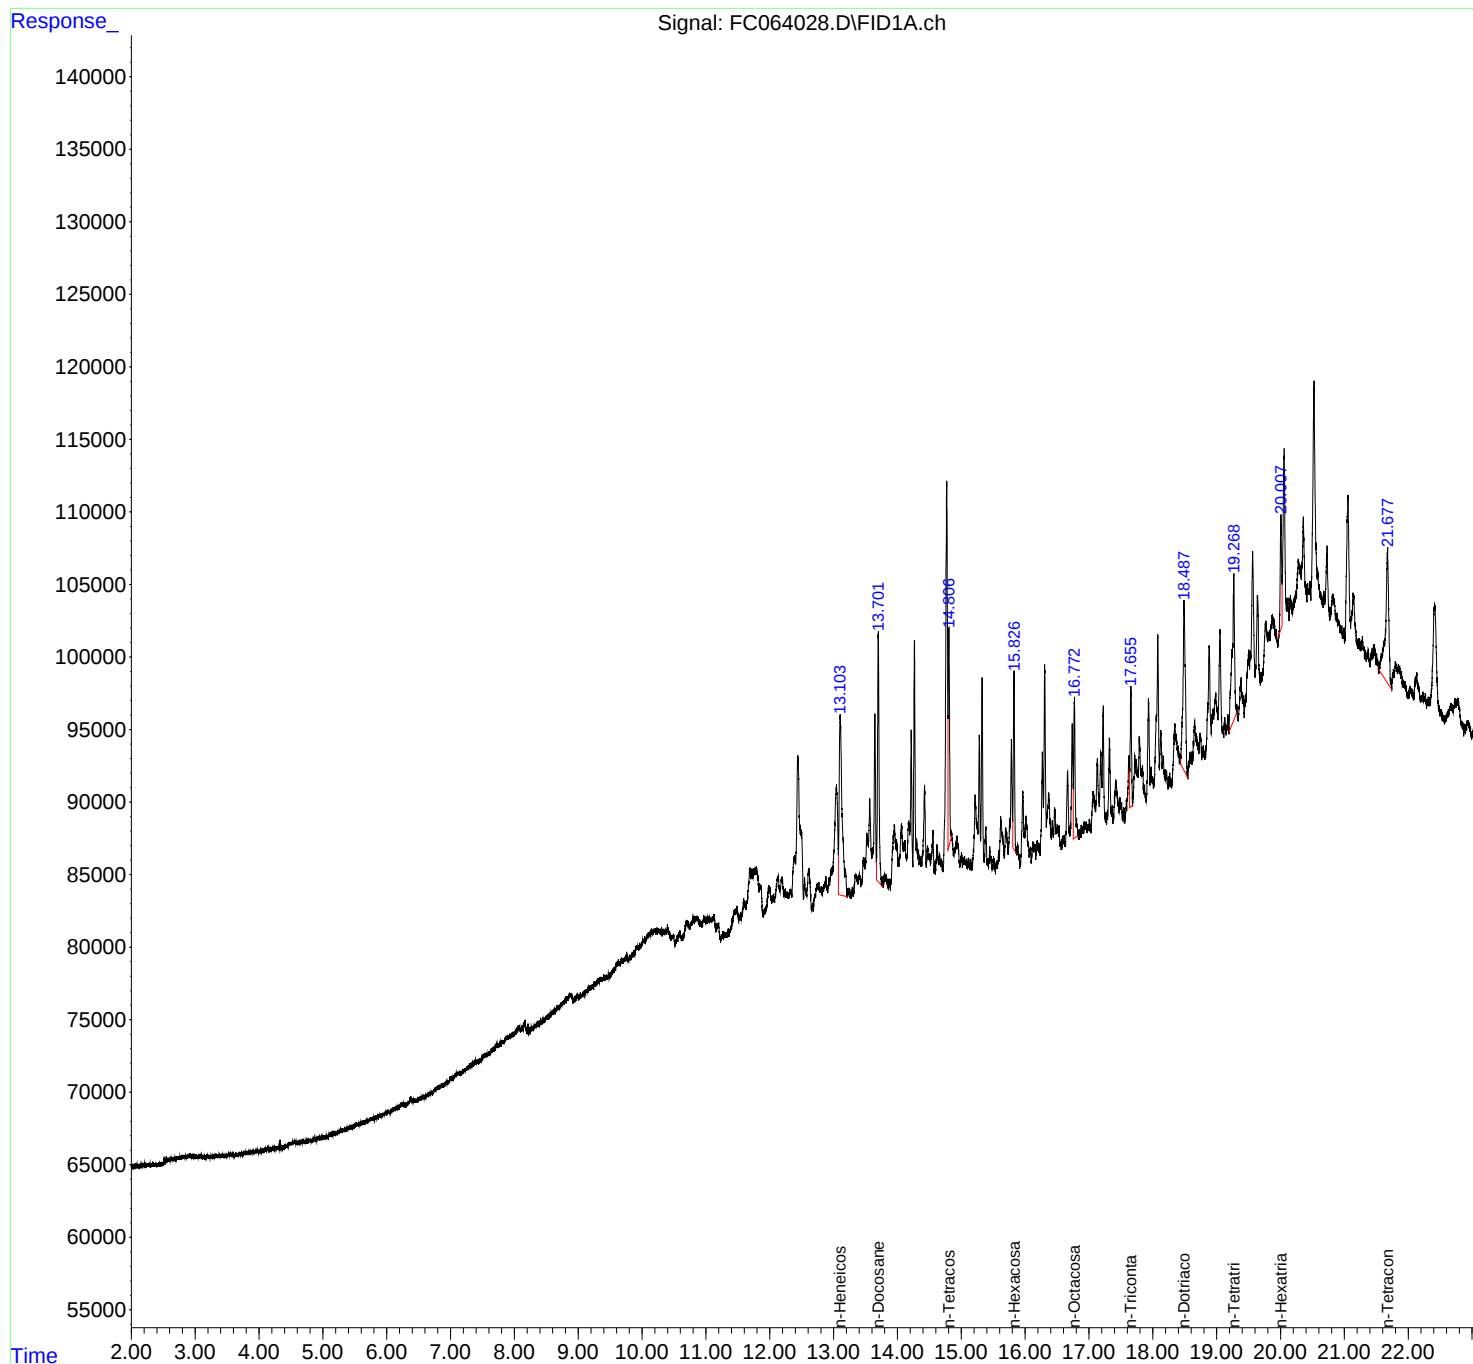


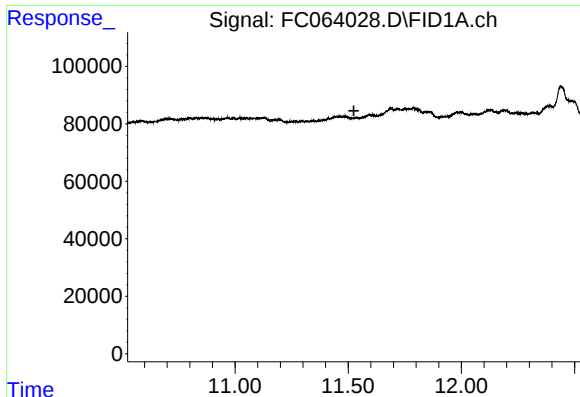

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.525 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

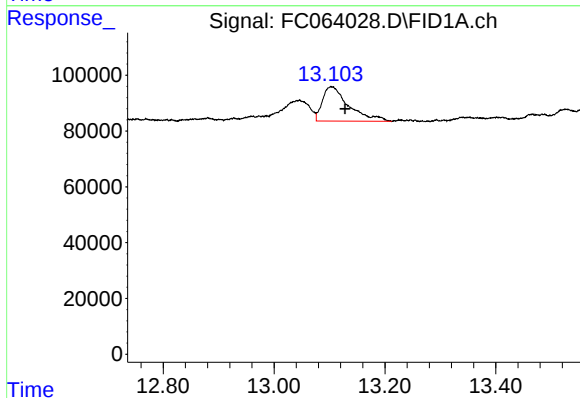


#11 n-Heneicosane (C21)

R.T.: 13.103 min
Delta R.T.: -0.025 min
Response: 406199
Conc: 2.54 ug/ml

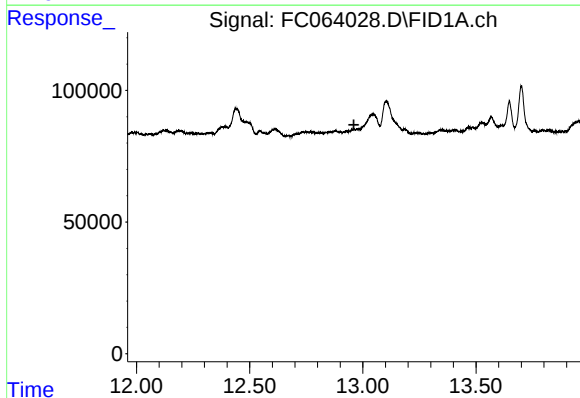


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.961 min
Response: 0
Conc: N.D.

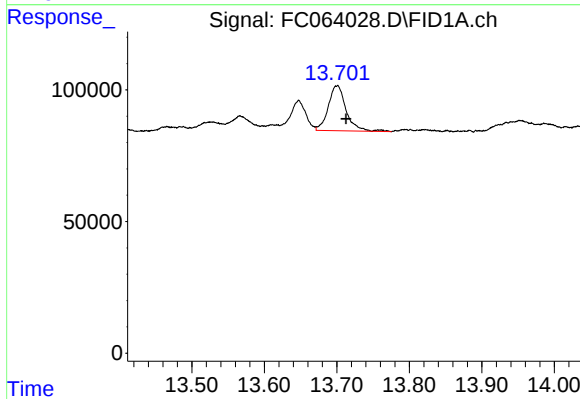

#13 n-Docosane (C22)


R.T.: 13.700 min
Delta R.T.: -0.012 min
Response: 292968
Conc: 1.86 ug/ml

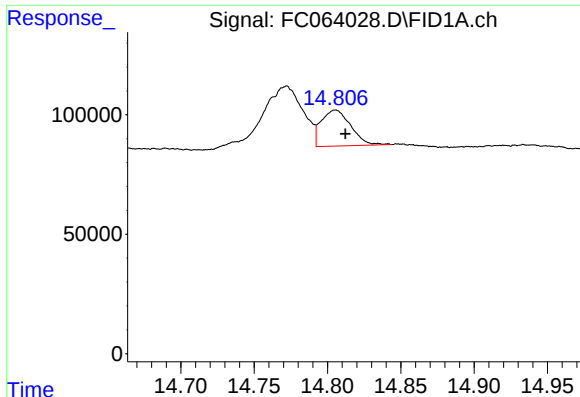

#14 n-Tetracosane (C24)


R.T.: 14.805 min
Delta R.T.: -0.007 min
Response: 210860
Conc: 1.34 ug/ml

Instrument :
FID_C
ClientSampleId :

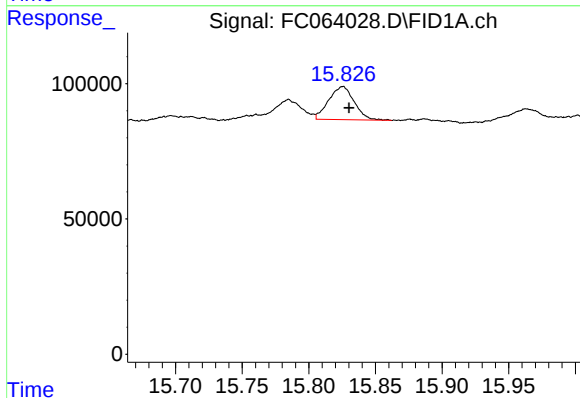


#15 n-Hexacosane (C26)

R.T.: 15.826 min
Delta R.T.: -0.005 min
Response: 163137
Conc: 1.08 ug/ml

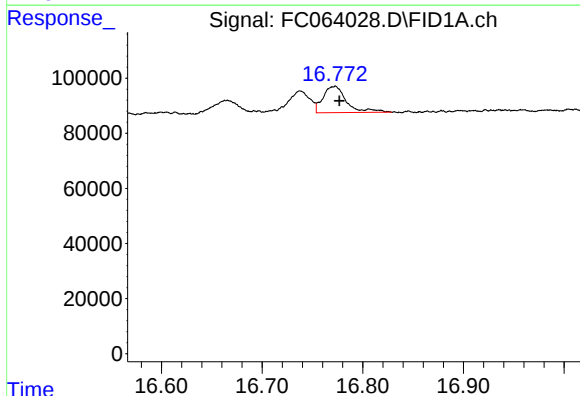


#16 n-Octacosane (C28)

R.T.: 16.772 min
Delta R.T.: -0.005 min
Response: 154546
Conc: 1.03 ug/ml

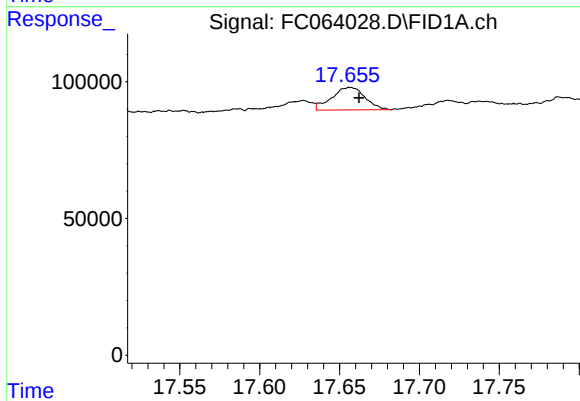

#17 n-Tricontane (C30)


R.T.: 17.657 min
Delta R.T.: -0.006 min
Response: 120238
Conc: 0.77 ug/ml

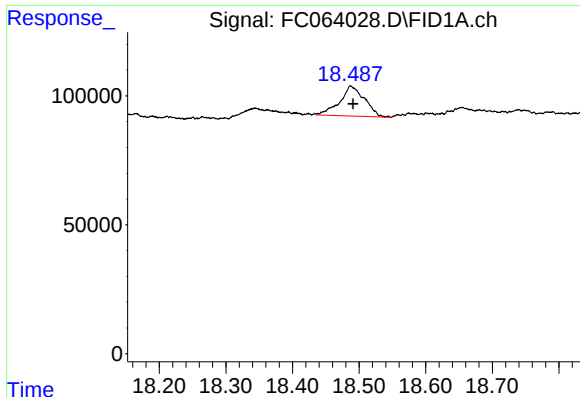

#18 n-Dotriacontane (C32)


R.T.: 18.487 min
Delta R.T.: -0.004 min
Response: 301725
Conc: 1.91 ug/ml

Instrument :
FID_C
ClientSampleId :

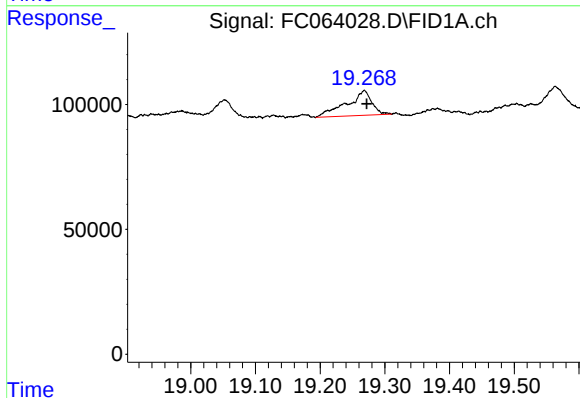


#19 n-Tetratriacontane (C34)

R.T.: 19.268 min
Delta R.T.: -0.004 min
Response: 270424
Conc: 1.76 ug/ml

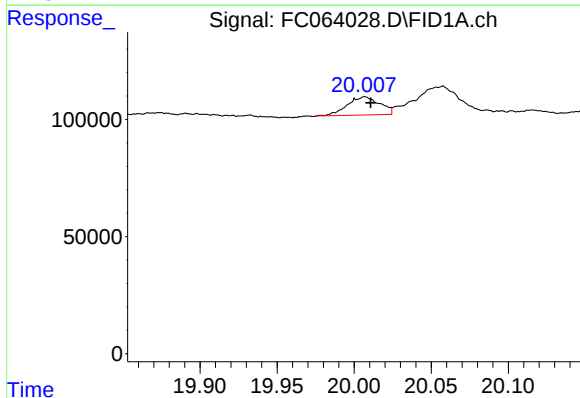

#20 n-Hexatriacontane (C36)

R.T.: 20.007 min
Delta R.T.: -0.004 min
Response: 113543
Conc: 0.77 ug/ml

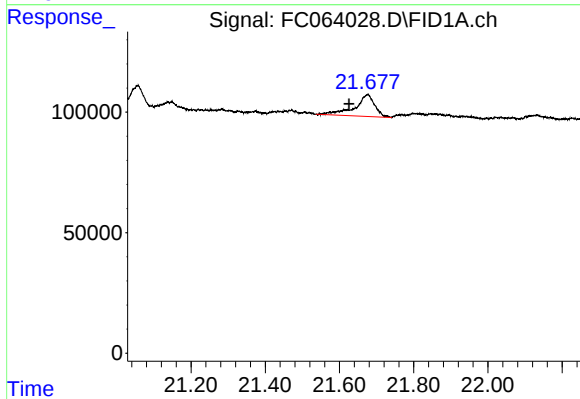

#22 n-Tetracontane (C40)

R.T.: 21.677 min
Delta R.T.: 0.051 min
Response: 335845
Conc: 2.30 ug/ml