

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071118\
Data File : FE028197.D
Signal(s) : FID1B.CH
Acq On : 11 Jul 2018 13:09
Operator : AJ\MA
Sample : J3897-03 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 11 15:11:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062618.M
Quant Title :
QLast Update : Tue Jun 26 18:10:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	15.030	401416	1.203 ug/ml
Target Compounds			
6) N-TETRADECANE	8.613	172208	0.865 ug/ml
10) N-TETRACOSANE	15.259	614701	2.166 ug/ml
11) N-OCTACOSANE	17.217	197739	0.742 ug/ml
12) N-DOTRIACONTANE	18.945	512360	2.211 ug/ml
14) N-HEXATRIACONTANE	20.475	334893	1.814 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071118\
Data File : FE028197.D
Signal(s) : FID1B.CH
Acq On : 11 Jul 2018 13:09
Operator : AJ\MA
Sample : J3897-03 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 11 15:11:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062618.M
Quant Title :
QLast Update : Tue Jun 26 18:10:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

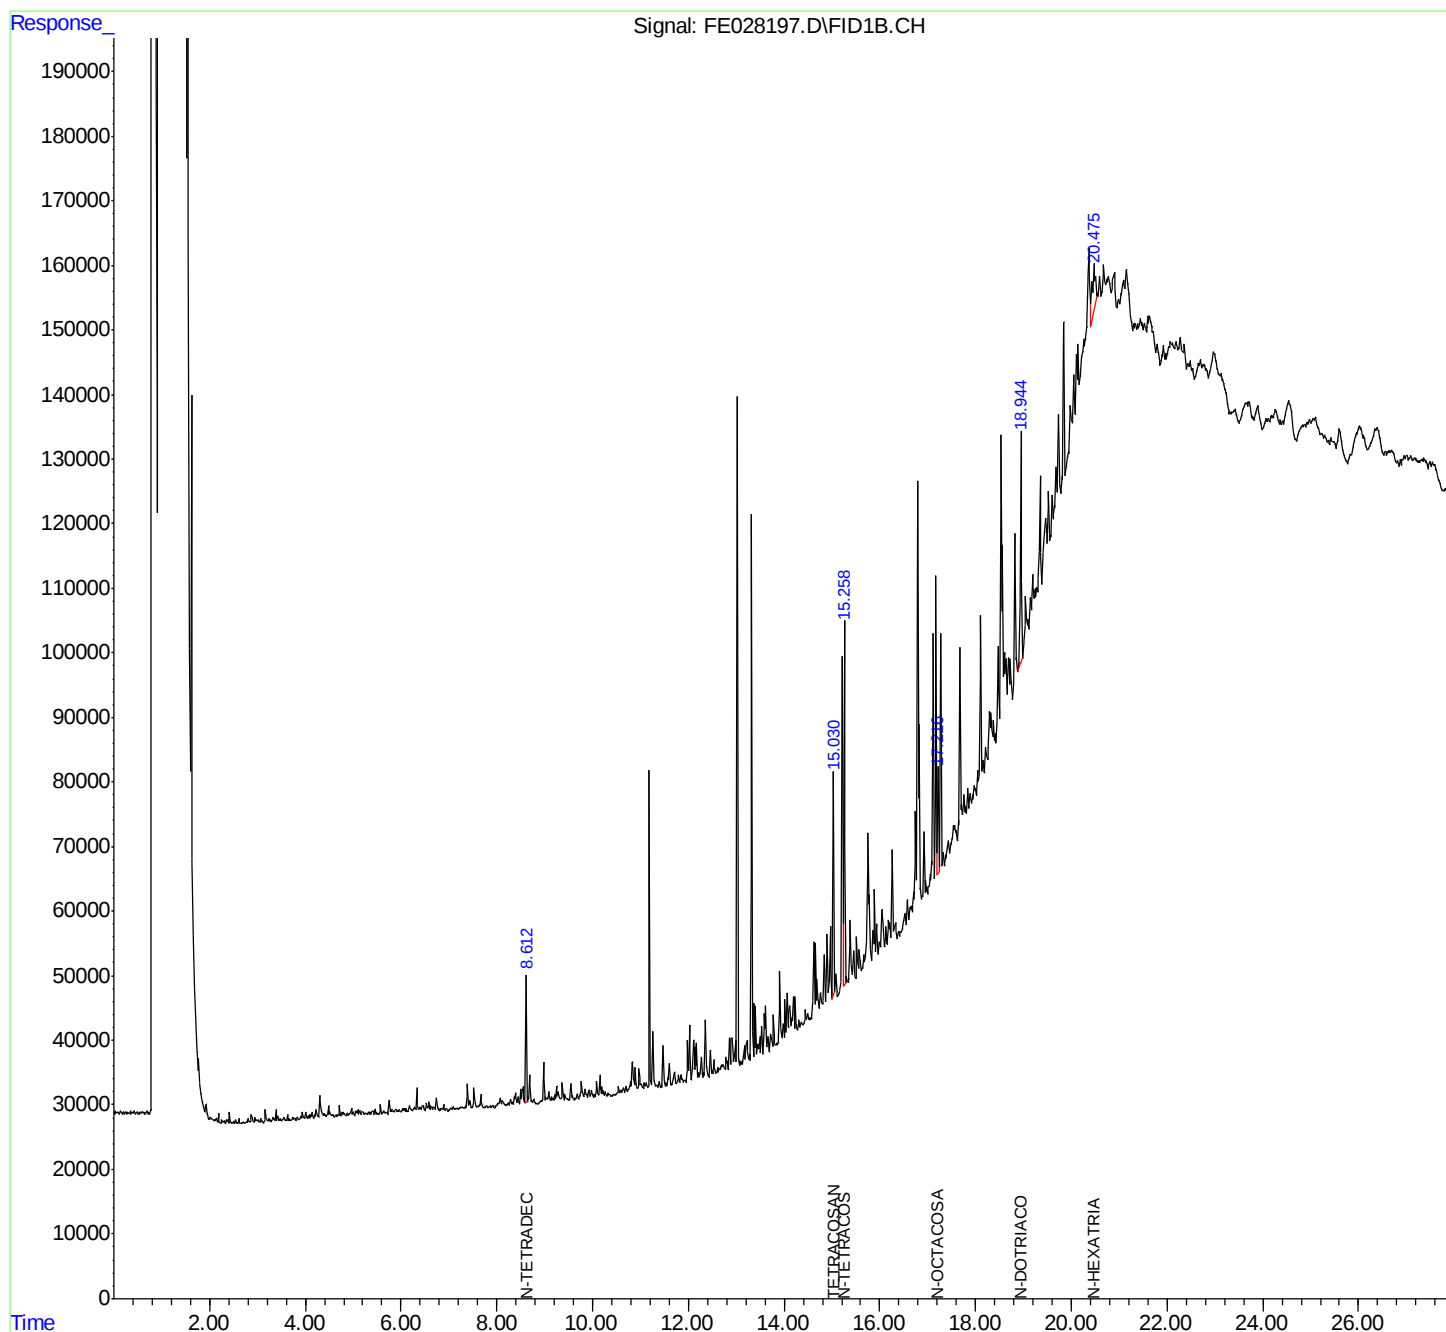

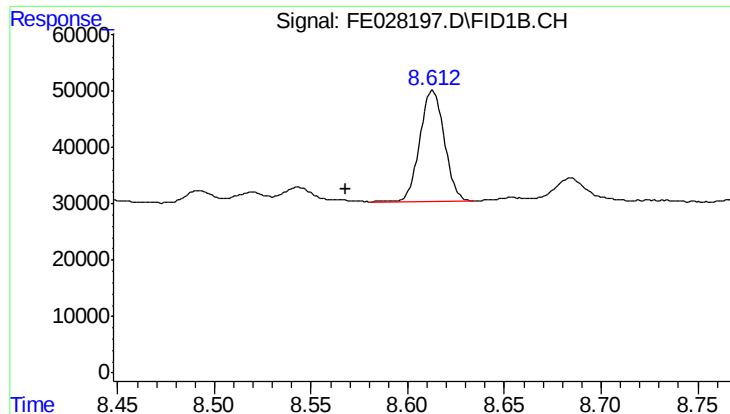


#6 N-TETRADECANE

R.T.: 8.613 min
Delta R.T.: 0.045 min
Response: 172208
Conc: 0.86 ug/ml

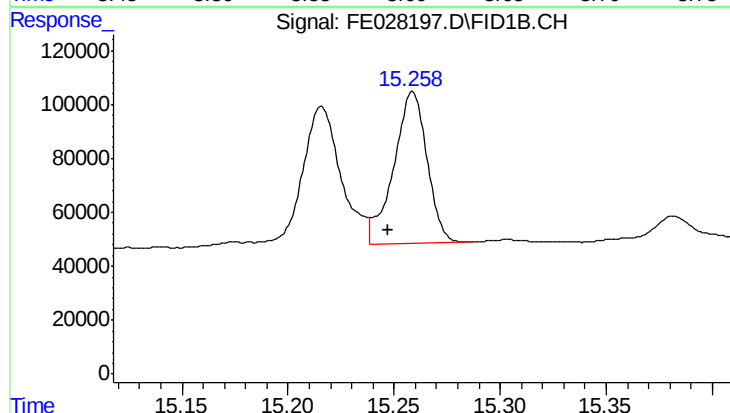


#10 N-TETRACOSANE

R.T.: 15.259 min
Delta R.T.: 0.012 min
Response: 614701
Conc: 2.17 ug/ml

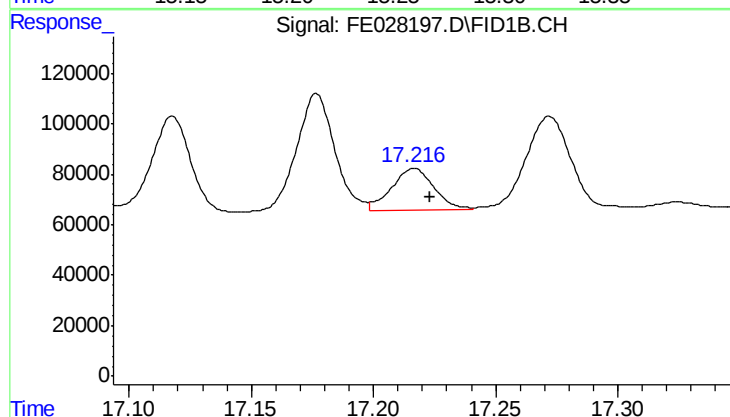


#11 N-OCTACOSANE

R.T.: 17.217 min
Delta R.T.: -0.007 min
Response: 197739
Conc: 0.74 ug/ml

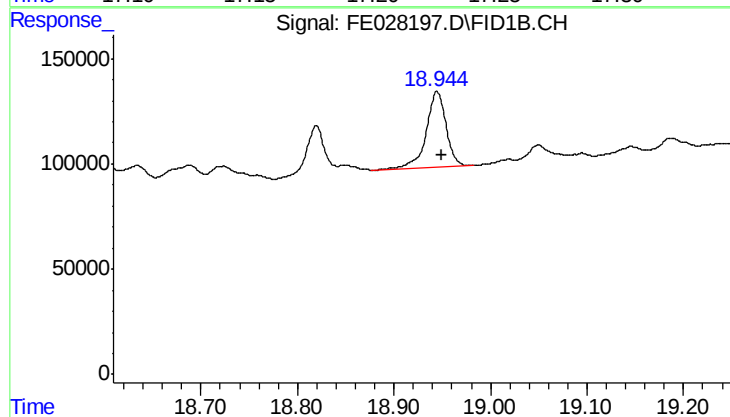


#12 N-DOTRIACONTANE

R.T.: 18.945 min
Delta R.T.: -0.005 min
Response: 512360
Conc: 2.21 ug/ml

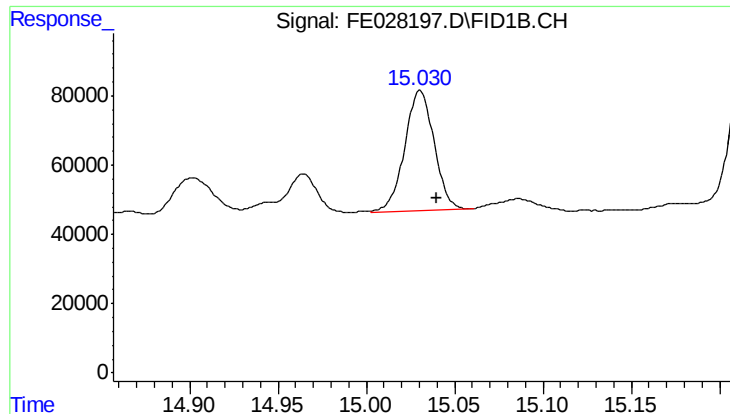

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.030 min
Delta R.T.: -0.009 min
Response: 401416
Conc: 1.20 ug/ml

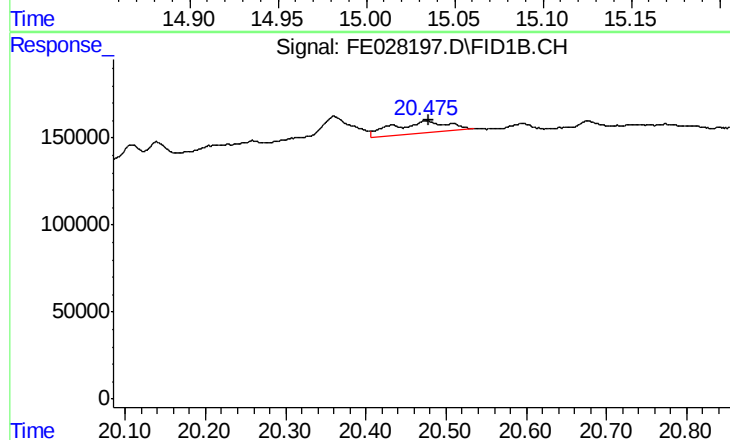

#14 N-HEXATRIACONTANE

R.T.: 20.475 min
Delta R.T.: -0.003 min
Response: 334893
Conc: 1.81 ug/ml