

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC071224AL\
 Data File : FC066773.D
 Signal(s) : FID1A.ch
 Acq On : 12 Jul 2024 06:14
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 13 01:49:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 17 13:44:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

11) T	n-Heneicosane (C21)	13.151	96960	0.602 ug/ml
14) T	n-Tetracosane (C24)	14.779f	353943	2.230 ug/ml
15) T	n-Hexacosane (C26)	15.858	387052	2.535 ug/ml
17) T	n-Tricontane (C30)	17.677	276399	1.978 ug/ml
18) T	n-Dotriacontane (C32)	18.511	79031	0.599 ug/ml
20) T	n-Hexatriacontane (C36)	20.065	193571	1.606 ug/ml
22) T	n-Tetracontane (C40)	21.632	313404	2.791 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC071224AL\
Data File : FC066773.D
Signal(s) : FID1A.ch
Acq On : 12 Jul 2024 06:14
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 01:49:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 061724.M
Quant Title : GC Extractables
QLast Update : Mon Jun 17 13:44:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

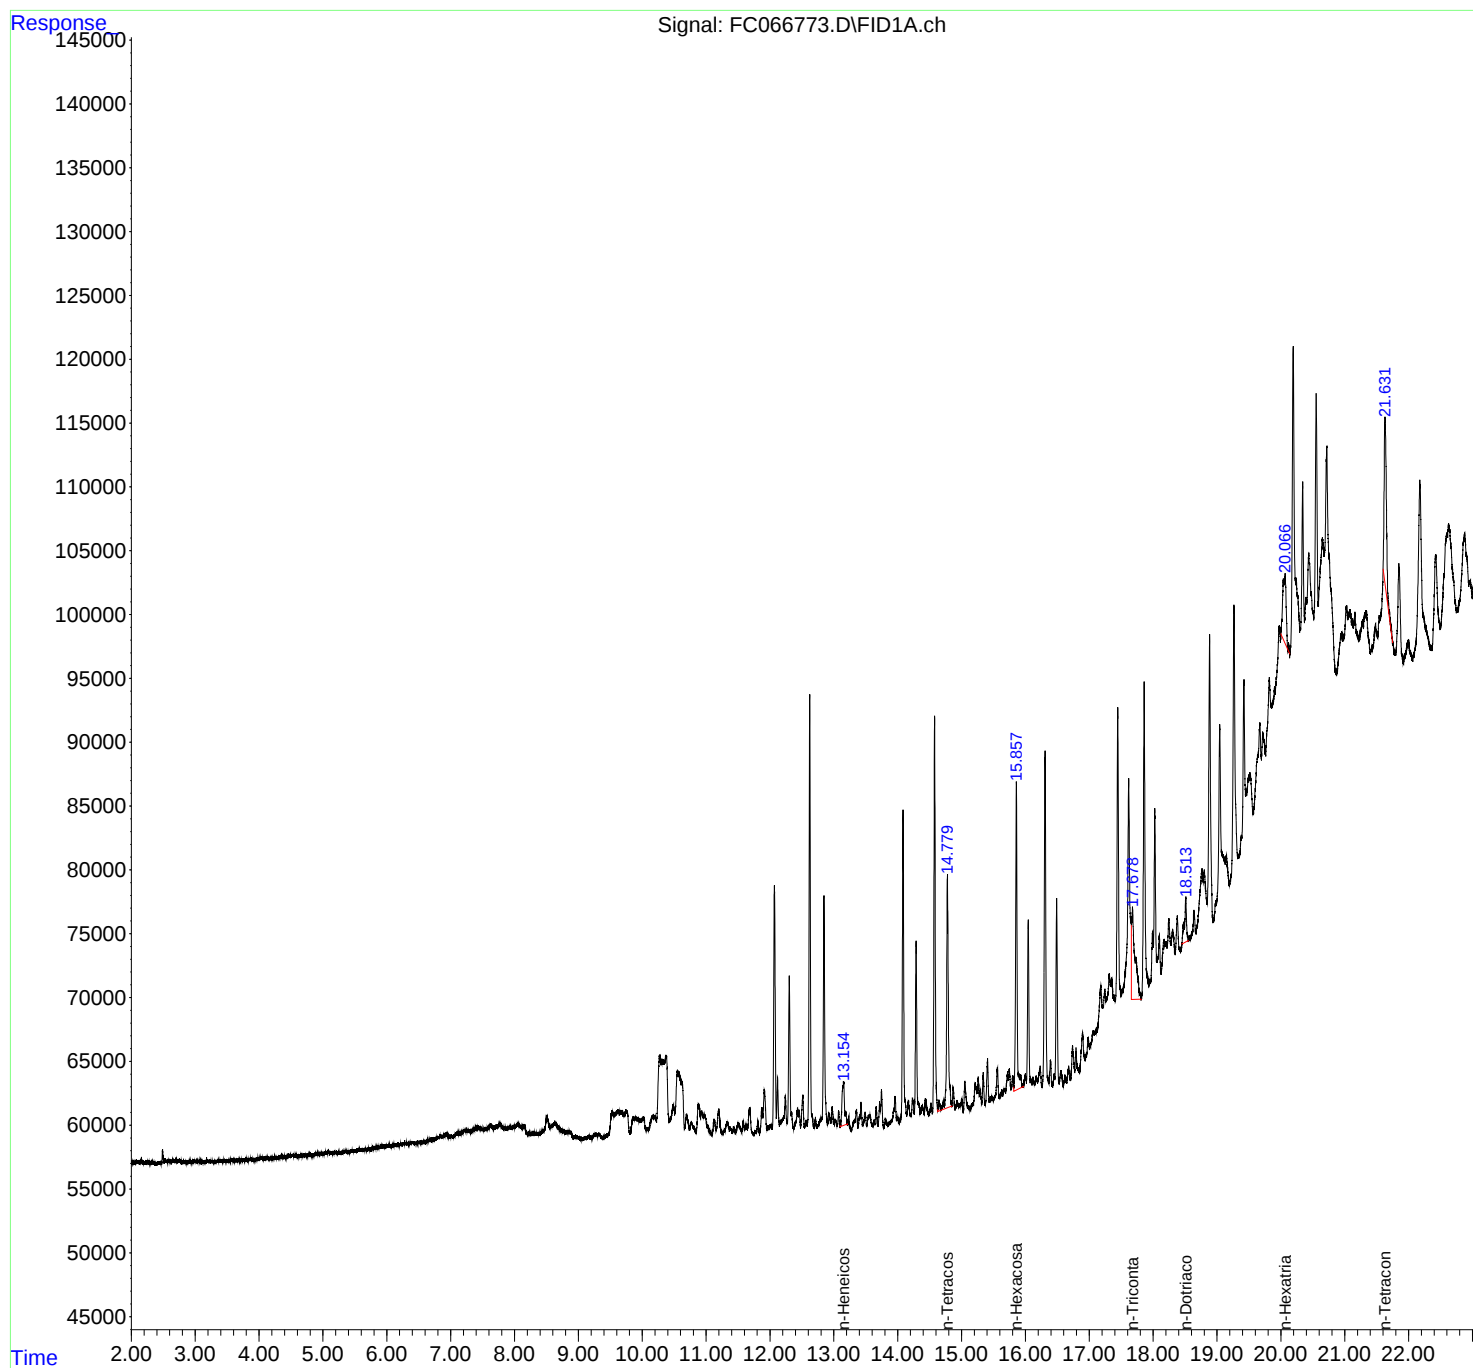


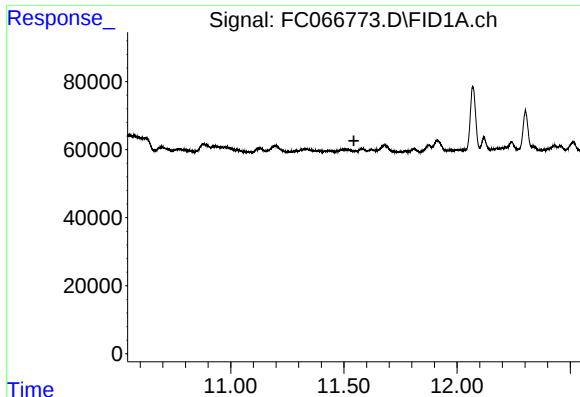

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.544 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

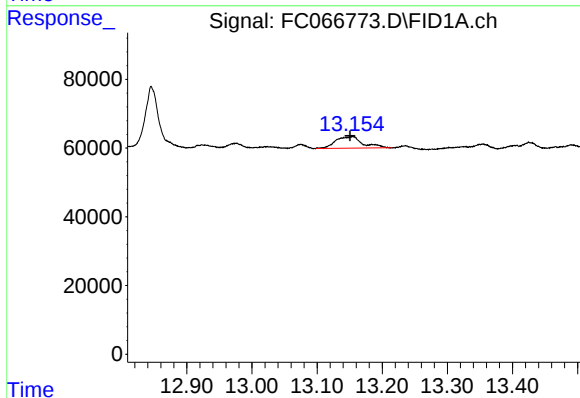


#11 n-Heneicosane (C21)

R.T.: 13.151 min
Delta R.T.: 0.000 min
Response: 96960
Conc: 0.60 ug/ml

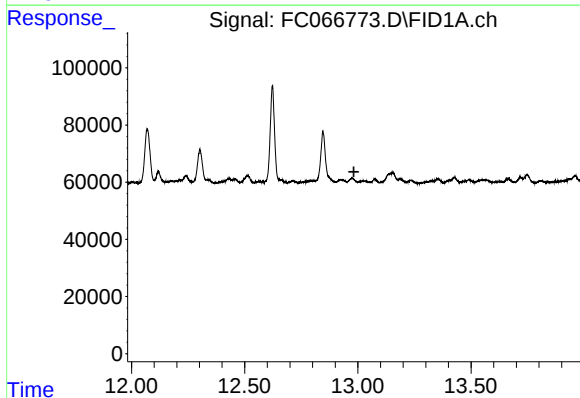


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.983 min
Response: 0
Conc: N.D.

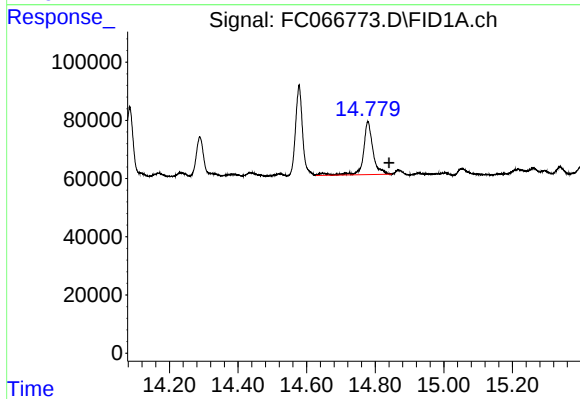

#14 n-Tetracosane (C24)


R.T.: 14.779 min
Delta R.T.: -0.061 min
Response: 353943
Conc: 2.23 ug/ml

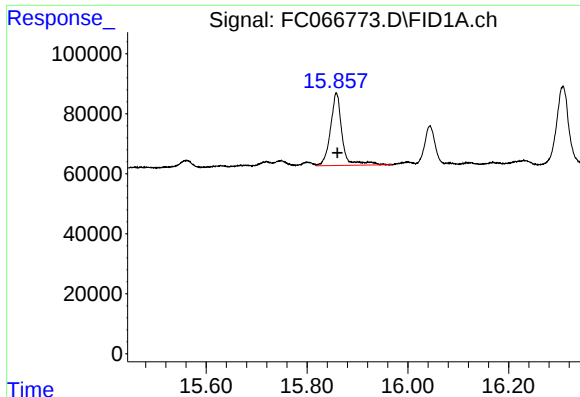

#15 n-Hexacosane (C26)


R.T.: 15.858 min
Delta R.T.: -0.003 min
Response: 387052
Conc: 2.53 ug/ml

Instrument :
FID_C
ClientSampleId :

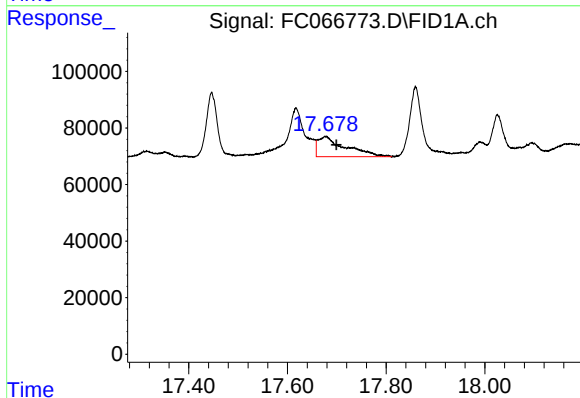


#17 n-Tricontane (C30)

R.T.: 17.677 min
Delta R.T.: -0.022 min
Response: 276399
Conc: 1.98 ug/ml

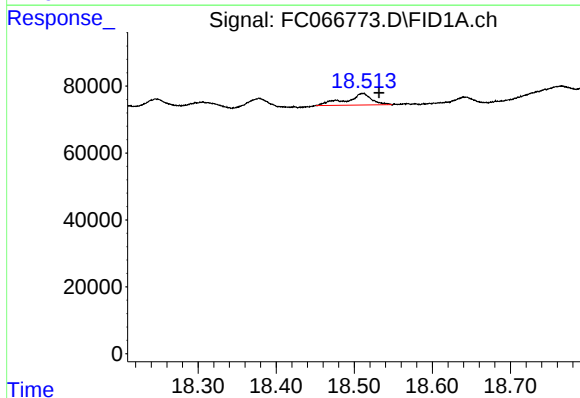


#18 n-Dotriacontane (C32)

R.T.: 18.511 min
Delta R.T.: -0.021 min
Response: 79031
Conc: 0.60 ug/ml

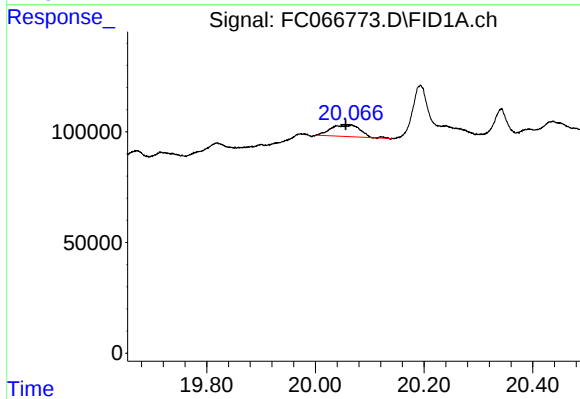

#20 n-Hexatriacontane (C36)

R.T.: 20.065 min
Delta R.T.: 0.009 min
Response: 193571
Conc: 1.61 ug/ml

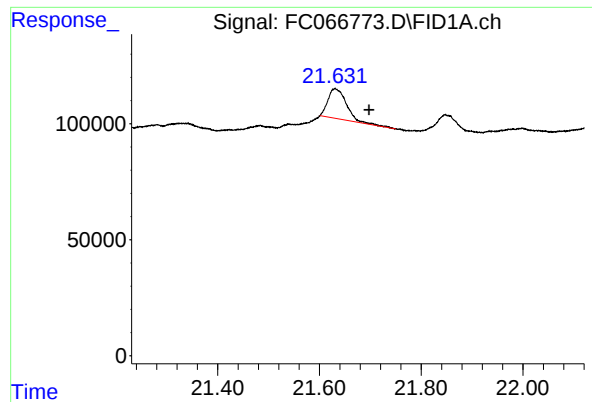

#22 n-Tetracontane (C40)

R.T.: 21.632 min
Delta R.T.: -0.065 min
Response: 313404
Conc: 2.79 ug/ml

Instrument :

FID_C

ClientSampleId :