

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC071724AL\
Data File : FC066825.D
Signal(s) : FID1A.ch
Acq On : 17 Jul 2024 06:47
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 18 01:36:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 071524.M
Quant Title : GC Extractables
QLast Update : Mon Jul 15 13:58:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.503	102808	0.817 ug/ml
19) T	n-Tetratriacontane (C34)	19.285	77915	0.630 ug/ml
20) T	n-Hexatriacontane (C36)	20.077	66941	0.575 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC071724AL\
Data File : FC066825.D
Signal(s) : FID1A.ch
Acq On : 17 Jul 2024 06:47
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 18 01:36:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 071524.M
Quant Title : GC Extractables
QLast Update : Mon Jul 15 13:58:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

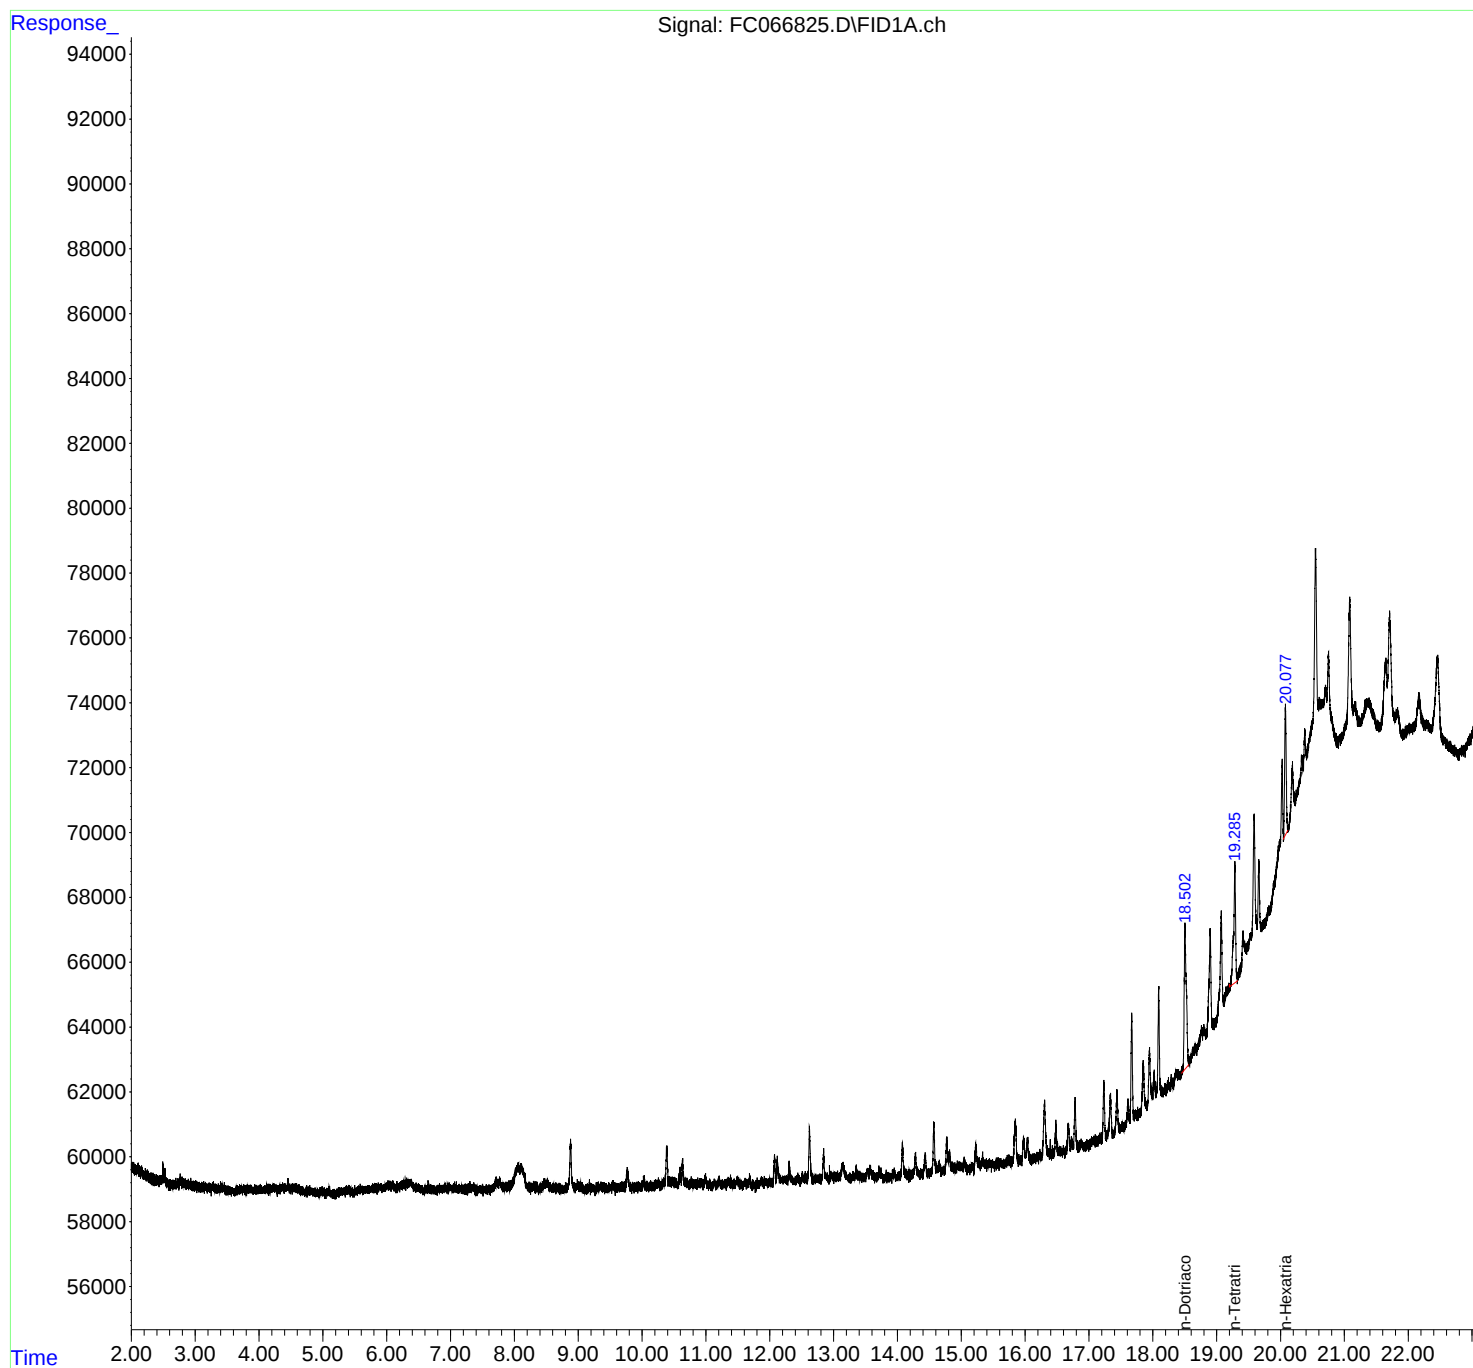


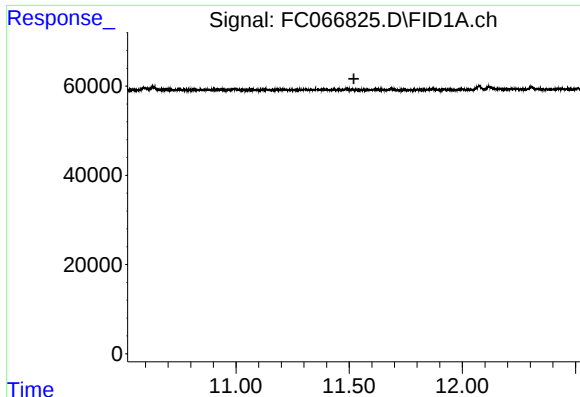

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.521 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

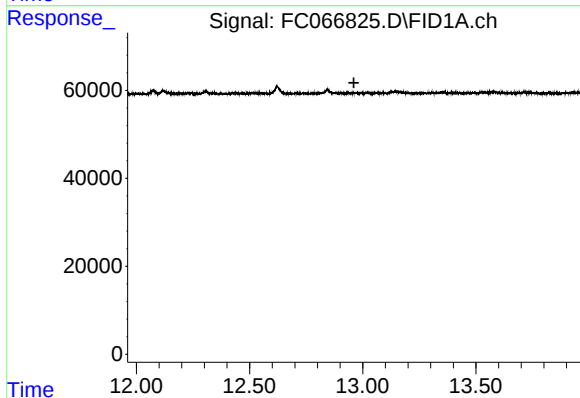


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 12.961 min
Response: 0
Conc: N.D.

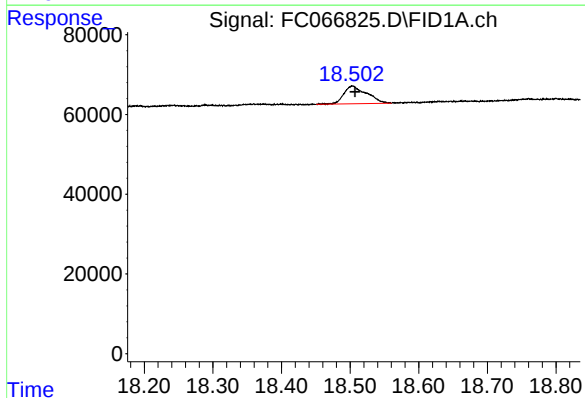


#18 n-Dotriacontane (C32)

R.T.: 18.503 min
Delta R.T.: -0.004 min
Response: 102808
Conc: 0.82 ug/ml

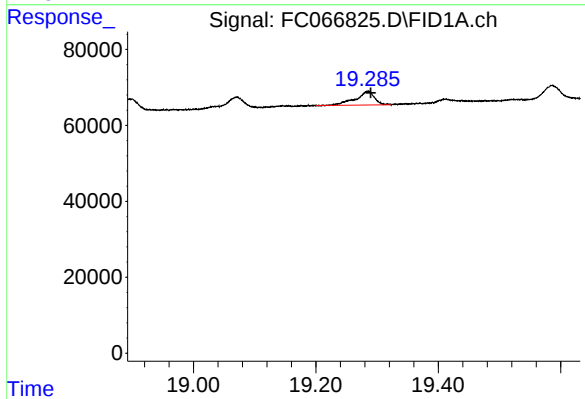

#19 n-Tetratriacontane (C34)

R.T.: 19.285 min
Delta R.T.: -0.005 min
Response: 77915
Conc: 0.63 ug/ml

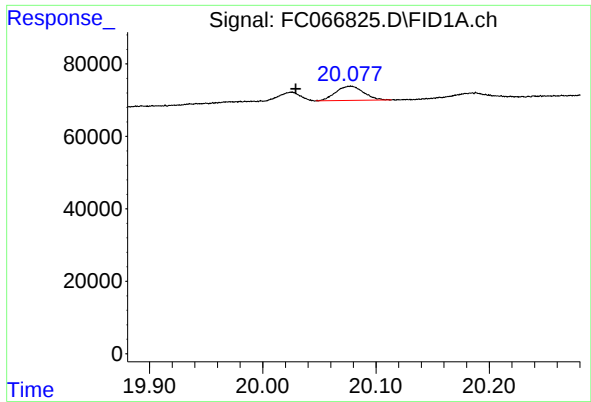

#20 n-Hexatriacontane (C36)

R.T.: 20.077 min
Delta R.T.: 0.048 min
Response: 66941
Conc: 0.58 ug/ml

Instrument :
FID_C
ClientSampleId :