

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC072120AL\
 Data File : FC048558.D
 Signal(s) : FID1A.CH
 Acq On : 21 Jul 2020 13:38
 Operator : DD\AJ
 Sample : L3177-03D
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 AU-05-071720-1

Integration File: autoint1.e
 Quant Time: Jul 22 02:05:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 070820.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 03:03:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.115	4076810	36.178 ug/ml
Spiked Amount 50.000		Recovery =	72.36%
Target Compounds			
4) T n-Dodecane (C12)	6.514	94354	0.771 ug/ml
6) T n-Tetradecane (C14)	8.311	66488	0.540 ug/ml
17) T n-Tricontane (C30)	17.819	117946	0.917 ug/ml
18) T n-Dotriacontane (C32)	18.652	102877	0.871 ug/ml
19) T n-Tetratriacontane (C34)	19.433	155506	1.393 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC072120AL\
Data File : FC048558.D
Signal(s) : FID1A.CH
Acq On : 21 Jul 2020 13:38
Operator : DD\AJ
Sample : L3177-03D
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
AU-05-071720-1

Integration File: autoint1.e
Quant Time: Jul 22 02:05:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 070820.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 03:03:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

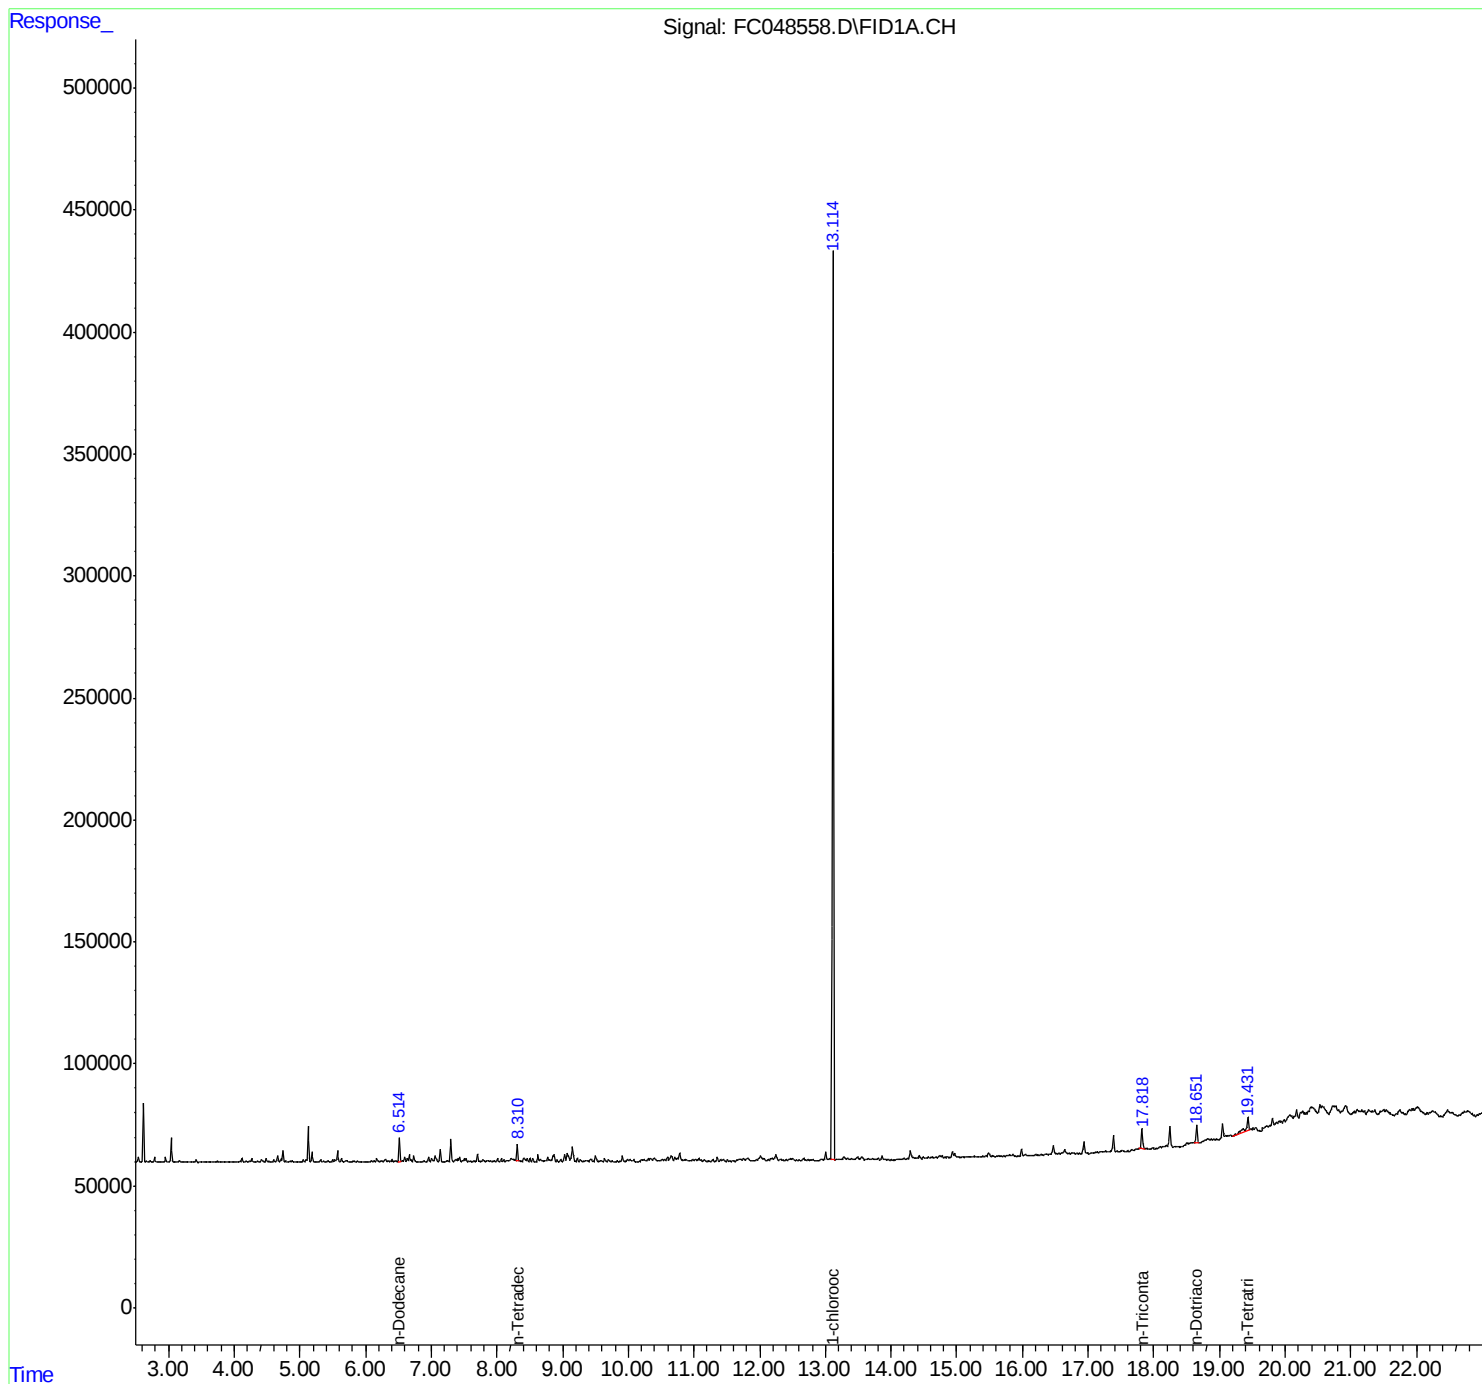


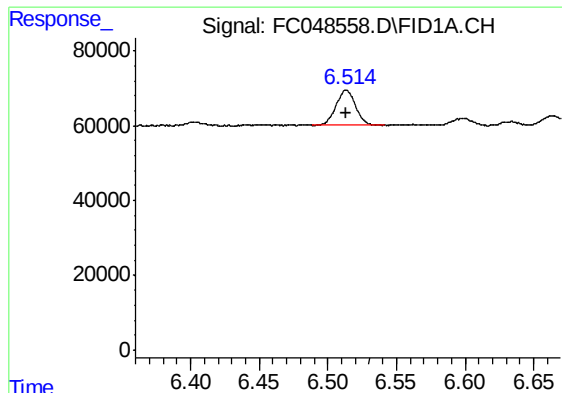

#4 n-Dodecane (C12)


R.T.: 6.514 min
Delta R.T.: 0.000 min
Response: 94354
Conc: 0.77 ug/ml

Instrument :
FID_C
ClientSampleId :
AU-05-071720-1

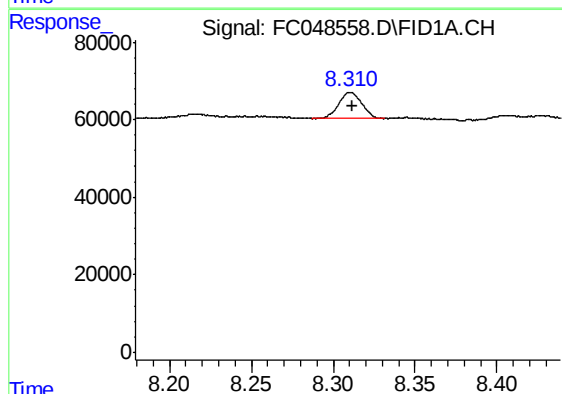


#6 n-Tetradecane (C14)

R.T.: 8.311 min
Delta R.T.: 0.000 min
Response: 66488
Conc: 0.54 ug/ml

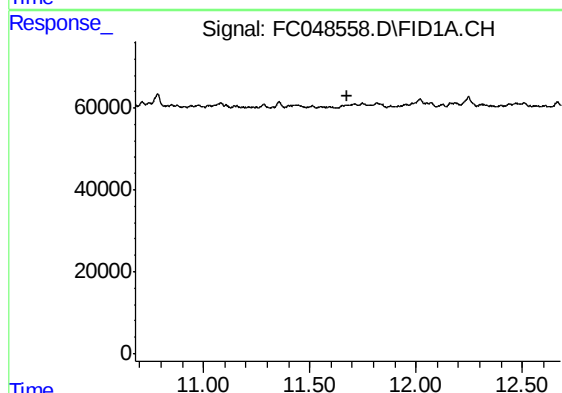


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.680 min
Response: 0
Conc: N.D.

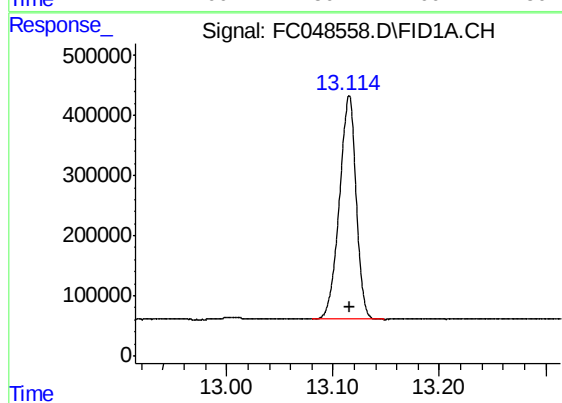

#12 1-chlorooctadecane (SURR)


R.T.: 13.115 min
Delta R.T.: 0.000 min
Response: 4076810
Conc: 36.18 ug/ml

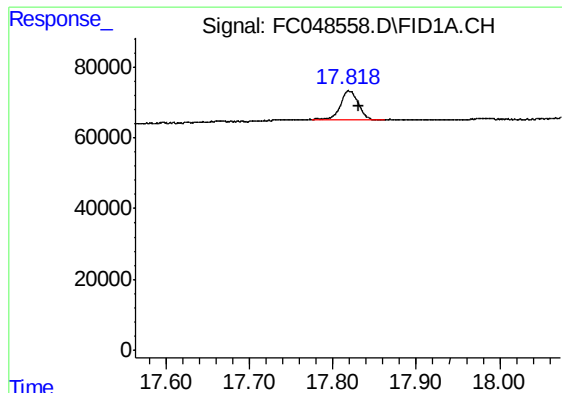

#17 n-Tricontane (C30)


R.T.: 17.819 min
Delta R.T.: -0.012 min
Response: 117946
Conc: 0.92 ug/ml

Instrument :
FID_C
ClientSampleId :
AU-05-071720-1

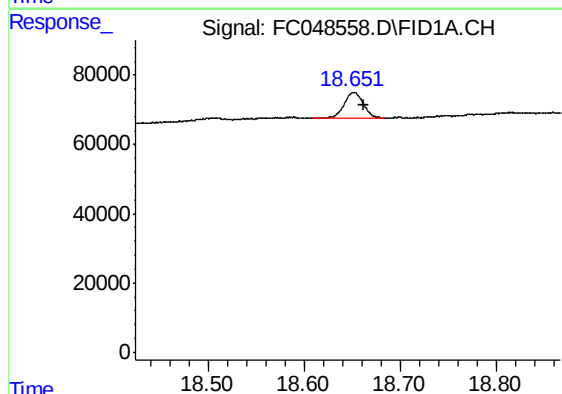

#18 n-Dotriacontane (C32)

R.T.: 18.652 min
Delta R.T.: -0.011 min
Response: 102877
Conc: 0.87 ug/ml

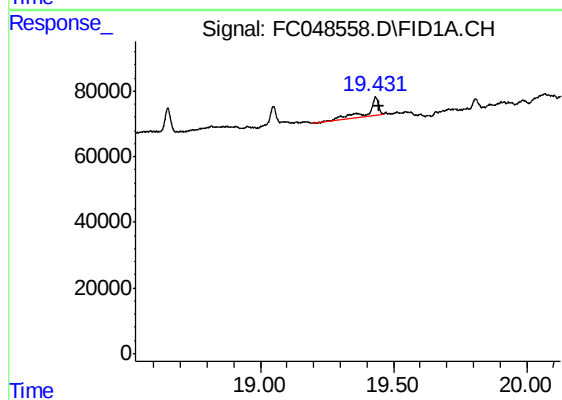

#19 n-Tetratriacontane (C34)

R.T.: 19.433 min
Delta R.T.: -0.014 min
Response: 155506
Conc: 1.39 ug/ml