

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC072325AL\
 Data File : FC069506.D
 Signal(s) : FID1A.ch
 Acq On : 23 Jul 2025 12:58
 Operator : YP/AJ
 Sample : Q2633-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 FIBER-GLASS-TANK

Integration File: autoint1.e
 Quant Time: Jul 24 01:27:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 071525.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 15 12:35:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.102	4565958	40.403 ug/ml
Spiked Amount 50.000		Recovery =	80.81%
Target Compounds			
4) T n-Dodecane (C12)	6.496	40960	0.289 ug/ml
6) T n-Tetradecane (C14)	8.294	62138	0.437 ug/ml
17) T n-Tricontane (C30)	17.817	46237	0.422 ug/ml
18) T n-Dotriacontane (C32)	18.650	73394	0.707 ug/ml
19) T n-Tetratriacontane (C34)	19.434	62708	0.665 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC072325AL\
Data File : FC069506.D
Signal(s) : FID1A.ch
Acq On : 23 Jul 2025 12:58
Operator : YP/AJ
Sample : Q2633-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
FIBER-GLASS-TANK

Integration File: autoint1.e
Quant Time: Jul 24 01:27:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 071525.M
Quant Title : GC Extractables
QLast Update : Tue Jul 15 12:35:59 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

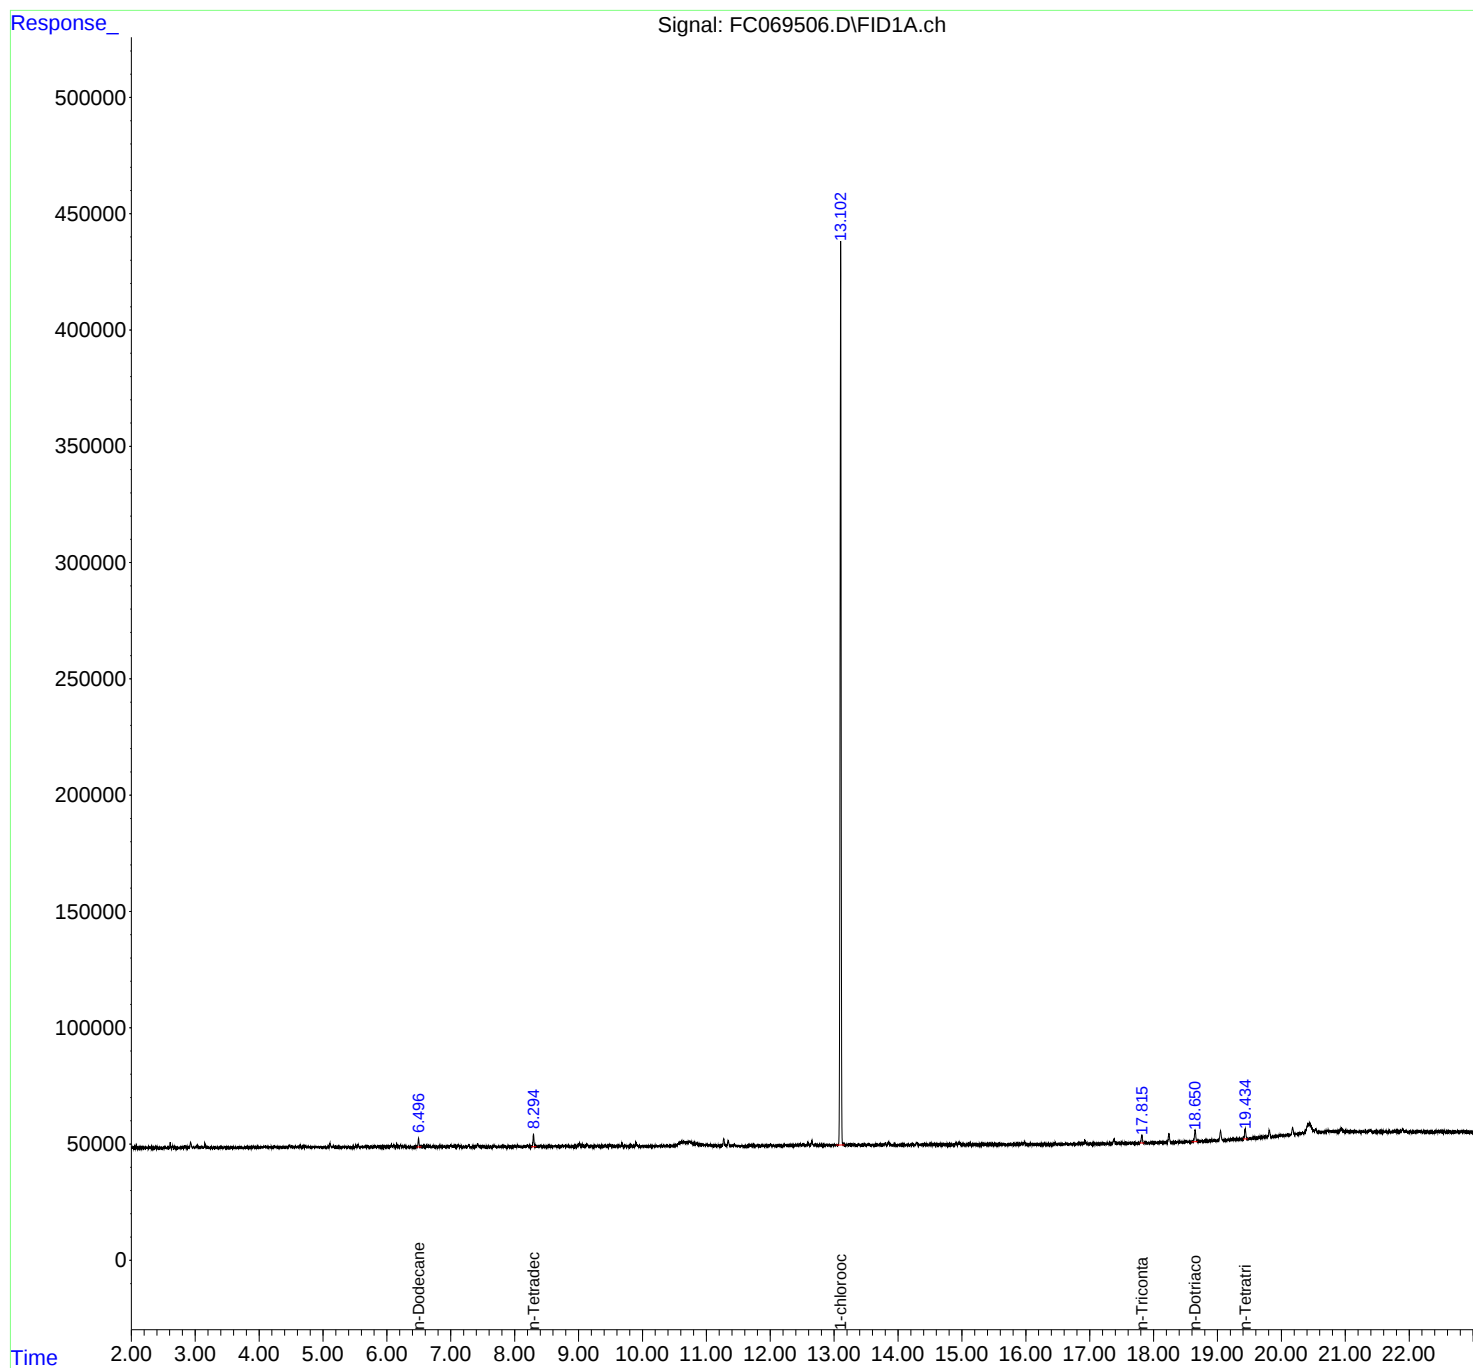


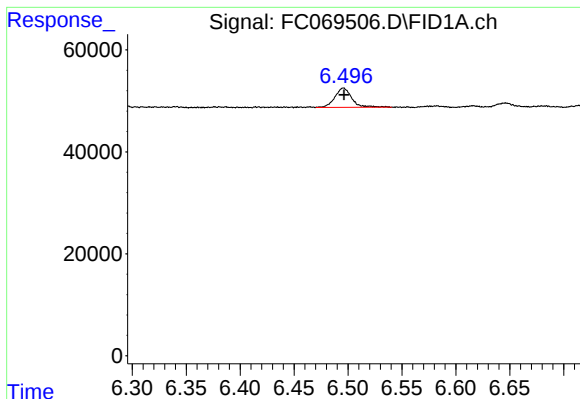

#4 n-Dodecane (C12)


R.T.: 6.496 min
Delta R.T.: 0.000 min
Response: 40960
Conc: 0.29 ug/ml

Instrument :
FID_C
ClientSampleId :
FIBER-GLASS-TANK

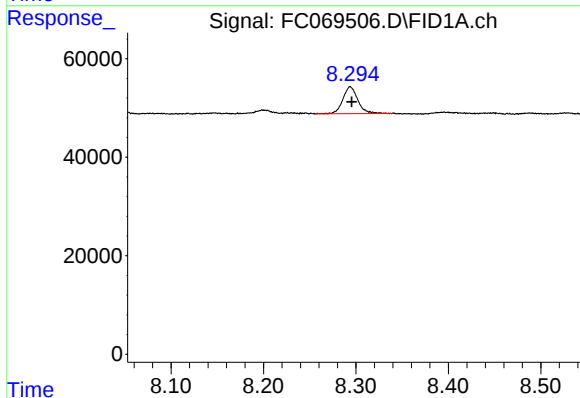


#6 n-Tetradecane (C14)

R.T.: 8.294 min
Delta R.T.: -0.001 min
Response: 62138
Conc: 0.44 ug/ml

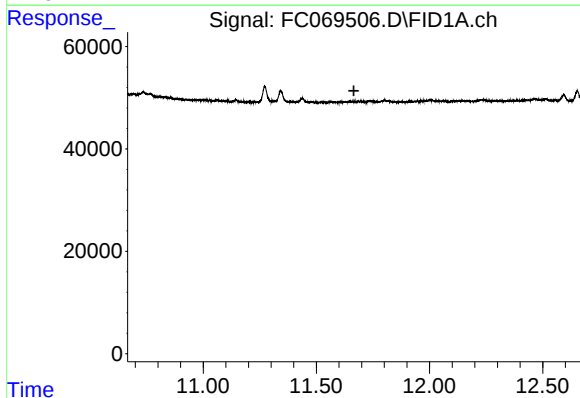


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.666 min
Response: 0
Conc: N.D.

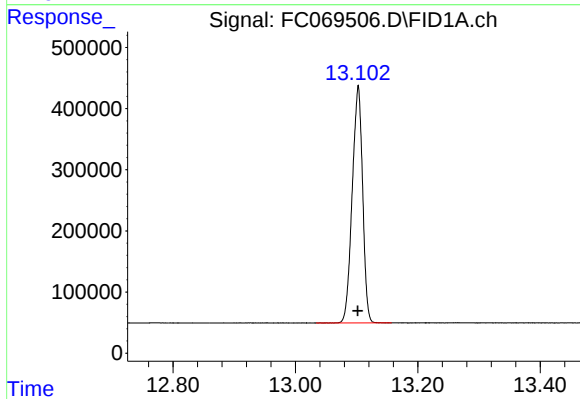

#12 1-chlorooctadecane (SURR)


R.T.: 13.102 min
Delta R.T.: 0.000 min
Response: 4565958
Conc: 40.40 ug/ml

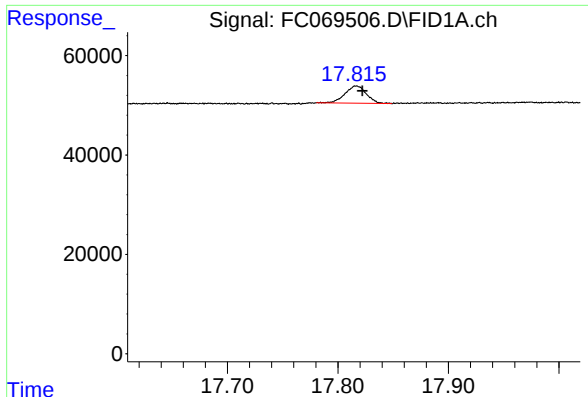

#17 n-Tricontane (C30)


R.T.: 17.817 min
Delta R.T.: -0.005 min
Response: 46237
Conc: 0.42 ug/ml

Instrument :
FID_C
ClientSampleId :
FIBER-GLASS-TANK

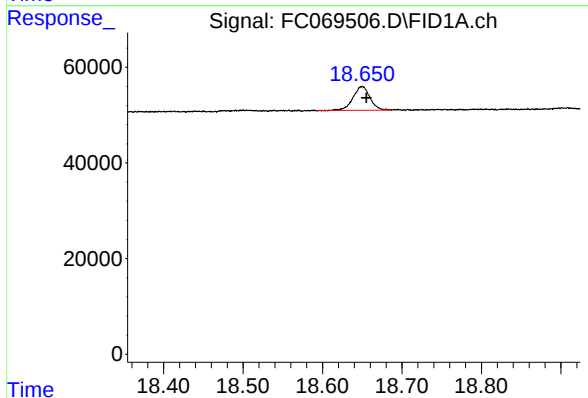

#18 n-Dotriacontane (C32)

R.T.: 18.650 min
Delta R.T.: -0.006 min
Response: 73394
Conc: 0.71 ug/ml

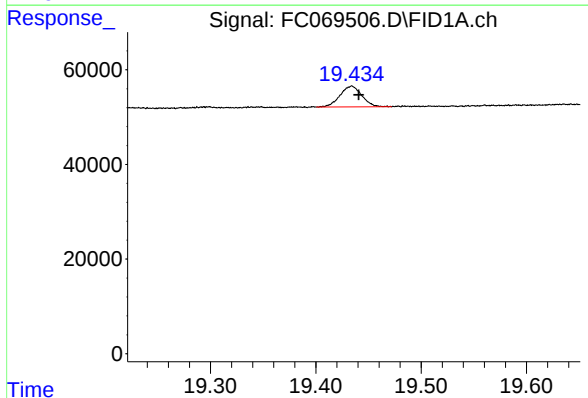

#19 n-Tetratriacontane (C34)

R.T.: 19.434 min
Delta R.T.: -0.007 min
Response: 62708
Conc: 0.67 ug/ml