

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC072423AL\
Data File : FC064246.D
Signal(s) : FID1A.ch
Acq On : 24 Jul 2023 07:59
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 25 03:24:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 072323.M
Quant Title : GC Extractables
QLast Update : Mon Jul 24 01:54:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T n-Tetracosane (C24)	14.769	69816	0.497 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC072423AL\
Data File : FC064246.D
Signal(s) : FID1A.ch
Acq On : 24 Jul 2023 07:59
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 25 03:24:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 072323.M
Quant Title : GC Extractables
QLast Update : Mon Jul 24 01:54:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

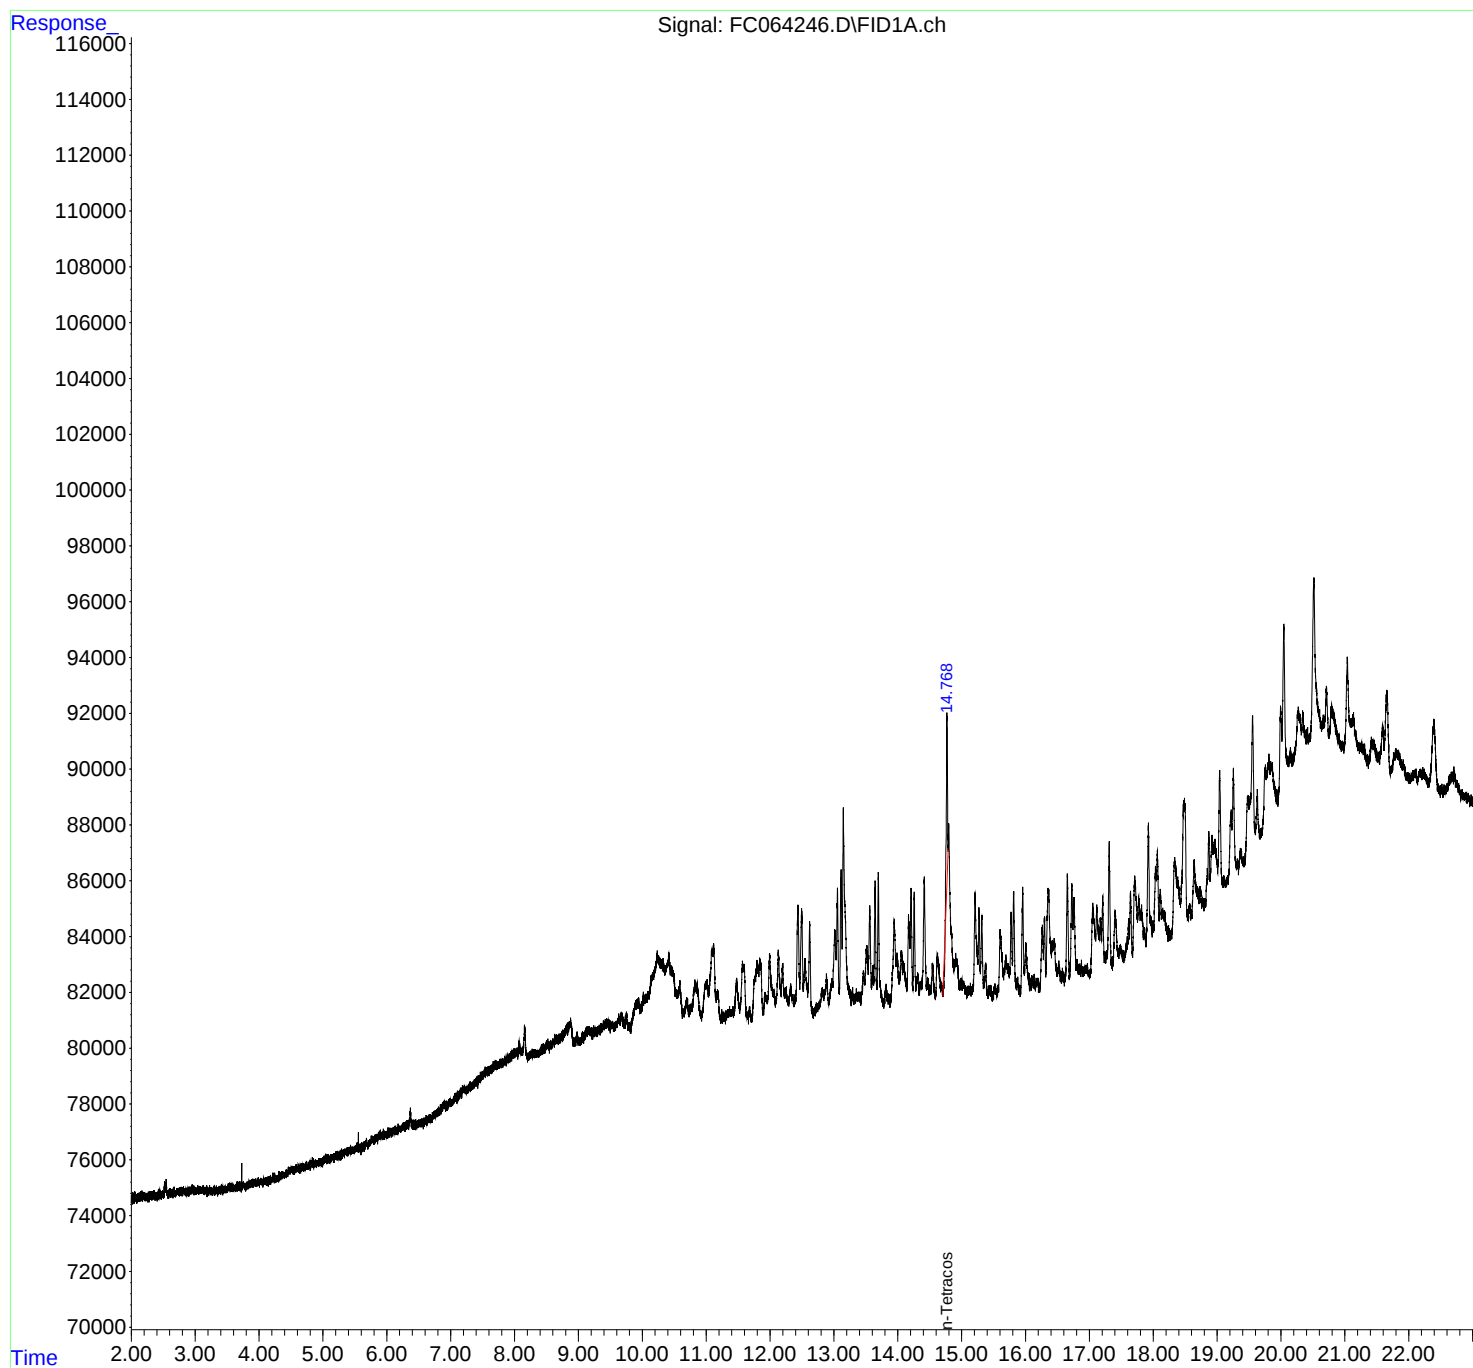


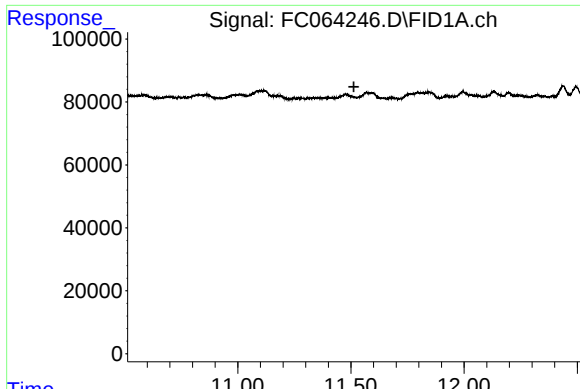

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.513 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

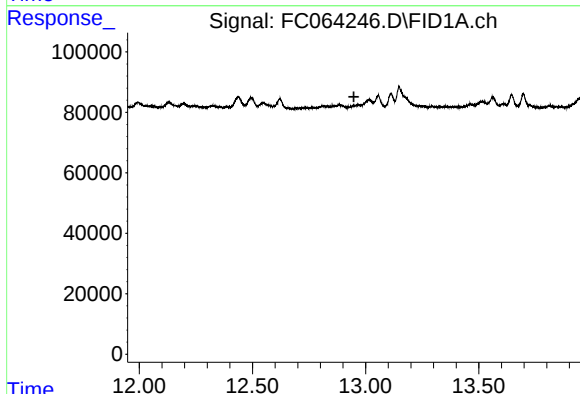

#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.948 min
Response: 0
Conc: N.D.

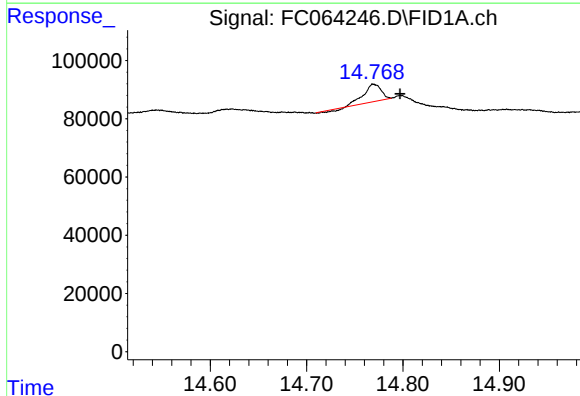

#14 n-Tetracosane (C24)

R.T.: 14.769 min
Delta R.T.: -0.027 min
Response: 69816
Conc: 0.50 ug/ml