

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC073020AL\
 Data File : FC048762.D
 Signal(s) : FID1A.CH
 Acq On : 30 Jul 2020 17:20
 Operator : DD\AJ
 Sample : L3436-04DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 4DL

Integration File: autoint1.e
 Quant Time: Jul 31 00:32:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 070820.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 08 03:03:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.112	571251	5.069 ug/ml
Spiked Amount 50.000		Recovery =	10.14%
Target Compounds			
15) T n-Hexacosane (C26)	15.989	119018	0.915 ug/ml
16) T n-Octacosane (C28)	16.938	122560	0.938 ug/ml
17) T n-Tricontane (C30)	17.822	232448	1.808 ug/ml
18) T n-Dotriacontane (C32)	18.655	151244	1.280 ug/ml
19) T n-Tetratriacontane (C34)	19.434	90246	0.808 ug/ml
20) T n-Hexatriacontane (C36)	20.178	98032	0.932 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC073020AL\
Data File : FC048762.D
Signal(s) : FID1A.CH
Acq On : 30 Jul 2020 17:20
Operator : DD\AJ
Sample : L3436-04DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_C
ClientSampled :
4DL

Integration File: autoint1.e
Quant Time: Jul 31 00:32:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 070820.M
Quant Title : GC Extractables
QLast Update : Wed Jul 08 03:03:00 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

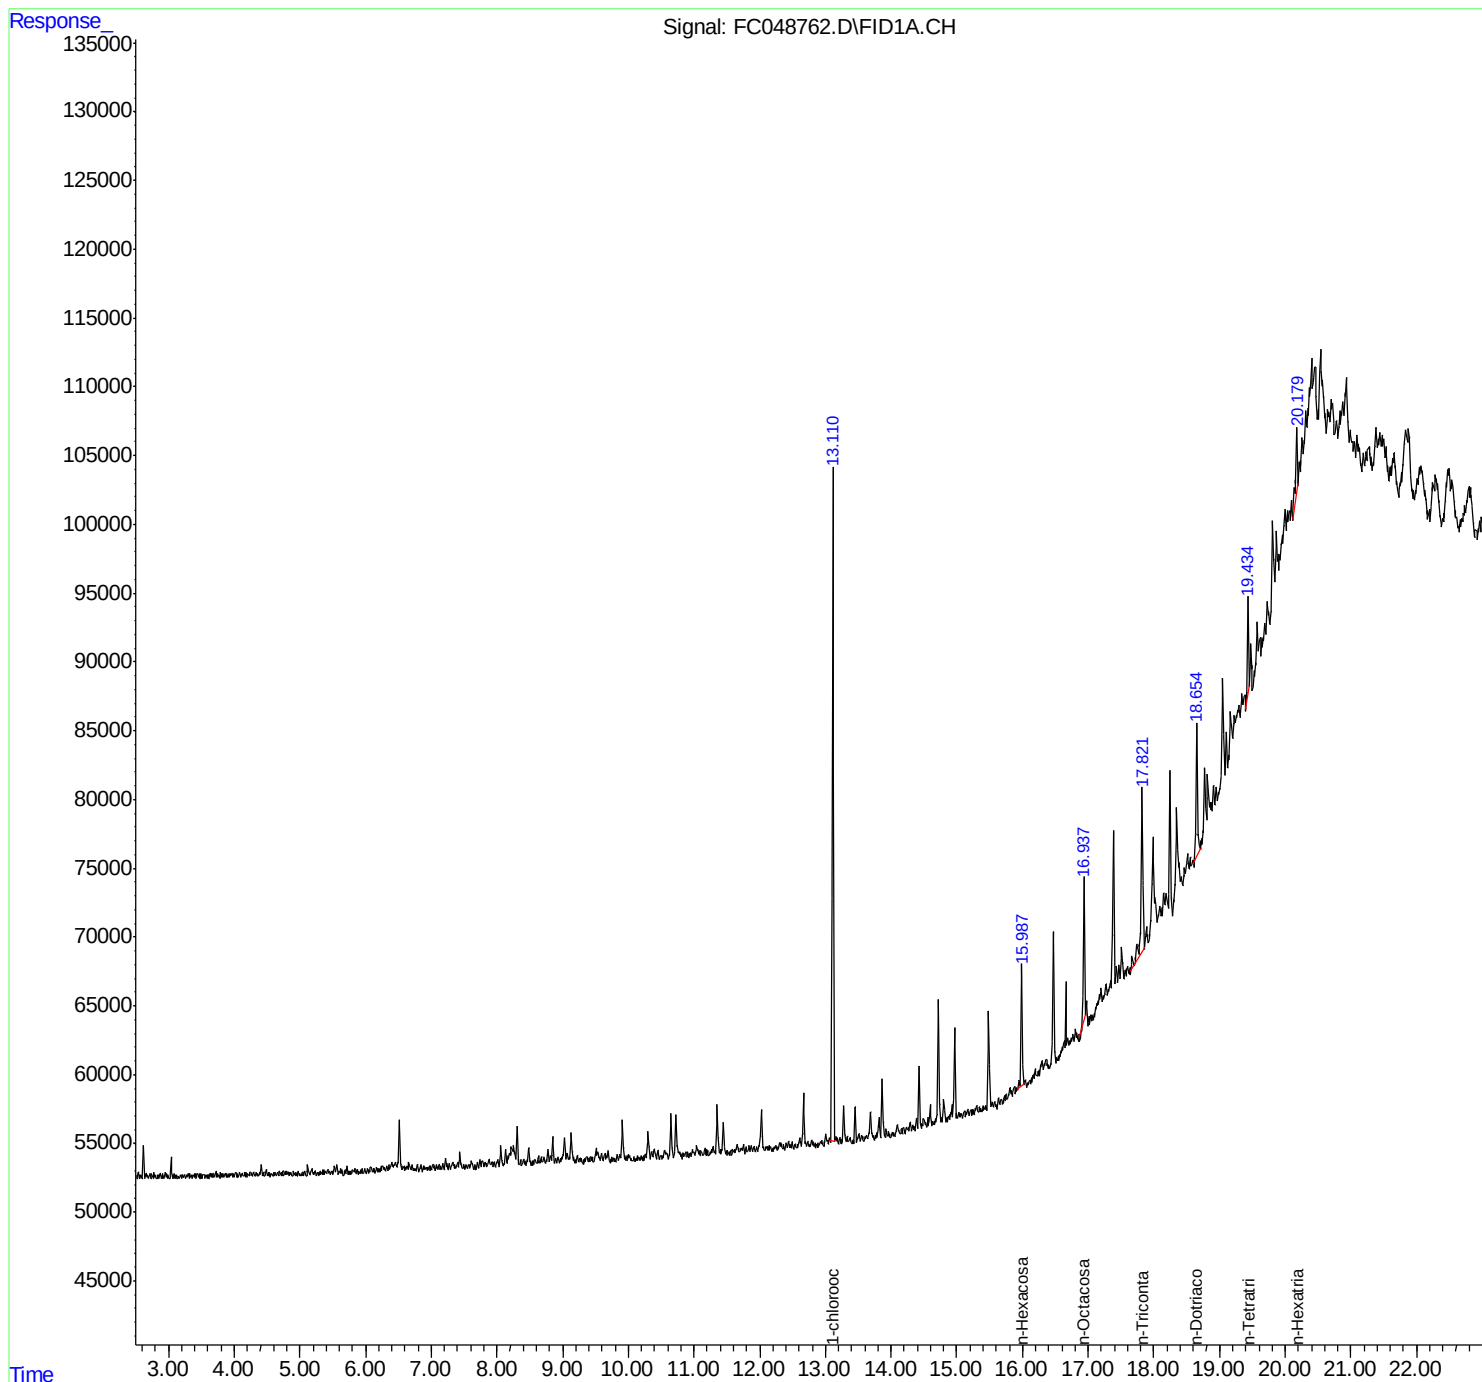


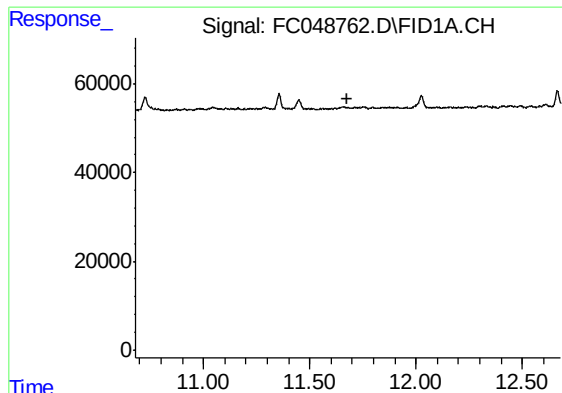

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.680 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
4DL

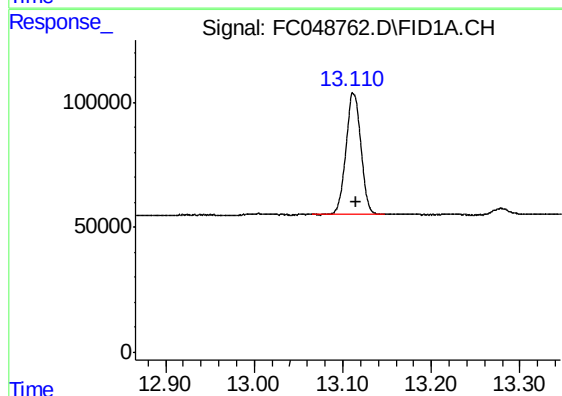


#12 1-chlorooctadecane (SURR)

R.T.: 13.112 min
Delta R.T.: -0.004 min
Response: 571251
Conc: 5.07 ug/ml

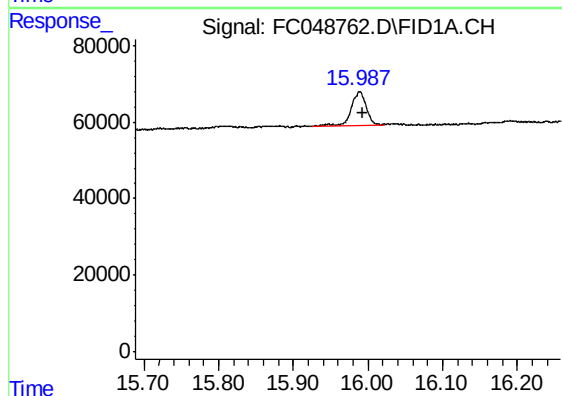


#15 n-Hexacosane (C26)

R.T.: 15.989 min
Delta R.T.: -0.003 min
Response: 119018
Conc: 0.92 ug/ml

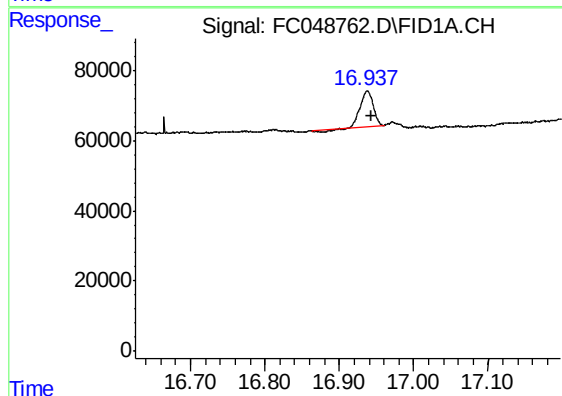

#16 n-Octacosane (C28)


R.T.: 16.938 min
Delta R.T.: -0.006 min
Response: 122560
Conc: 0.94 ug/ml

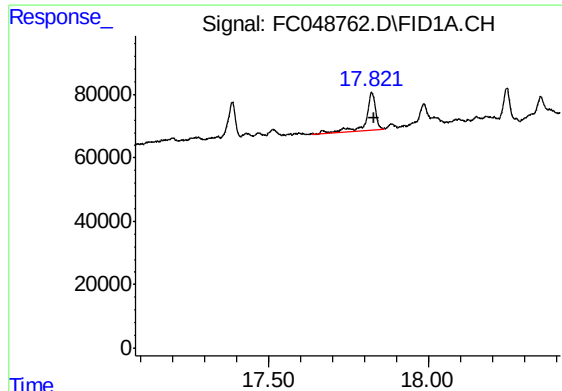

#17 n-Tricontane (C30)


R.T.: 17.822 min
Delta R.T.: -0.009 min
Response: 232448
Conc: 1.81 ug/ml

Instrument :
FID_C
ClientSampleId :
4DL

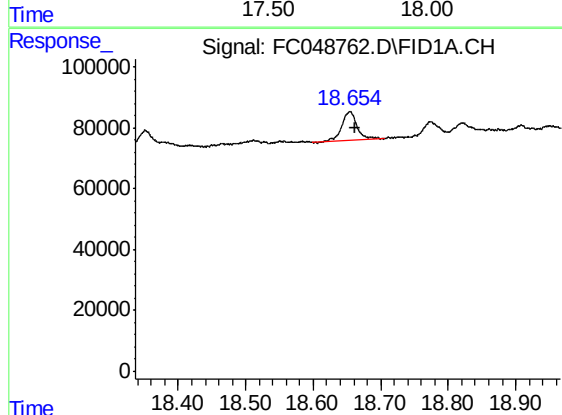


#18 n-Dotriacontane (C32)

R.T.: 18.655 min
Delta R.T.: -0.008 min
Response: 151244
Conc: 1.28 ug/ml

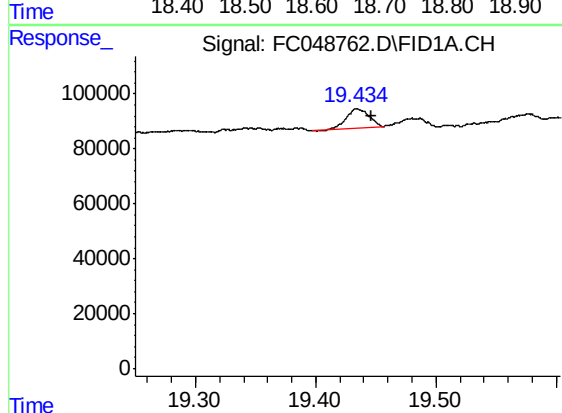

#19 n-Tetratriacontane (C34)

R.T.: 19.434 min
Delta R.T.: -0.013 min
Response: 90246
Conc: 0.81 ug/ml

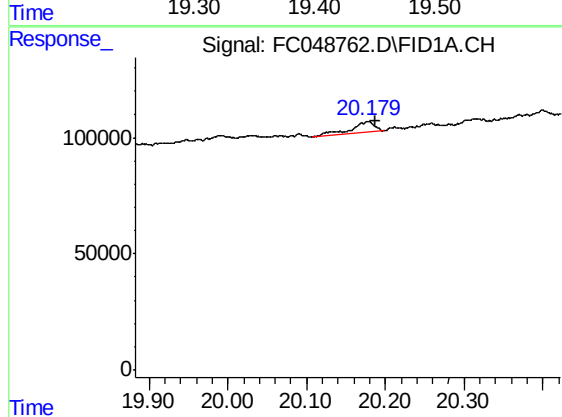

#20 n-Hexatriacontane (C36)

R.T.: 20.178 min
Delta R.T.: -0.008 min
Response: 98032
Conc: 0.93 ug/ml