

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC080122AL\
 Data File : FC060915.D
 Signal(s) : FID1A.ch
 Acq On : 01 Aug 2022 08:57
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 02 02:50:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 072522.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 25 19:40:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) T n-Heneicosane (C21)	12.130	475091	3.036 ug/ml
13) T n-Docosane (C22)	12.718	395250	2.535 ug/ml
14) T n-Tetracosane (C24)	13.800	300720	1.970 ug/ml
15) T n-Hexacosane (C26)	14.798	278691	1.867 ug/ml
16) T n-Octacosane (C28)	15.726	229591	1.602 ug/ml
17) T n-Tricontane (C30)	16.592	340059	2.429 ug/ml
18) T n-Dotriacontane (C32)	17.405	412125	3.054 ug/ml
19) T n-Tetratriacontane (C34)	18.170	227005	1.810 ug/ml
20) T n-Hexatriacontane (C36)	18.890	150329	1.230 ug/ml
21) T n-Octatriacontane (C38)	19.569	186830	1.583 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC080122AL\
Data File : FC060915.D
Signal(s) : FID1A.ch
Acq On : 01 Aug 2022 08:57
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 02 02:50:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 072522.M
Quant Title : GC Extractables
QLast Update : Mon Jul 25 19:40:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

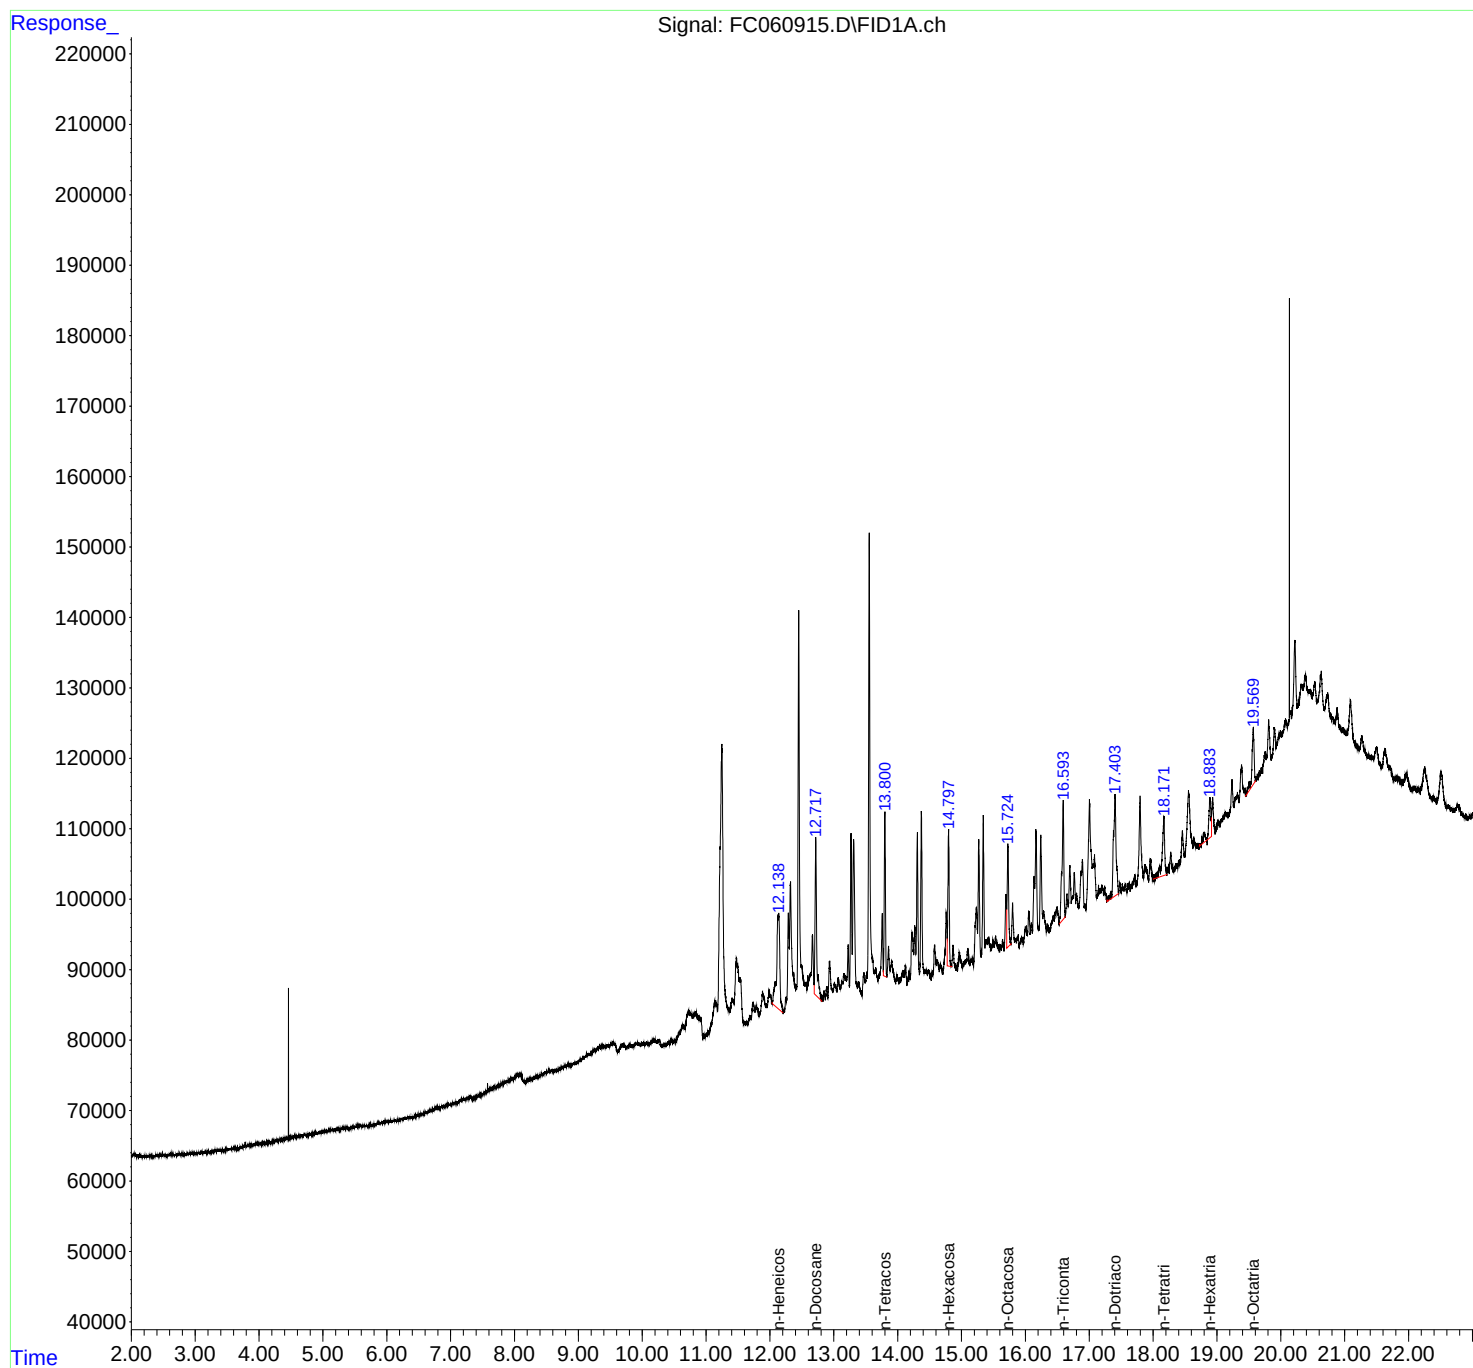


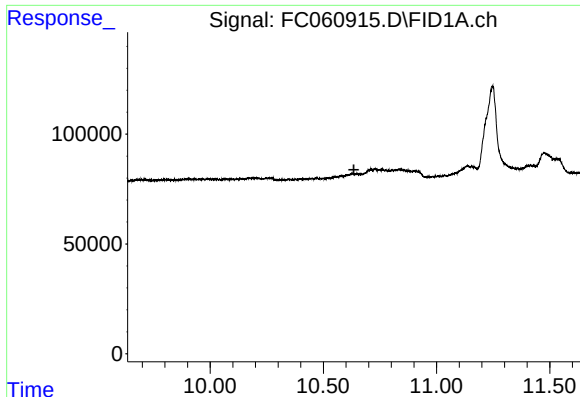

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.635 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

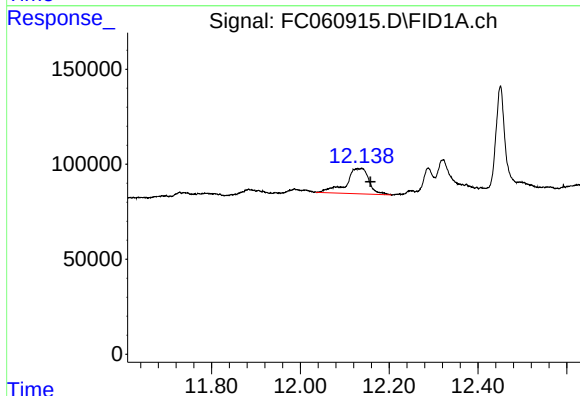


#11 n-Heneicosane (C21)

R.T.: 12.130 min
Delta R.T.: -0.028 min
Response: 475091
Conc: 3.04 ug/ml

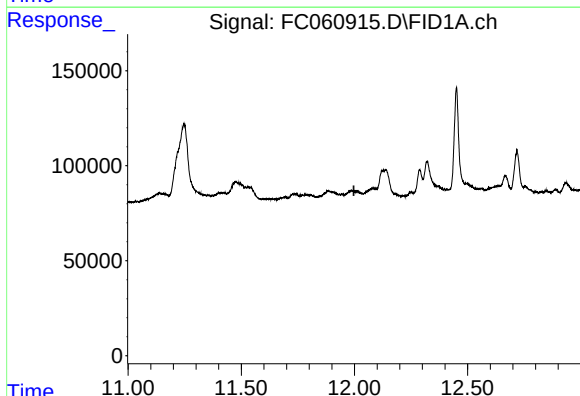


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 11.998 min
Response: 0
Conc: N.D.

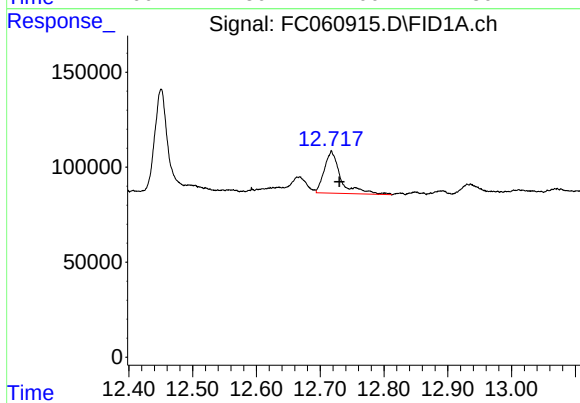

#13 n-Docosane (C22)


R.T.: 12.718 min
Delta R.T.: -0.012 min
Response: 395250
Conc: 2.54 ug/ml

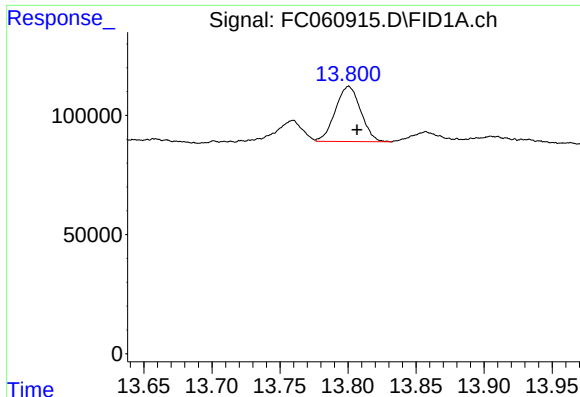

#14 n-Tetracosane (C24)


R.T.: 13.800 min
Delta R.T.: -0.006 min
Response: 300720
Conc: 1.97 ug/ml

Instrument :
FID_C
ClientSampleId :

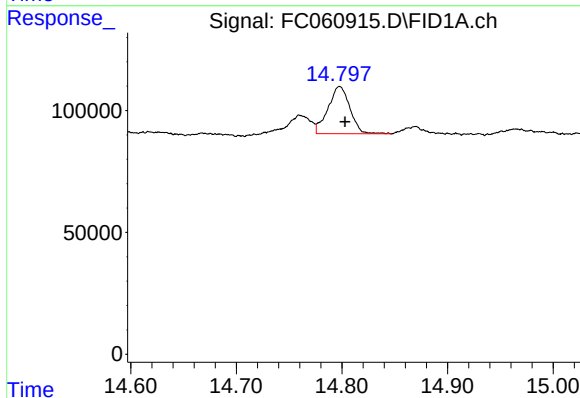


#15 n-Hexacosane (C26)

R.T.: 14.798 min
Delta R.T.: -0.005 min
Response: 278691
Conc: 1.87 ug/ml

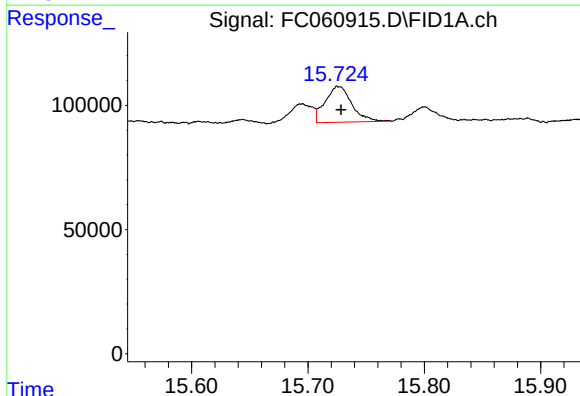


#16 n-Octacosane (C28)

R.T.: 15.726 min
Delta R.T.: -0.002 min
Response: 229591
Conc: 1.60 ug/ml

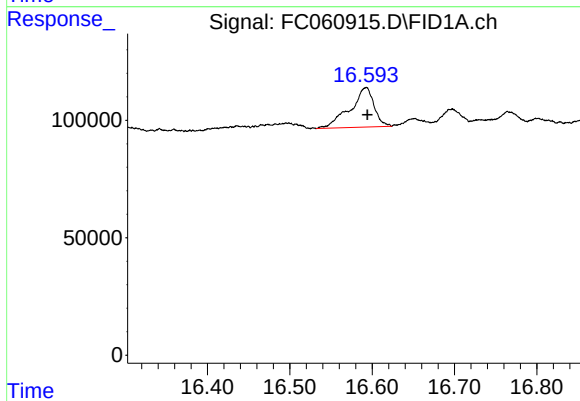

#17 n-Tricontane (C30)


R.T.: 16.592 min
Delta R.T.: -0.002 min
Response: 340059
Conc: 2.43 ug/ml

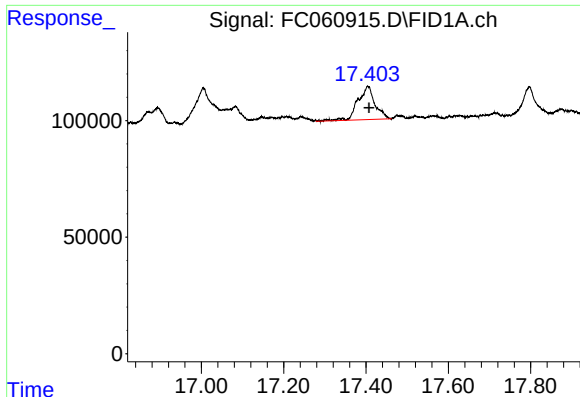

#18 n-Dotriacontane (C32)


R.T.: 17.405 min
Delta R.T.: -0.002 min
Response: 412125
Conc: 3.05 ug/ml

Instrument :
FID_C
ClientSampleId :

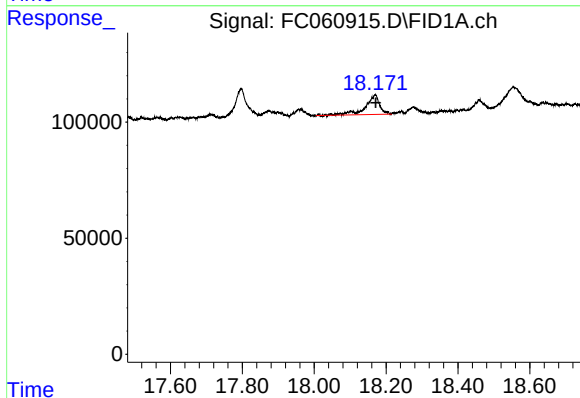


#19 n-Tetratriacontane (C34)

R.T.: 18.170 min
Delta R.T.: 0.000 min
Response: 227005
Conc: 1.81 ug/ml

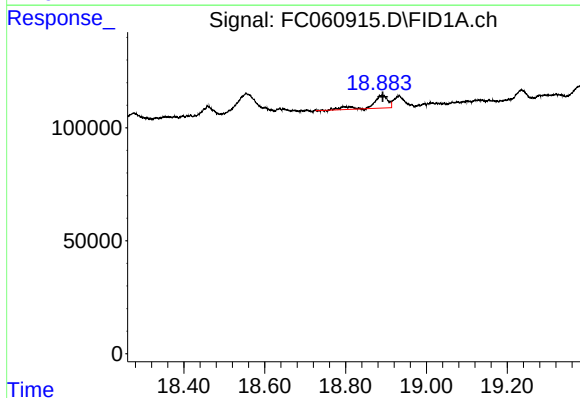

#20 n-Hexatriacontane (C36)

R.T.: 18.890 min
Delta R.T.: -0.002 min
Response: 150329
Conc: 1.23 ug/ml

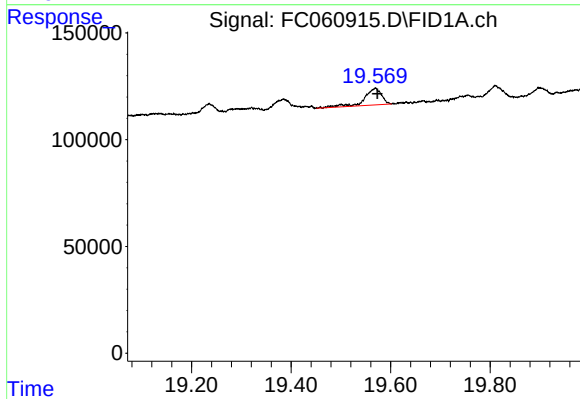

#21 n-Octatriacontane (C38)

R.T.: 19.569 min
Delta R.T.: -0.005 min
Response: 186830
Conc: 1.58 ug/ml