

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC080122AL\
 Data File : FC060941.D
 Signal(s) : FID1A.ch
 Acq On : 02 Aug 2022 05:54
 Operator : YP/AJ
 Sample : N3962-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 02 07:04:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 072522.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 25 19:40:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.632	6430517	39.184 ug/ml
Spiked Amount 50.000		Recovery =	78.37%
12) S 1-chlorooctadecane (S...	11.998	5329945	40.149 ug/ml
Spiked Amount 50.000		Recovery =	80.30%
Target Compounds			
10) T n-Eicosane (C20)	11.541	158896	1.013 ug/ml
14) T n-Tetracosane (C24)	13.816	185540	1.215 ug/ml
16) T n-Octacosane (C28)	15.747	269058	1.878 ug/ml
17) T n-Tricontane (C30)	16.590	216480	1.546 ug/ml
18) T n-Dotriacontane (C32)	17.404	805836	5.971 ug/ml
19) T n-Tetratriacontane (C34)	18.179	156140	1.245 ug/ml
21) T n-Octatriacontane (C38)	19.600	215582	1.827 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC080122AL\
Data File : FC060941.D
Signal(s) : FID1A.ch
Acq On : 02 Aug 2022 05:54
Operator : YP/AJ
Sample : N3962-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 02 07:04:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 072522.M
Quant Title : GC Extractables
QLast Update : Mon Jul 25 19:40:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

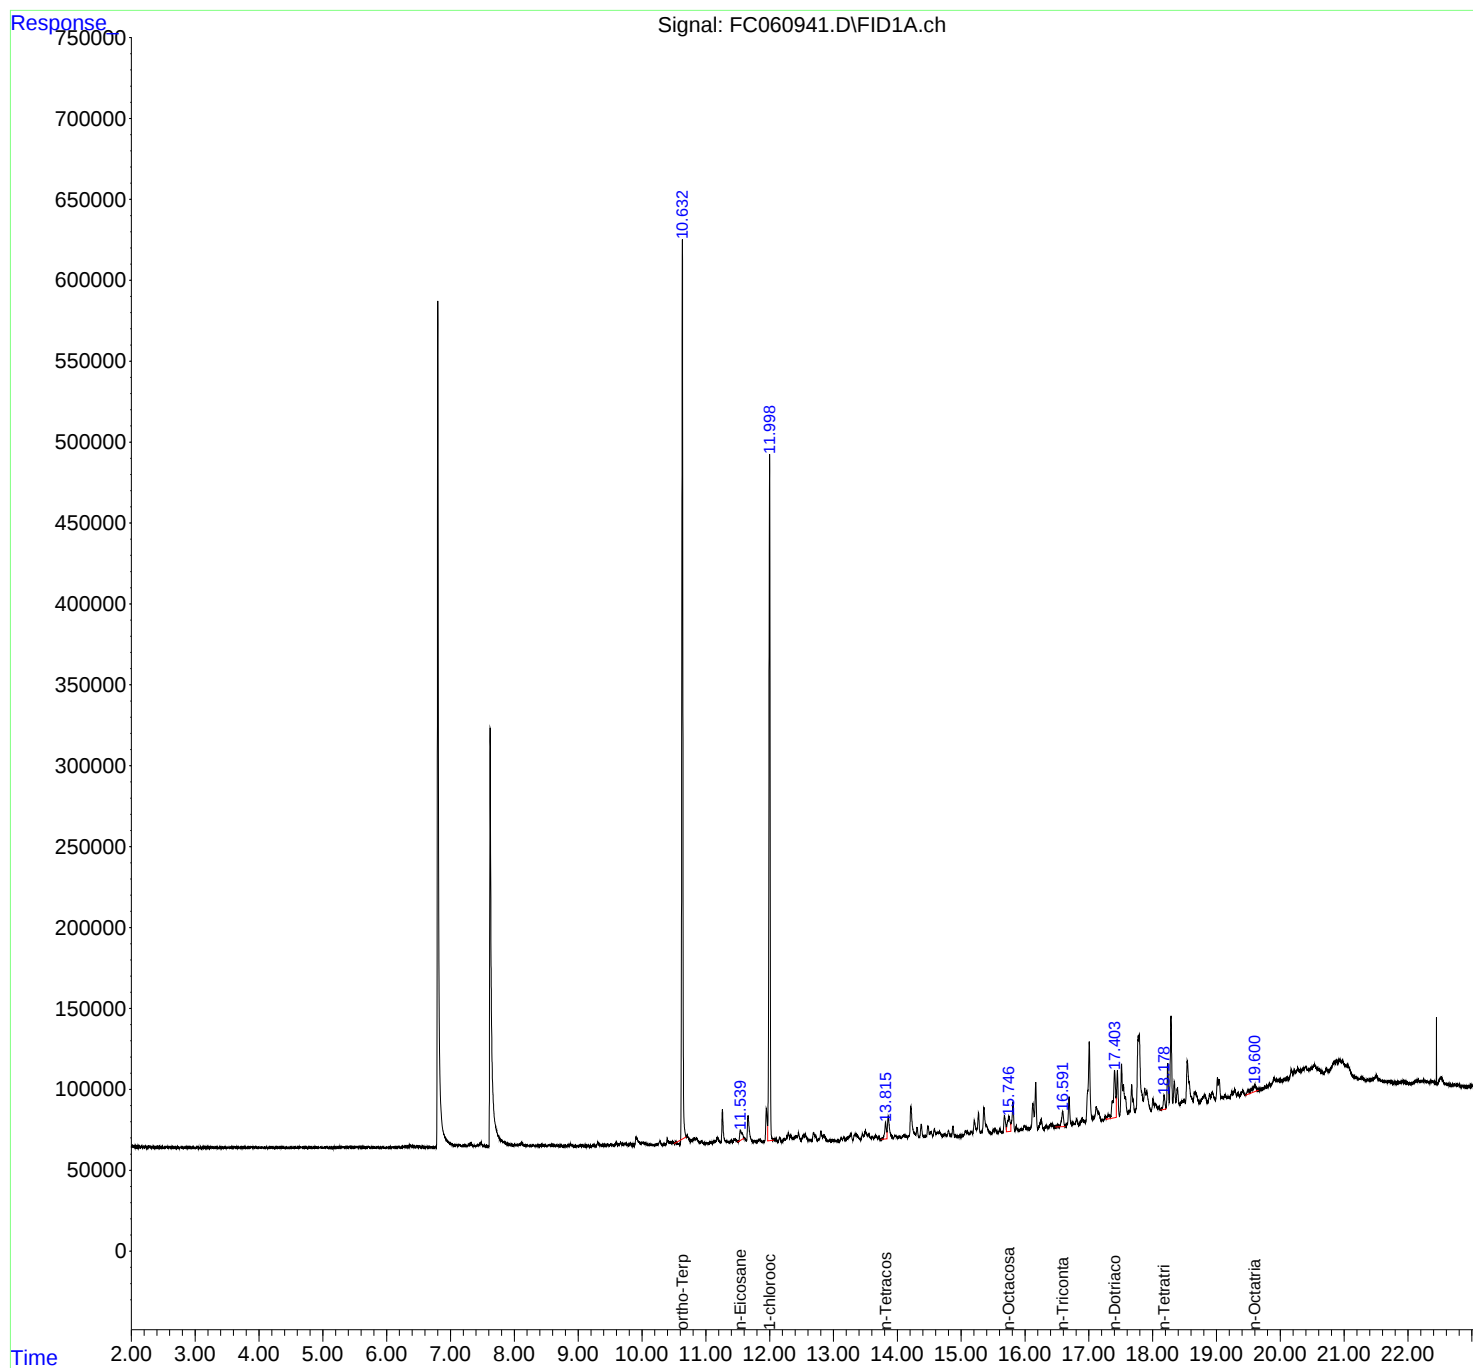


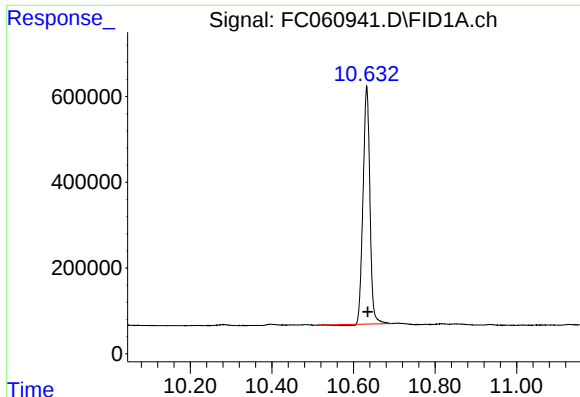

#9 ortho-Terphenyl (SURR)


R.T.: 10.632 min
Delta R.T.: -0.002 min
Response: 6430517
Conc: 39.18 ug/ml

Instrument :
FID_C
ClientSampleId :

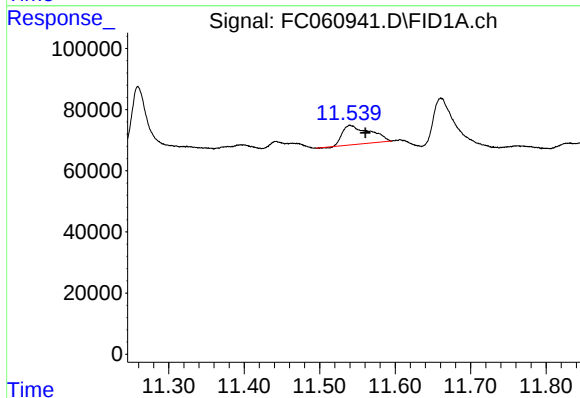


#10 n-Eicosane (C20)

R.T.: 11.541 min
Delta R.T.: -0.020 min
Response: 158896
Conc: 1.01 ug/ml

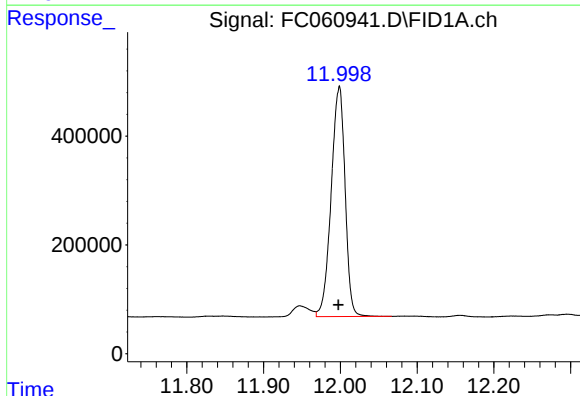


#12 1-chlorooctadecane (SURR)

R.T.: 11.998 min
Delta R.T.: 0.000 min
Response: 5329945
Conc: 40.15 ug/ml

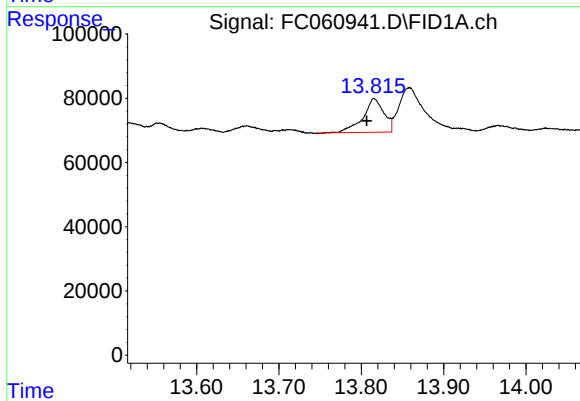

#14 n-Tetracosane (C24)


R.T.: 13.816 min
Delta R.T.: 0.009 min
Response: 185540
Conc: 1.22 ug/ml

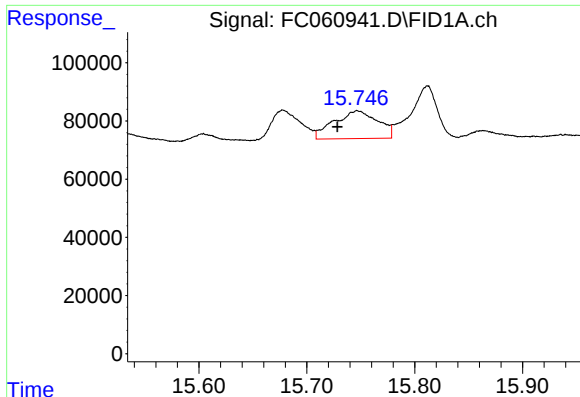

#16 n-Octacosane (C28)


R.T.: 15.747 min
Delta R.T.: 0.018 min
Response: 269058
Conc: 1.88 ug/ml

Instrument :
FID_C
ClientSampleId :

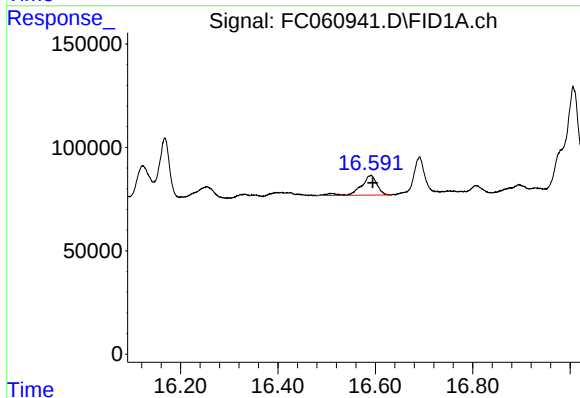


#17 n-Tricontane (C30)

R.T.: 16.590 min
Delta R.T.: -0.004 min
Response: 216480
Conc: 1.55 ug/ml

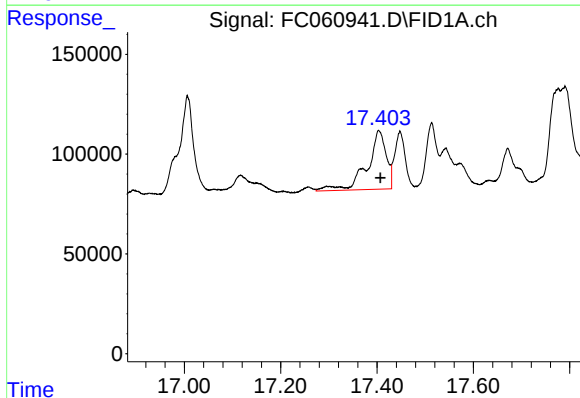


#18 n-Dotriacontane (C32)

R.T.: 17.404 min
Delta R.T.: -0.003 min
Response: 805836
Conc: 5.97 ug/ml

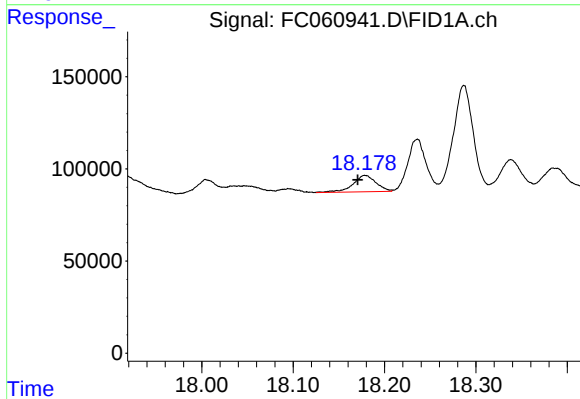

#19 n-Tetratriacontane (C34)

R.T.: 18.179 min
Delta R.T.: 0.008 min
Response: 156140
Conc: 1.24 ug/ml

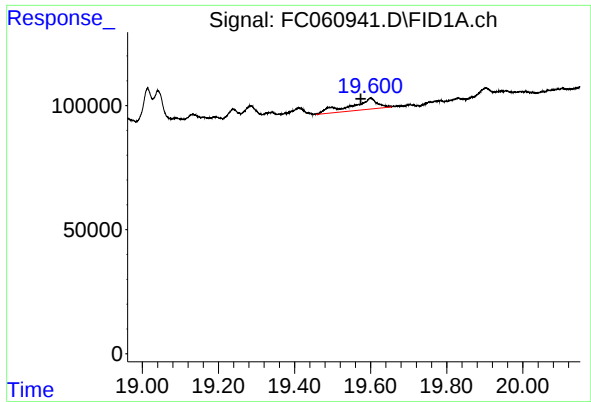

#21 n-Octatriacontane (C38)

R.T.: 19.600 min
Delta R.T.: 0.026 min
Response: 215582
Conc: 1.83 ug/ml

Instrument :
FID_C
ClientSampleId :