

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC080124AL\
 Data File : FC066881.D
 Signal(s) : FID1A.ch
 Acq On : 01 Aug 2024 08:15
 Operator : YP/AJ
 Sample : P3394-01DL 2X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 02 02:55:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 071524.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 15 13:58:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.956	1356824	12.134 ug/ml
Spiked Amount 50.000		Recovery =	24.27%
Target Compounds			
4) T n-Dodecane (C12)	6.367	40408	0.270 ug/ml
16) T n-Octacosane (C28)	16.799	81917	0.649 ug/ml
17) T n-Tricontane (C30)	17.667	141990	1.104 ug/ml
18) T n-Dotriacontane (C32)	18.500	114231	0.907 ug/ml
19) T n-Tetratriacontane (C34)	19.286	142962	1.156 ug/ml
20) T n-Hexatriacontane (C36)	20.086f	56177	0.483 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC080124AL\
Data File : FC066881.D
Signal(s) : FID1A.ch
Acq On : 01 Aug 2024 08:15
Operator : YP/AJ
Sample : P3394-01DL 2X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 02 02:55:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 071524.M
Quant Title : GC Extractables
QLast Update : Mon Jul 15 13:58:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

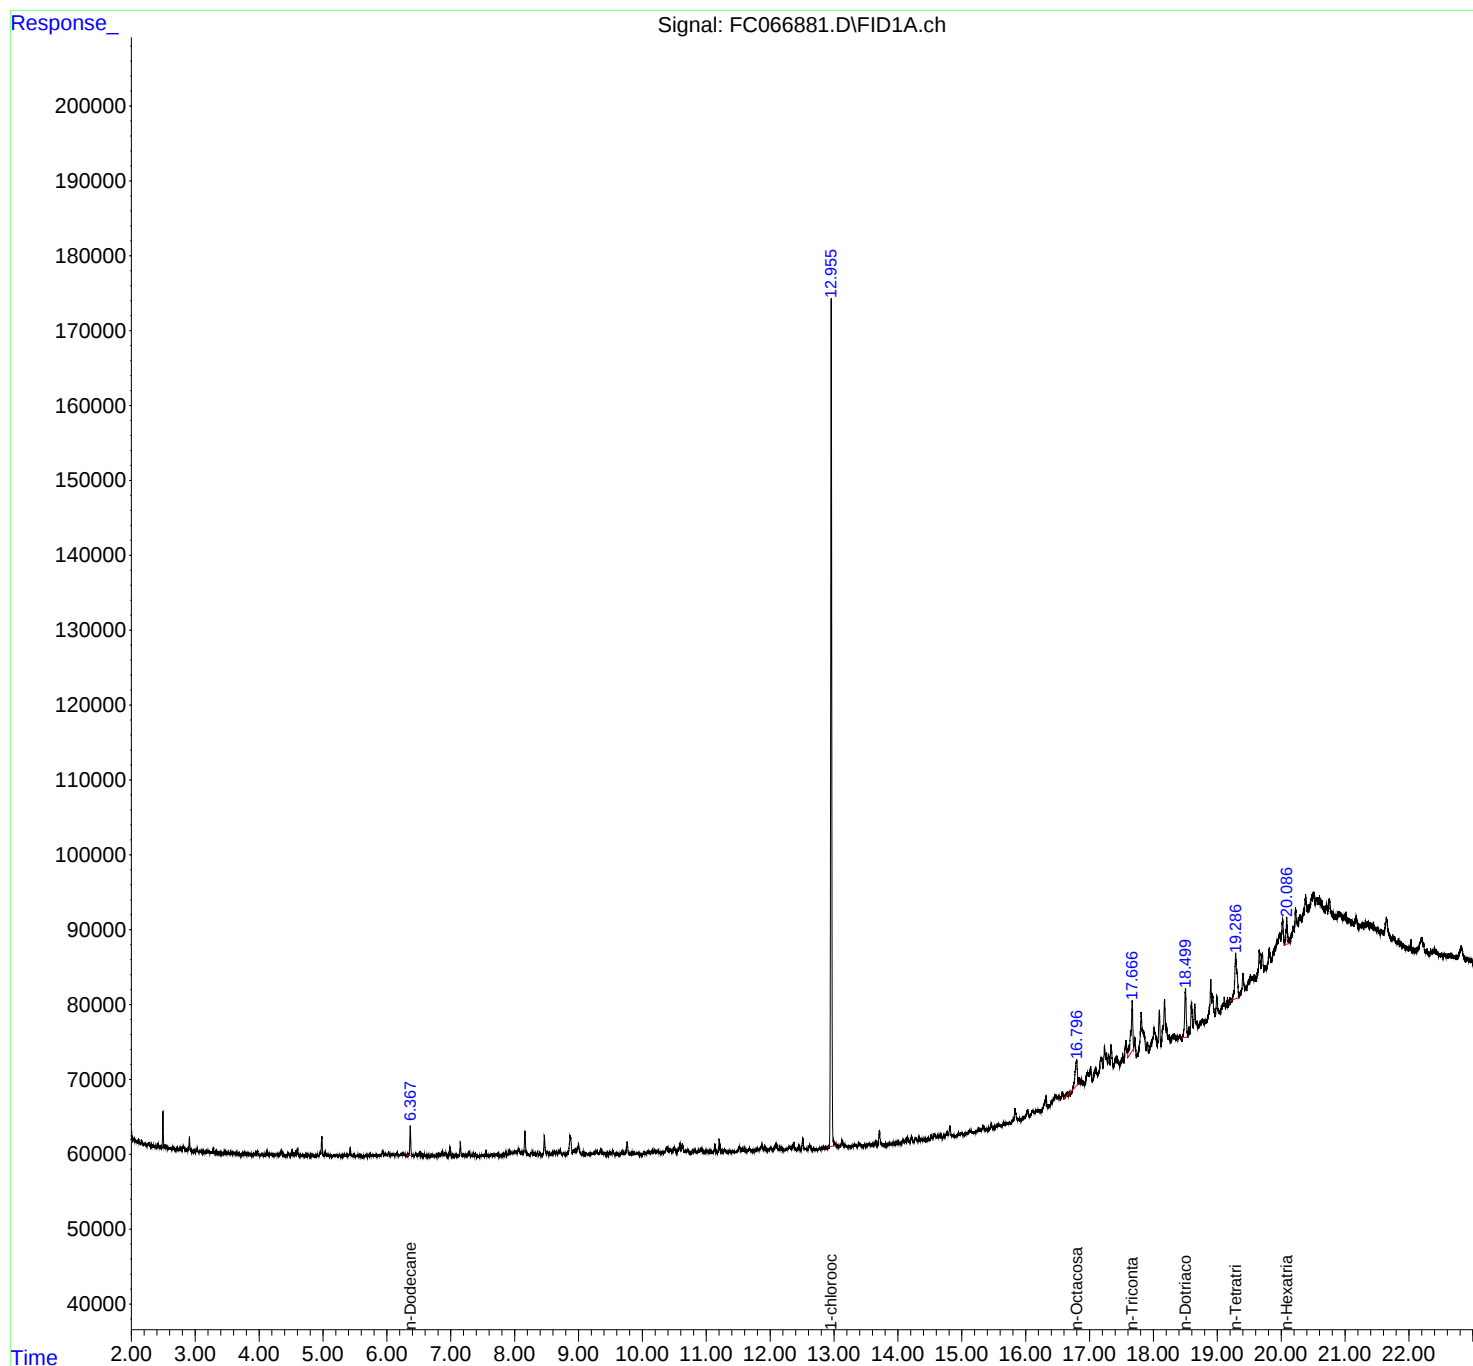


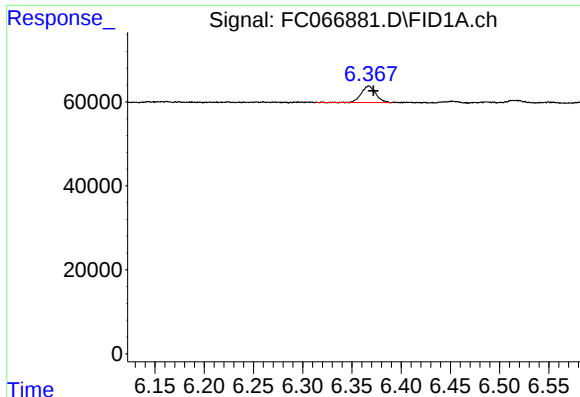

#4 n-Dodecane (C12)


R.T.: 6.367 min
Delta R.T.: -0.005 min
Response: 40408
Conc: 0.27 ug/ml

Instrument :
FID_C
ClientSampleId :

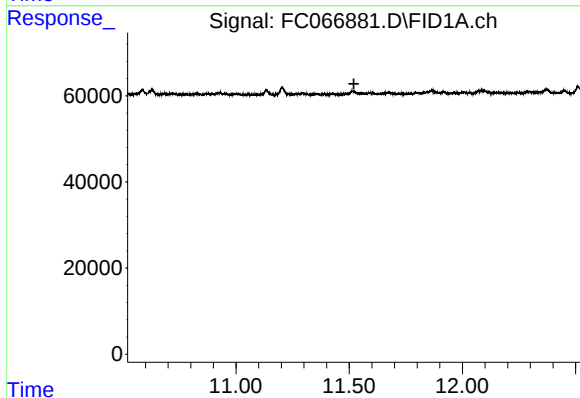


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.521 min
Response: 0
Conc: N.D.

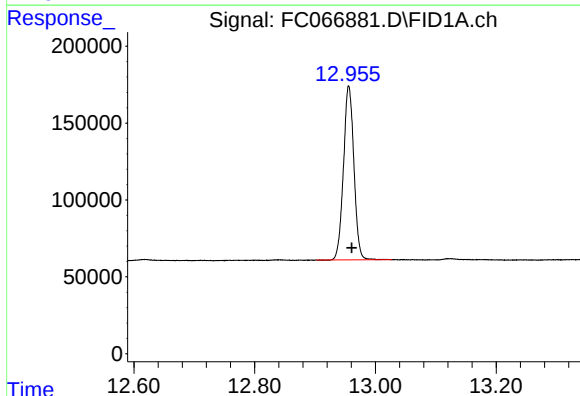


#12 1-chlorooctadecane (SURR)

R.T.: 12.956 min
Delta R.T.: -0.005 min
Response: 1356824
Conc: 12.13 ug/ml

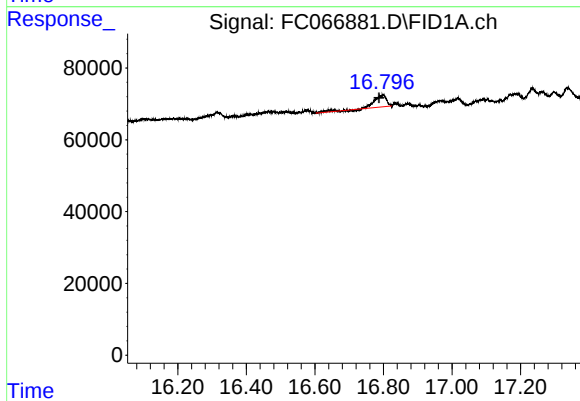

#16 n-Octacosane (C28)


R.T.: 16.799 min
Delta R.T.: 0.011 min
Response: 81917
Conc: 0.65 ug/ml

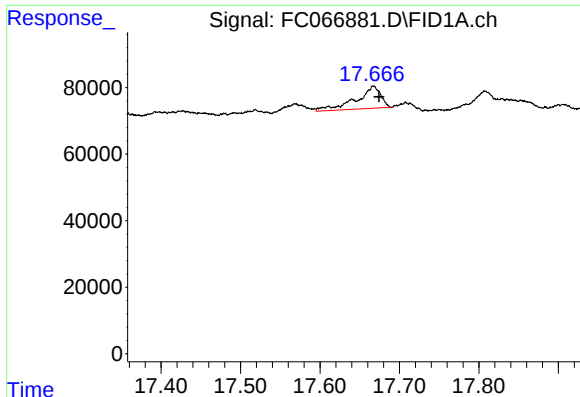

#17 n-Tricontane (C30)


R.T.: 17.667 min
Delta R.T.: -0.007 min
Response: 141990
Conc: 1.10 ug/ml

Instrument :
FID_C
ClientSampleId :

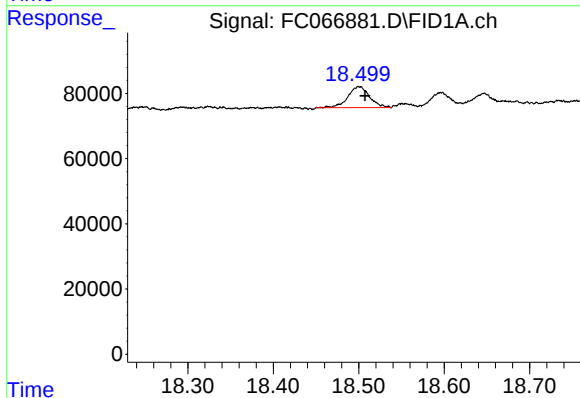


#18 n-Dotriacontane (C32)

R.T.: 18.500 min
Delta R.T.: -0.007 min
Response: 114231
Conc: 0.91 ug/ml

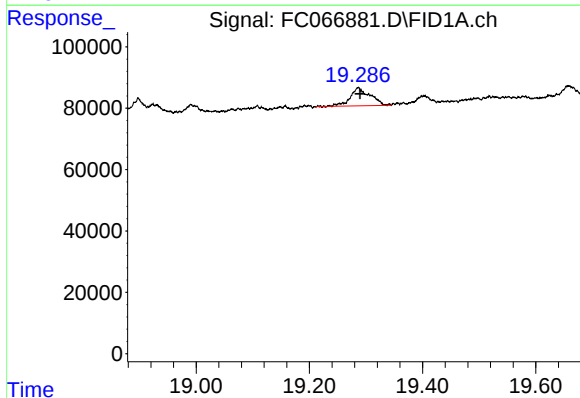

#19 n-Tetratriacontane (C34)

R.T.: 19.286 min
Delta R.T.: -0.003 min
Response: 142962
Conc: 1.16 ug/ml

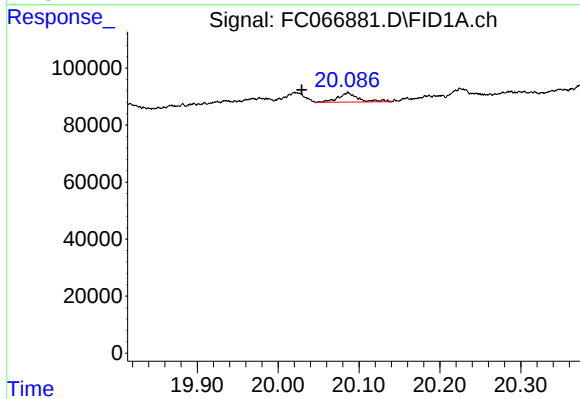

#20 n-Hexatriacontane (C36)

R.T.: 20.086 min
Delta R.T.: 0.057 min
Response: 56177
Conc: 0.48 ug/ml