

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC080624AL\  
 Data File : FC066936.D  
 Signal(s) : FID1A.ch  
 Acq On : 06 Aug 2024 08:13  
 Operator : YP/AJ  
 Sample : P3461-01DL 2X  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 FID\_C  
 ClientSampleId :  
 CHRT-28607DL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 08/07/2024  
 Supervised By :Ankita Jodhani 08/07/2024

Integration File: autoint1.e  
 Quant Time: Aug 07 03:41:23 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 071524.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Jul 15 13:58:41 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units    |
|--------------------------------|--------|----------|---------------|
| -----                          |        |          |               |
| System Monitoring Compounds    |        |          |               |
| 9) S ortho-Terphenyl (SURR)    | 11.519 | 2074295  | 13.474 ug/mlm |
| Spiked Amount                  | 50.000 | Recovery | = 26.95%      |
| 12) S 1-chlorooctadecane (S... | 12.961 | 1463535  | 13.089 ug/mlm |
| Spiked Amount                  | 50.000 | Recovery | = 26.18%      |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC080624AL\  
Data File : FC066936.D  
Signal(s) : FID1A.ch  
Acq On : 06 Aug 2024 08:13  
Operator : YP/AJ  
Sample : P3461-01DL 2X  
Misc :  
ALS Vial : 7 Sample Multiplier: 1


Instrument :  
FID\_C  
ClientSampleId :  
CHRT-28607DL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/07/2024  
Supervised By :Ankita Jodhani 08/07/2024

Integration File: autoint1.e  
Quant Time: Aug 07 03:41:23 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 071524.M  
Quant Title : GC Extractables  
QLast Update : Mon Jul 15 13:58:41 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

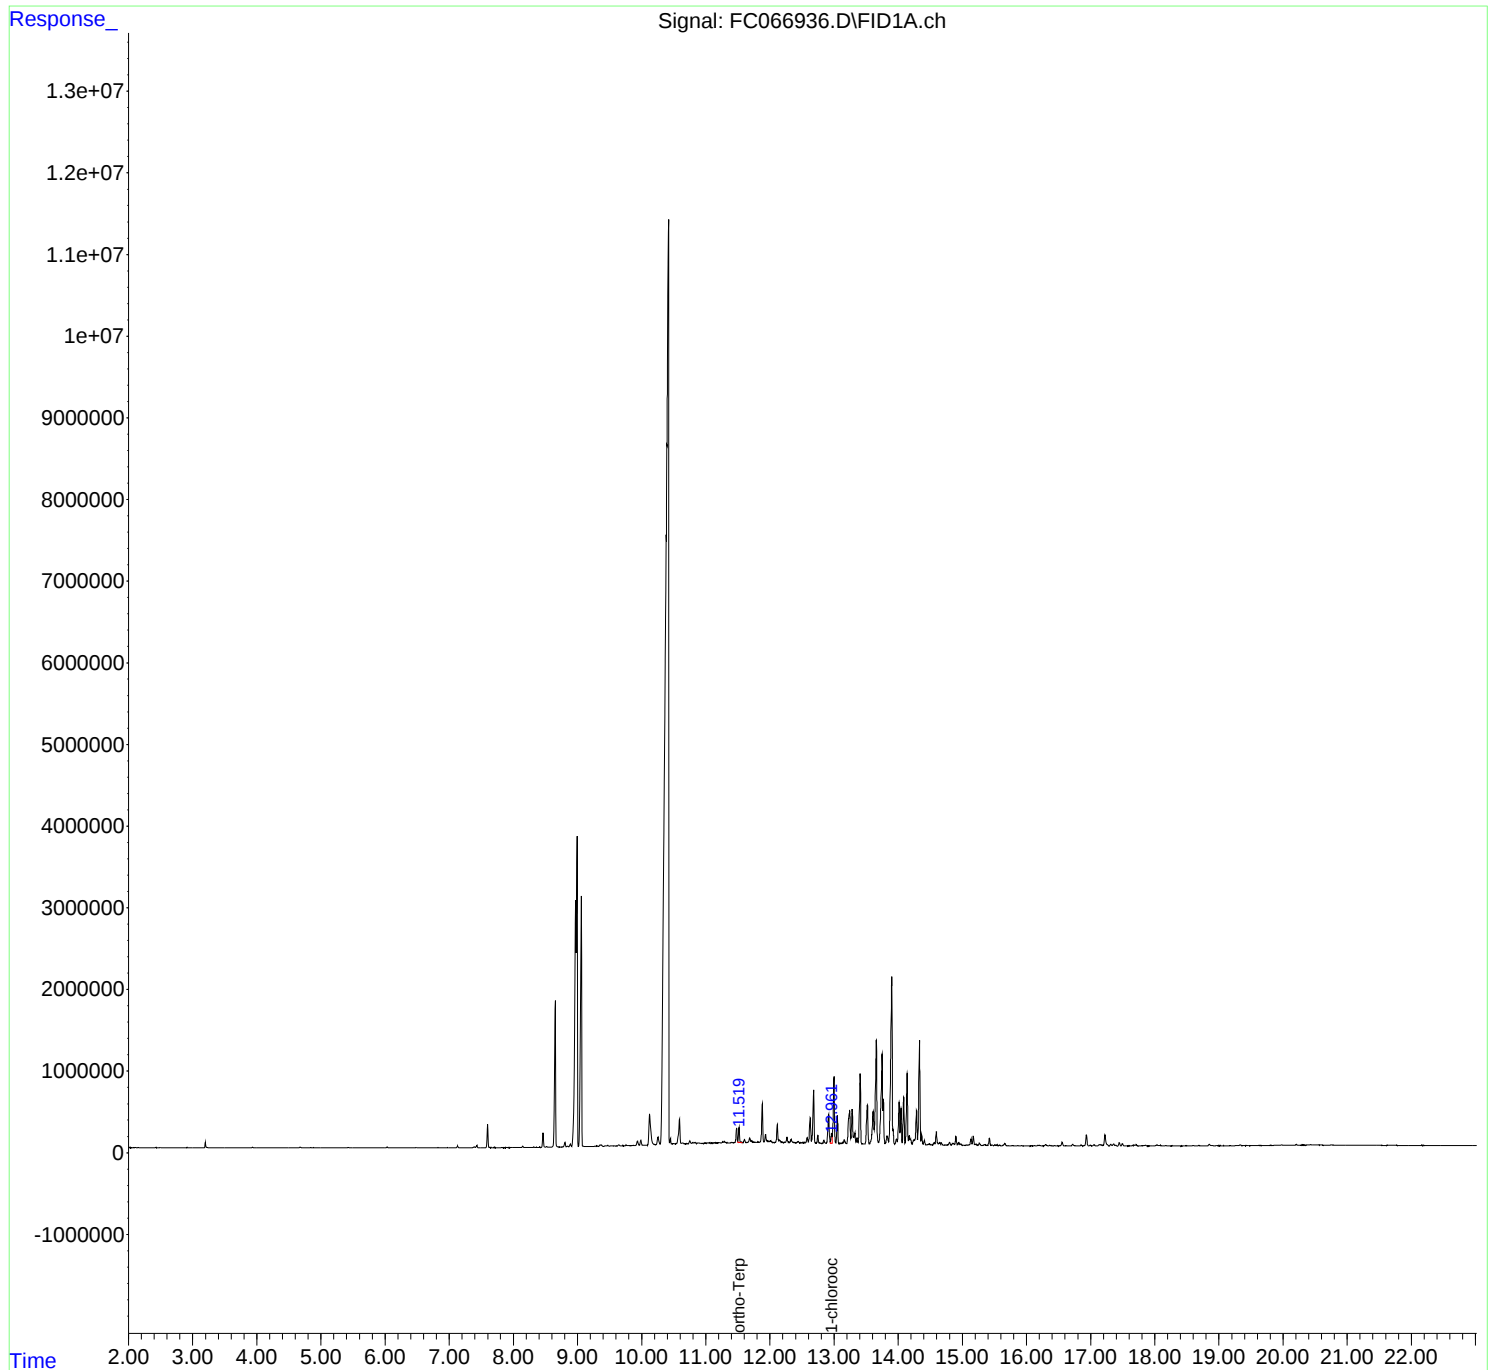

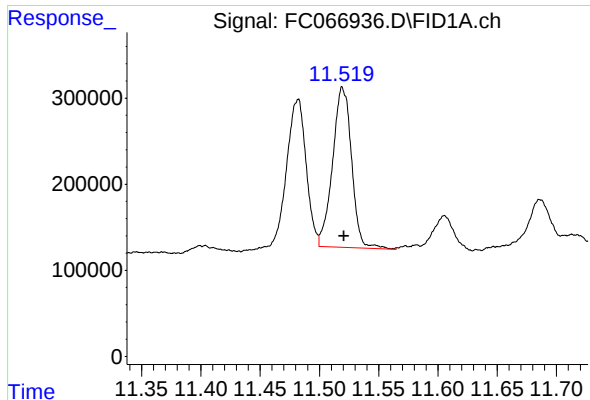


#9 ortho-Terphenyl (SURR)

R.T.: 11.519 min  
Delta R.T.: -0.002 min  
Response: 2074295  
Conc: 13.47 ug/ml

Instrument :  
FID\_C  
ClientSampleId :  
CHRT-28607DL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/07/2024  
Supervised By :Ankita Jodhani 08/07/2024

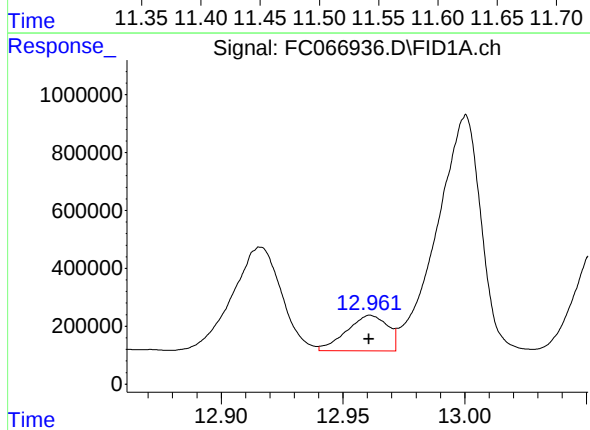

#12 1-chlorooctadecane (SURR)

R.T.: 12.961 min  
Delta R.T.: 0.000 min  
Response: 1463535  
Conc: 13.09 ug/ml m