

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC080724AL\
 Data File : FC066949.D
 Signal(s) : FID1A.ch
 Acq On : 07 Aug 2024 16:23
 Operator : YP/AJ
 Sample : PB162552BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 08 02:11:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 071524.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 15 13:58:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.957	5038361	45.059 ug/ml
Spiked Amount 50.000		Recovery =	90.12%
Target Compounds			
4) T n-Dodecane (C12)	6.365	95071	0.634 ug/ml
6) T n-Tetradecane (C14)	8.159	58347	0.399 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC080724AL\
Data File : FC066949.D
Signal(s) : FID1A.ch
Acq On : 07 Aug 2024 16:23
Operator : YP/AJ
Sample : PB162552BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 08 02:11:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 071524.M
Quant Title : GC Extractables
QLast Update : Mon Jul 15 13:58:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

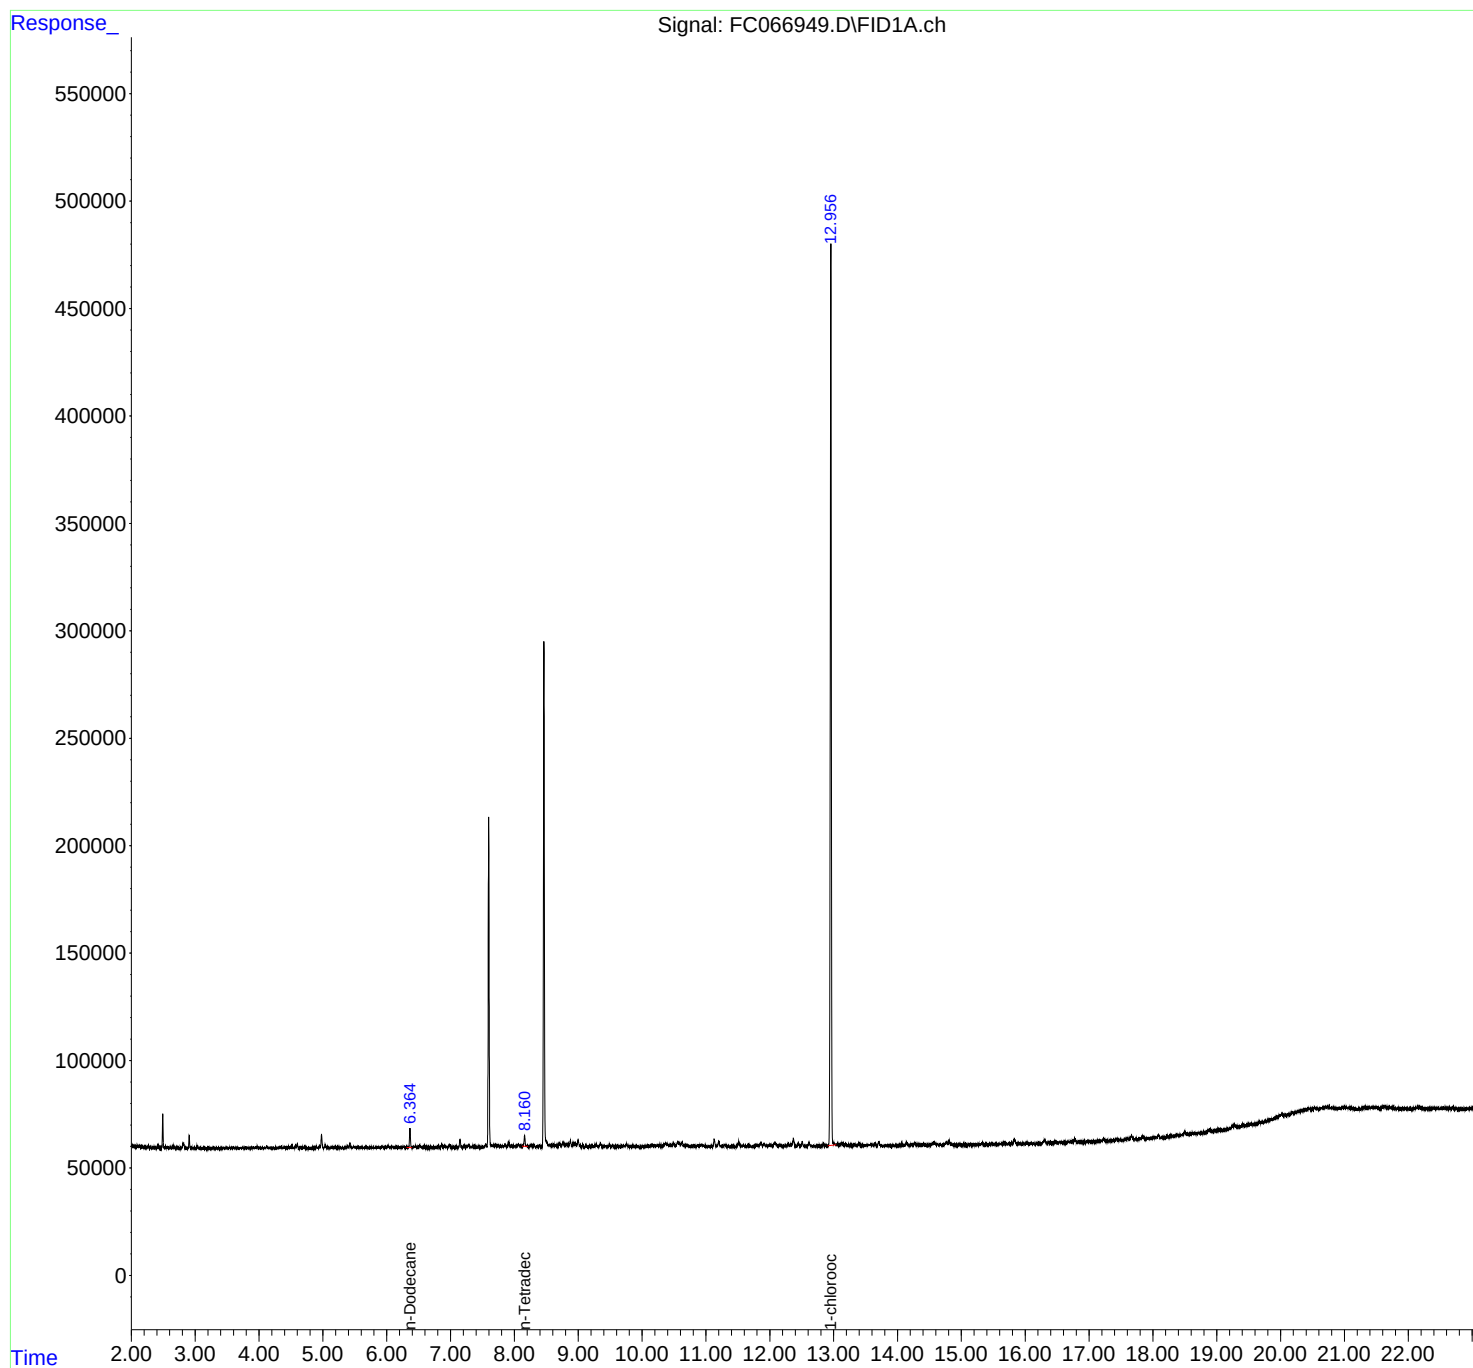


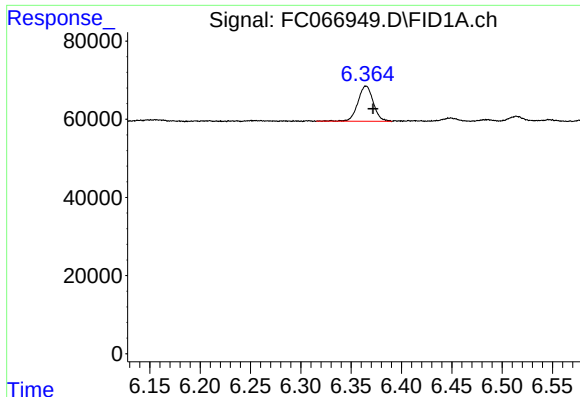

#4 n-Dodecane (C12)


R.T.: 6.365 min
Delta R.T.: -0.007 min
Response: 95071
Conc: 0.63 ug/ml

Instrument :
FID_C
ClientSampleId :

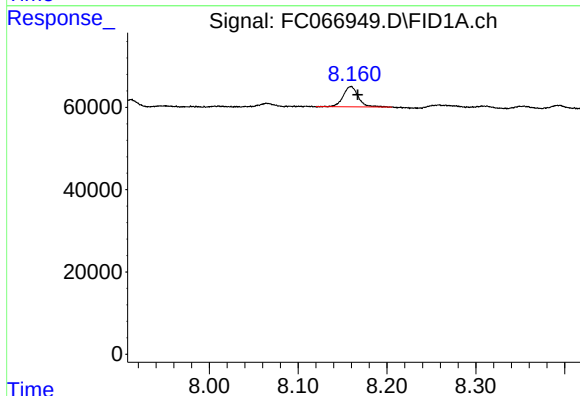


#6 n-Tetradecane (C14)

R.T.: 8.159 min
Delta R.T.: -0.008 min
Response: 58347
Conc: 0.40 ug/ml

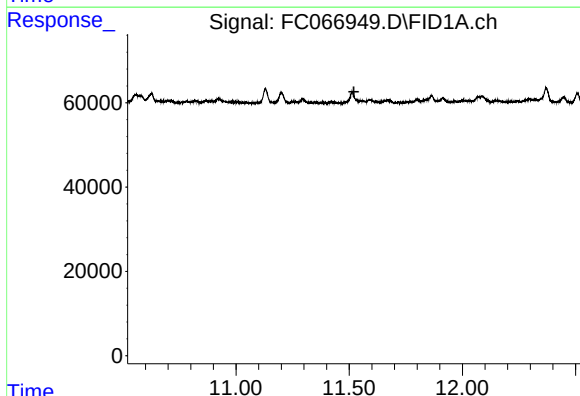

#9 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.521 min
Response: 0
Conc: N.D.

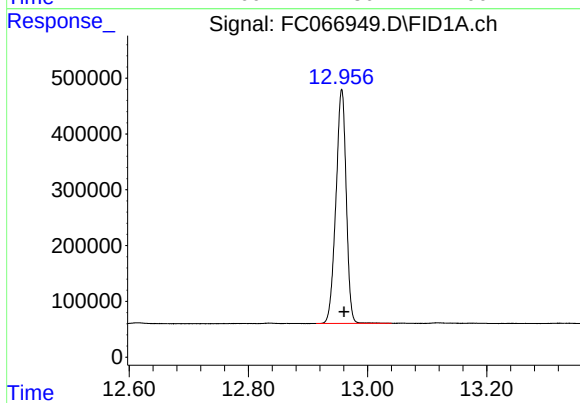

#12 1-chlorooctadecane (SURRE)

R.T.: 12.957 min
Delta R.T.: -0.004 min
Response: 5038361
Conc: 45.06 ug/ml