

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC081123AL\
Data File : FC064350.D
Signal(s) : FID1A.ch
Acq On : 11 Aug 2023 09:14
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 12 01:19:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 072323.M
Quant Title : GC Extractables
QLast Update : Mon Jul 24 01:54:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.494	205626	1.461 ug/ml
20) T	n-Hexatriacontane (C36)	20.041	260797	1.922 ug/ml
22) T	n-Tetracontane (C40)	21.653	802714	5.976 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC081123AL\
Data File : FC064350.D
Signal(s) : FID1A.ch
Acq On : 11 Aug 2023 09:14
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 12 01:19:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 072323.M
Quant Title : GC Extractables
QLast Update : Mon Jul 24 01:54:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

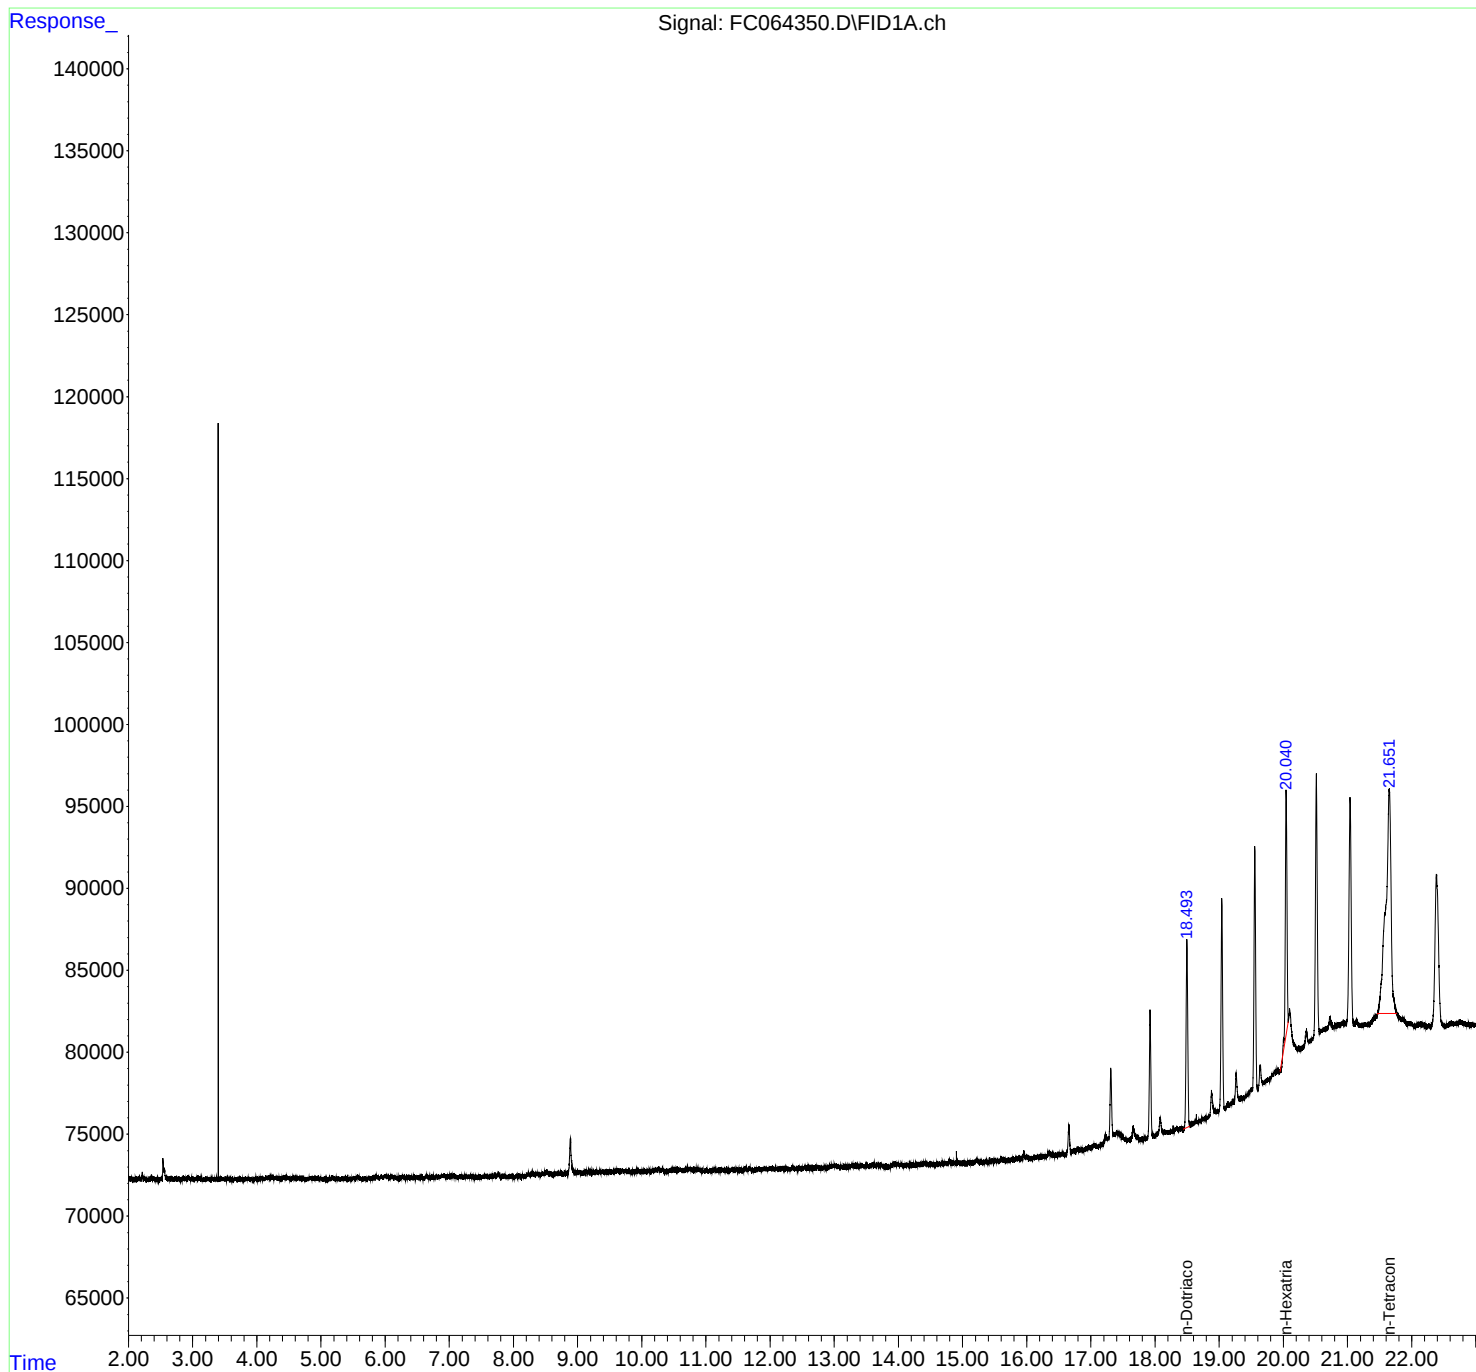


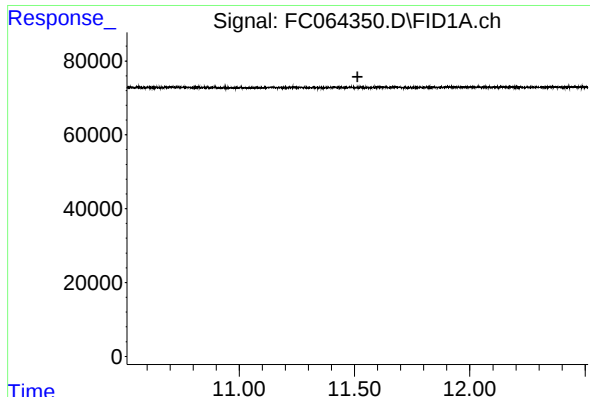

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.513 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

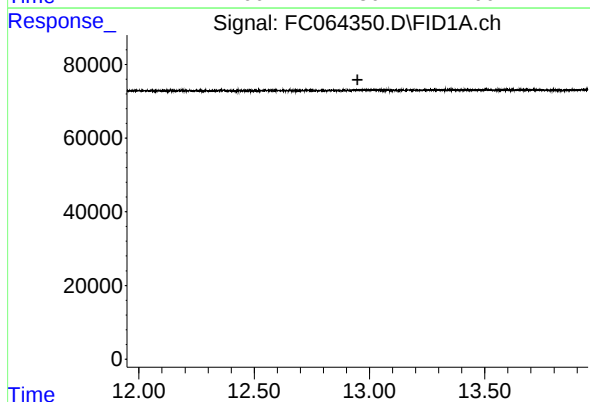


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.948 min
Response: 0
Conc: N.D.

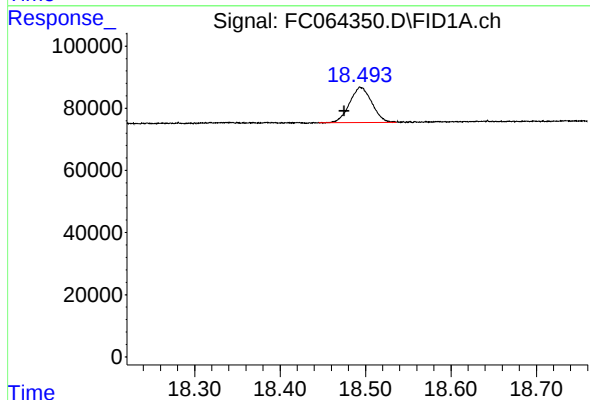


#18 n-Dotriacontane (C32)

R.T.: 18.494 min
Delta R.T.: 0.019 min
Response: 205626
Conc: 1.46 ug/ml

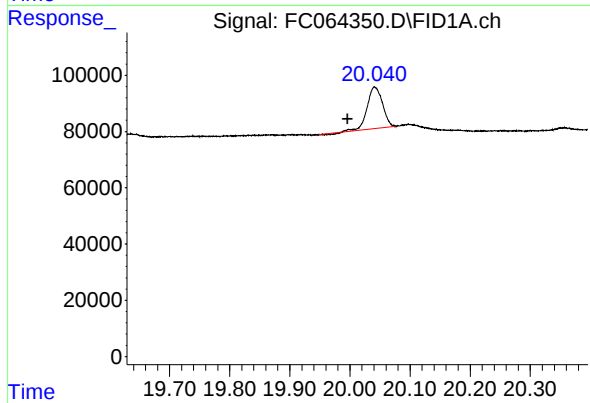

#20 n-Hexatriacontane (C36)

R.T.: 20.041 min
Delta R.T.: 0.045 min
Response: 260797
Conc: 1.92 ug/ml

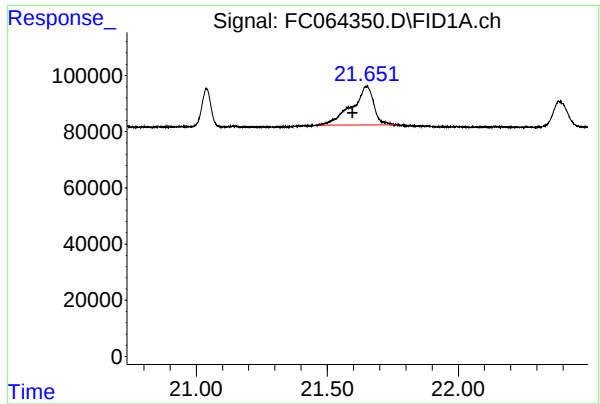

#22 n-Tetracontane (C40)

R.T.: 21.653 min
Delta R.T.: 0.056 min
Response: 802714
Conc: 5.98 ug/ml

Instrument :
FID_C
ClientSampleId :