

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC081123AL\
 Data File : FC064353.D
 Signal(s) : FID1A.ch
 Acq On : 11 Aug 2023 14:14
 Operator : YP/AJ
 Sample : PB154746BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 12 01:19:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 072323.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 24 01:54:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.949	7526814	59.684 ug/ml
Spiked Amount 50.000		Recovery =	119.37%
Target Compounds			
13) T n-Docosane (C22)	13.698	186945	1.310 ug/ml
14) T n-Tetracosane (C24)	14.796	454722	3.237 ug/ml
15) T n-Hexacosane (C26)	15.814	617553	4.497 ug/ml
16) T n-Octacosane (C28)	16.760	793547	5.918 ug/ml
17) T n-Tricontane (C30)	17.644	957176	6.896 ug/ml
18) T n-Dotriacontane (C32)	18.475	909853	6.466 ug/ml
19) T n-Tetratriacontane (C34)	19.253	522831	3.766 ug/ml
20) T n-Hexatriacontane (C36)	19.992	299253	2.205 ug/ml
21) T n-Octatriacontane (C38)	20.712	150738	1.111 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC081123AL\
Data File : FC064353.D
Signal(s) : FID1A.ch
Acq On : 11 Aug 2023 14:14
Operator : YP/AJ
Sample : PB154746BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 12 01:19:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 072323.M
Quant Title : GC Extractables
QLast Update : Mon Jul 24 01:54:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

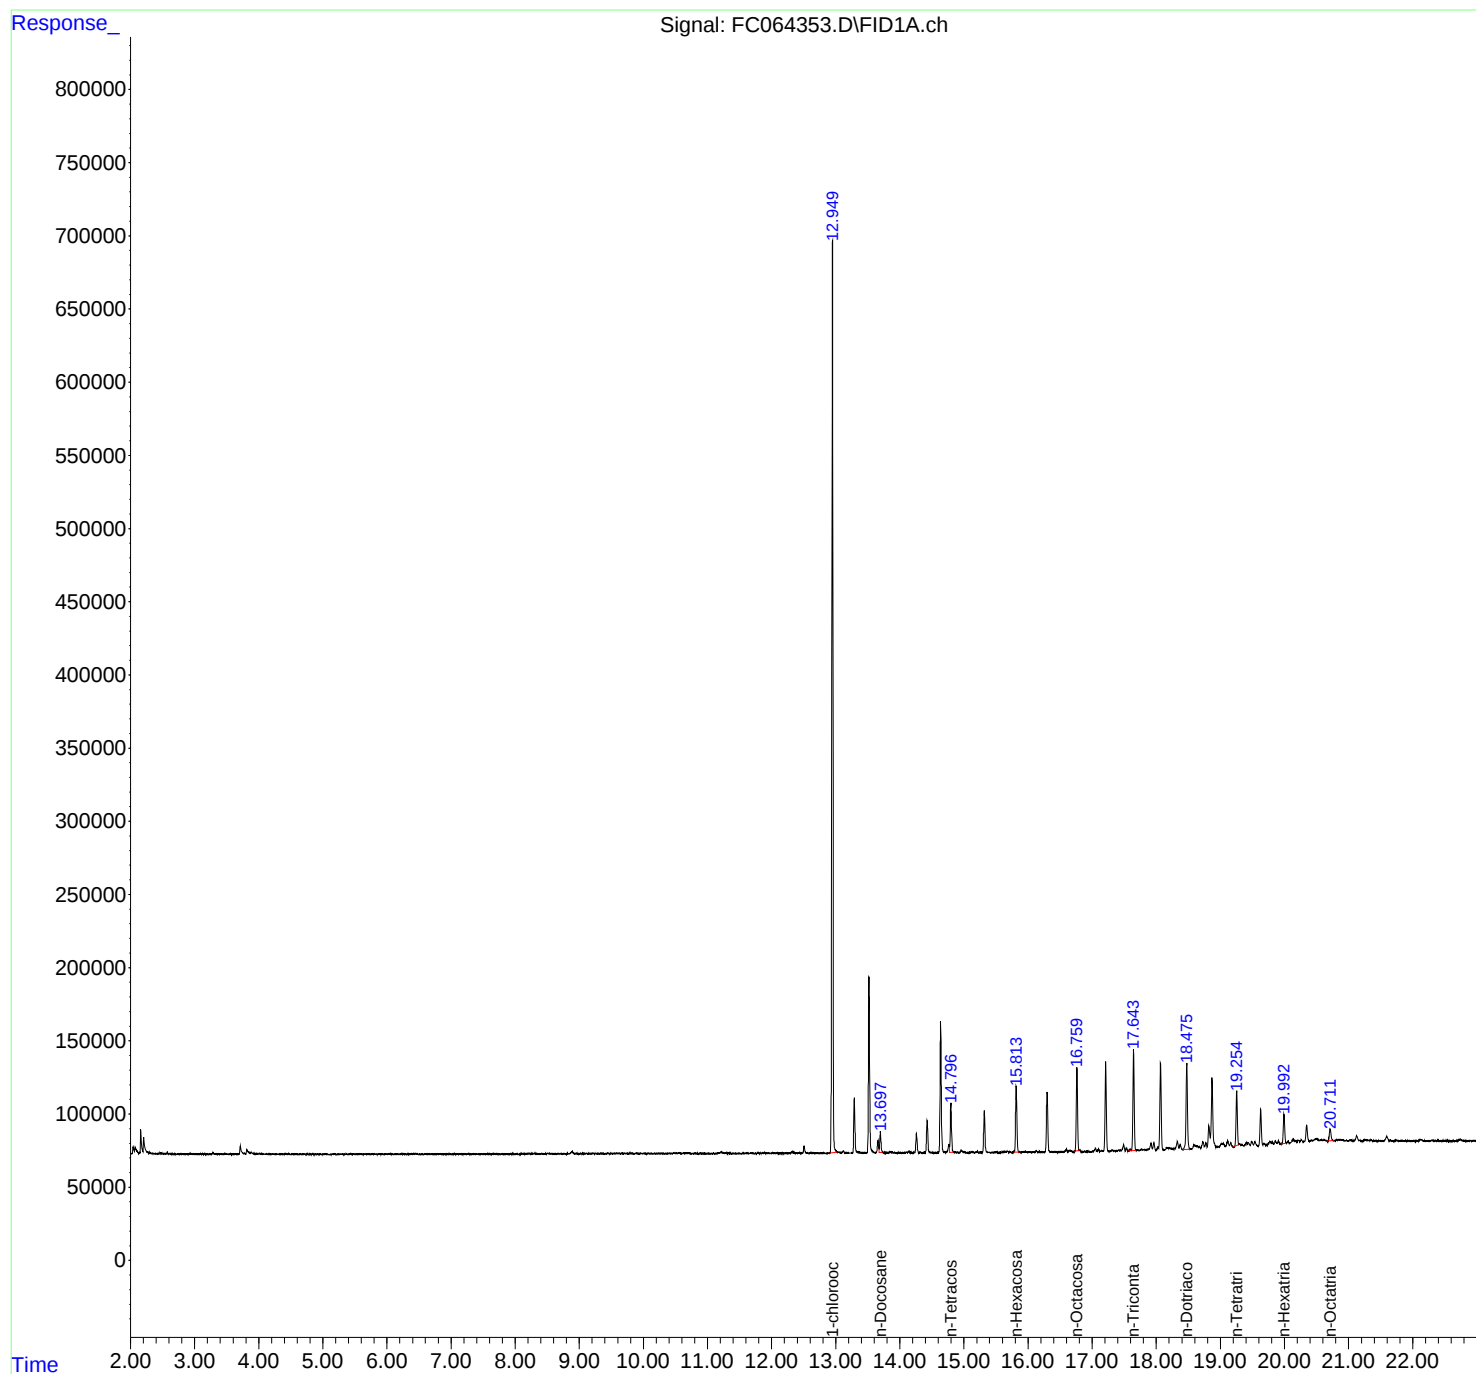


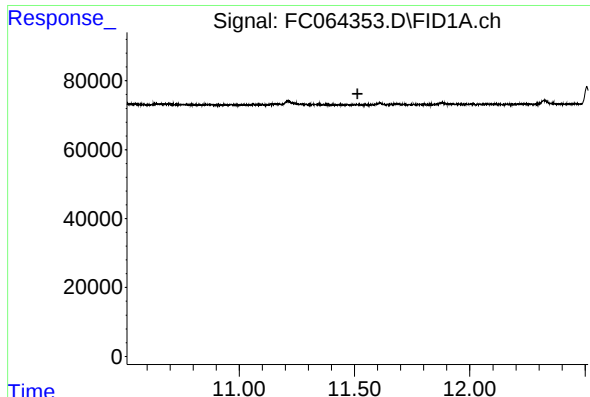

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.513 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

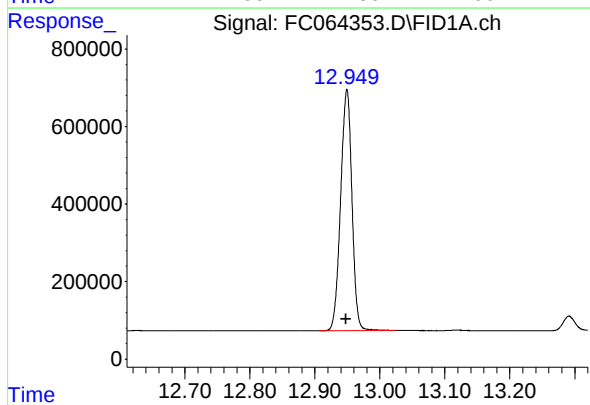


#12 1-chlorooctadecane (SURR)

R.T.: 12.949 min
Delta R.T.: 0.001 min
Response: 7526814
Conc: 59.68 ug/ml

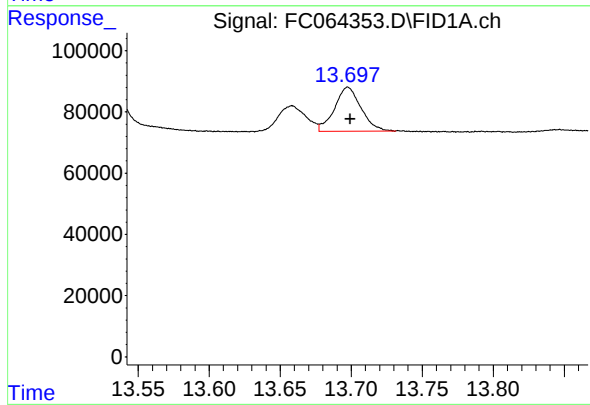


#13 n-Docosane (C22)

R.T.: 13.698 min
Delta R.T.: -0.002 min
Response: 186945
Conc: 1.31 ug/ml

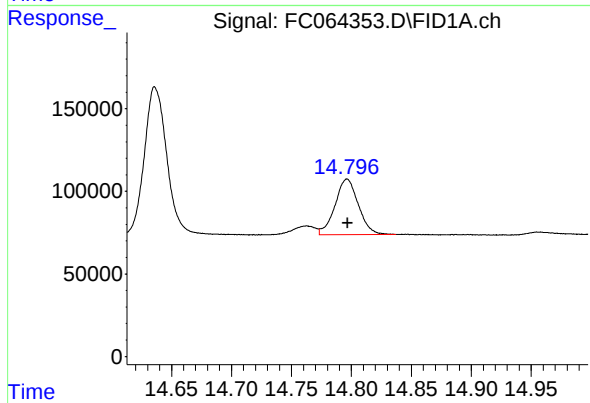

#14 n-Tetracosane (C24)


R.T.: 14.796 min
Delta R.T.: 0.000 min
Response: 454722
Conc: 3.24 ug/ml

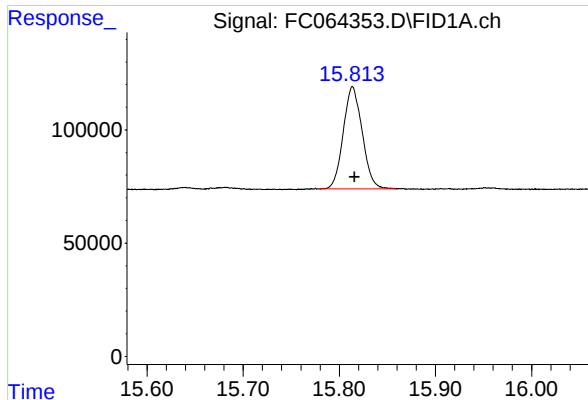

#15 n-Hexacosane (C26)


R.T.: 15.814 min
Delta R.T.: -0.002 min
Response: 617553
Conc: 4.50 ug/ml

Instrument :
FID_C
ClientSampleId :

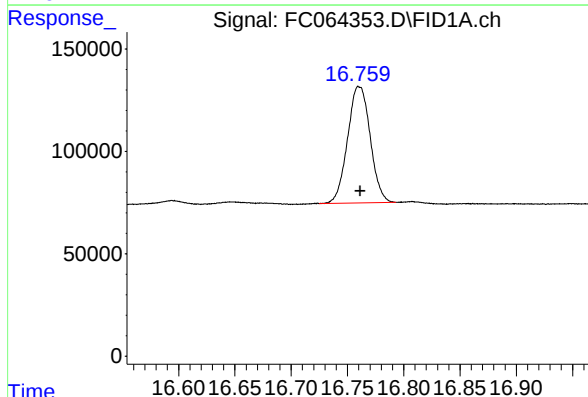


#16 n-Octacosane (C28)

R.T.: 16.760 min
Delta R.T.: -0.001 min
Response: 793547
Conc: 5.92 ug/ml

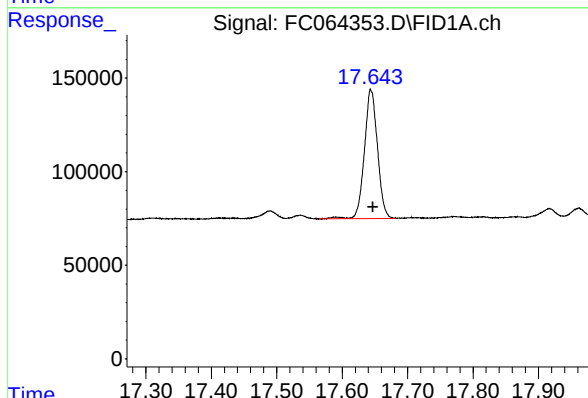


#17 n-Tricontane (C30)

R.T.: 17.644 min
Delta R.T.: -0.003 min
Response: 957176
Conc: 6.90 ug/ml

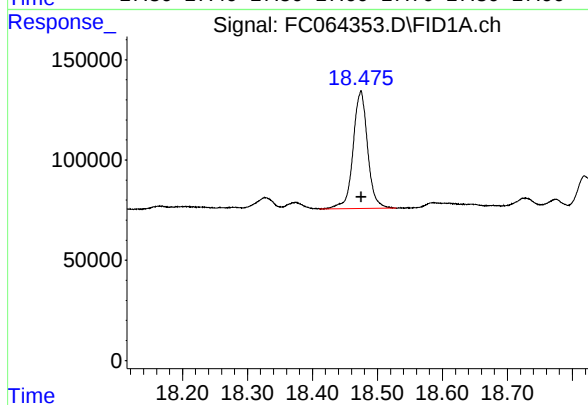

#18 n-Dotriacontane (C32)


R.T.: 18.475 min
Delta R.T.: 0.000 min
Response: 909853
Conc: 6.47 ug/ml

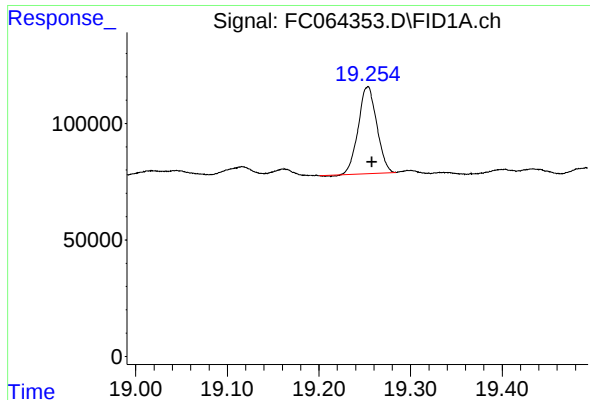

#19 n-Tetratriacontane (C34)


R.T.: 19.253 min
Delta R.T.: -0.004 min
Response: 522831
Conc: 3.77 ug/ml

Instrument :
FID_C
ClientSampleId :

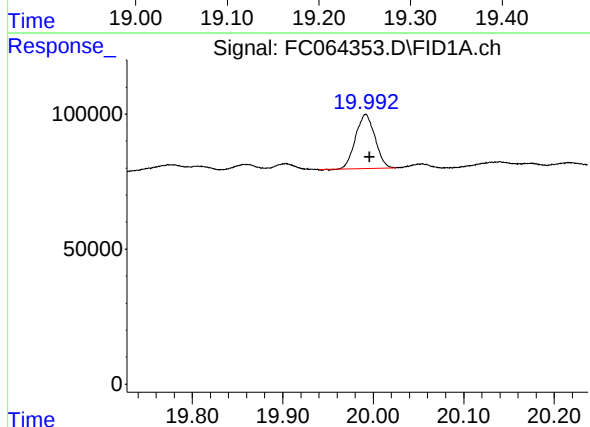

#20 n-Hexatriacontane (C36)

R.T.: 19.992 min
Delta R.T.: -0.004 min
Response: 299253
Conc: 2.21 ug/ml

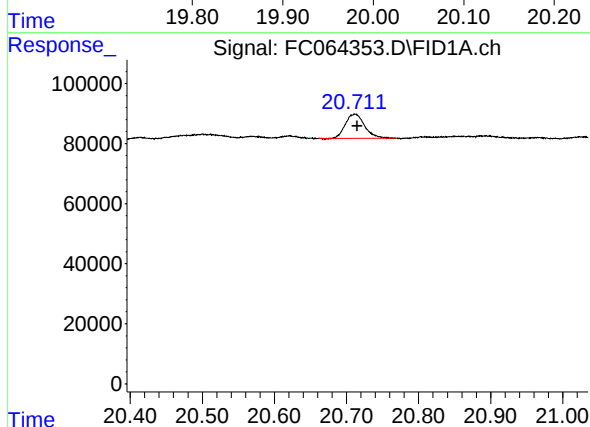

#21 n-Octatriacontane (C38)

R.T.: 20.712 min
Delta R.T.: -0.003 min
Response: 150738
Conc: 1.11 ug/ml