

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC081222AL\
Data File : FC061096.D
Signal(s) : FID1A.ch
Acq On : 12 Aug 2022 16:05
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 14 22:22:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 072522.M
Quant Title : GC Extractables
QLast Update : Mon Jul 25 19:40:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
20) T	n-Hexatriacontane (C36)	18.832f	207260	1.696 ug/ml
21) T	n-Octatriacontane (C38)	19.620	138310	1.172 ug/ml
22) T	n-Tetracontane (C40)	20.238	11340	0.099 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC081222AL\
Data File : FC061096.D
Signal(s) : FID1A.ch
Acq On : 12 Aug 2022 16:05
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 14 22:22:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 072522.M
Quant Title : GC Extractables
QLast Update : Mon Jul 25 19:40:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

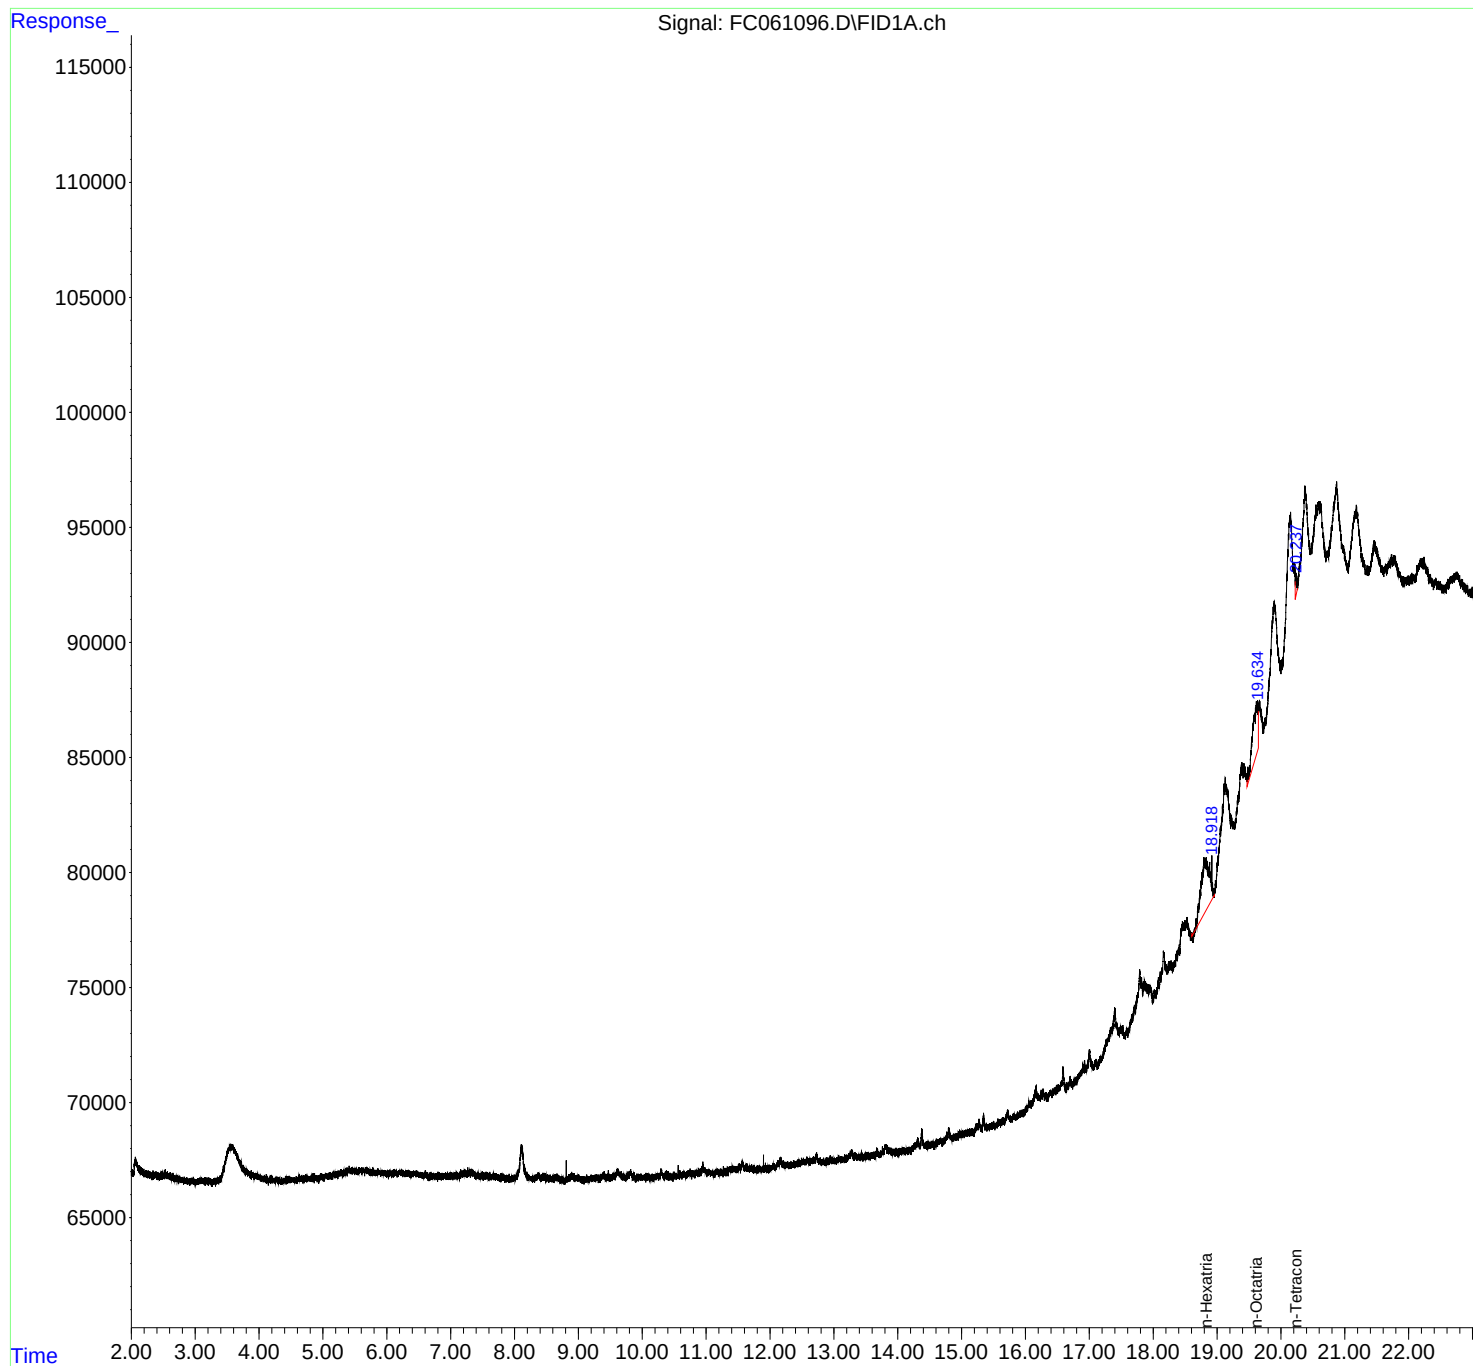


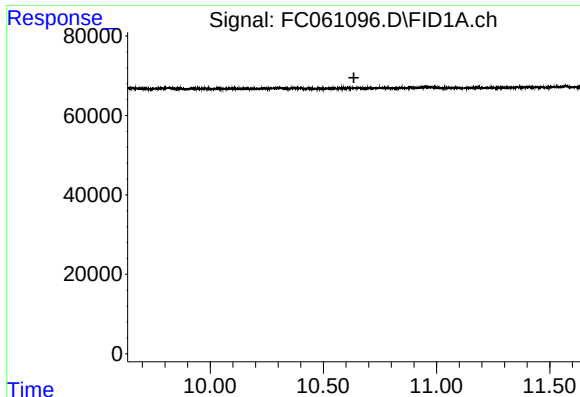

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.635 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

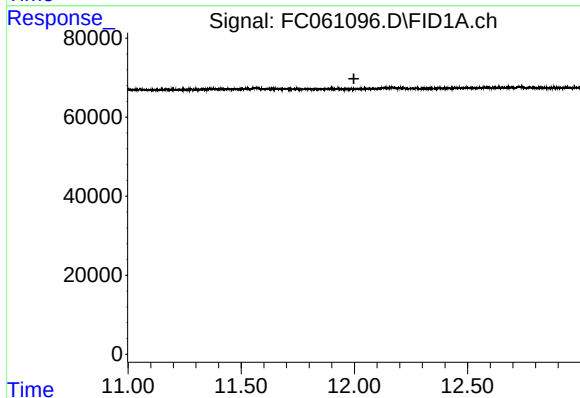


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 11.998 min
Response: 0
Conc: N.D.

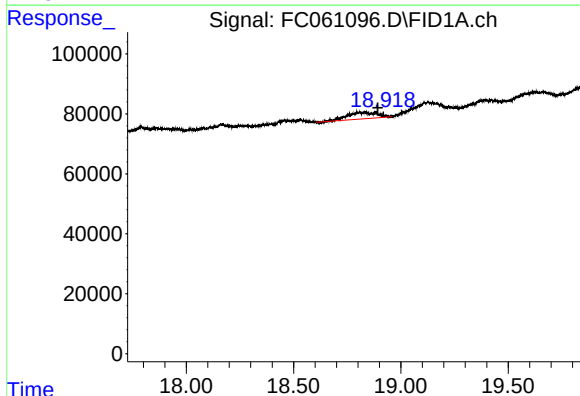


#20 n-Hexatriacontane (C36)

R.T.: 18.832 min
Delta R.T.: -0.060 min
Response: 207260
Conc: 1.70 ug/ml

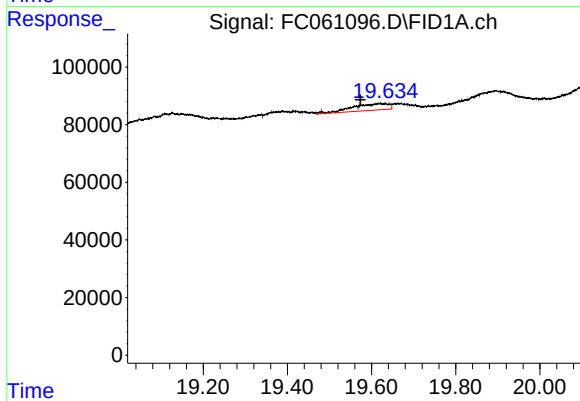

#21 n-Octatriacontane (C38)

R.T.: 19.620 min
Delta R.T.: 0.047 min
Response: 138310
Conc: 1.17 ug/ml

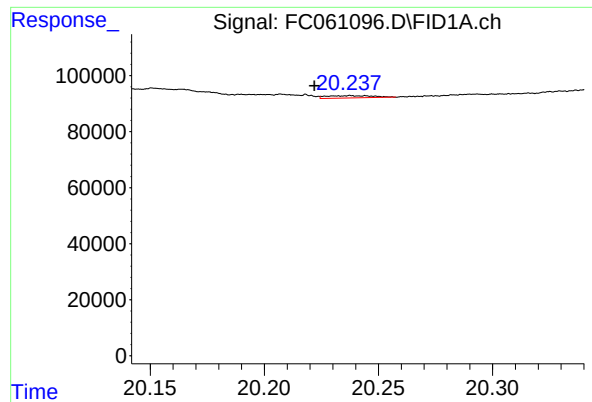

#22 n-Tetracontane (C40)

R.T.: 20.238 min
Delta R.T.: 0.016 min
Response: 11340
Conc: 0.10 ug/ml

Instrument :

FID_C

ClientSampleId :