

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC081320AL\
 Data File : FC048988.D
 Signal(s) : FID1A.CH
 Acq On : 13 Aug 2020 19:05
 Operator : DD\AJ
 Sample : PB130944BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 PB130944BL

Integration File: autoint1.e
 Quant Time: Aug 14 03:15:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 080720.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 08 02:38:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.112	1939106	19.933 ug/ml
Spiked Amount 50.000		Recovery =	39.87%
Target Compounds			
15) T n-Hexacosane (C26)	16.035	28907	0.253 ug/ml
19) T n-Tetratriacontane (C34)	19.462	98366	0.948 ug/ml
20) T n-Hexatriacontane (C36)	20.166	298310	3.000 ug/ml
21) T n-Octatriacontane (C38)	20.978f	8771	0.093 ug/ml
22) T n-Tetracontane (C40)	21.848	346201	3.626 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC081320AL\
Data File : FC048988.D
Signal(s) : FID1A.CH
Acq On : 13 Aug 2020 19:05
Operator : DD\AJ
Sample : PB130944BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_C
ClientSampled :
PB130944BL

Integration File: autoint1.e
Quant Time: Aug 14 03:15:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 080720.M
Quant Title : GC Extractables
QLast Update : Sat Aug 08 02:38:47 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

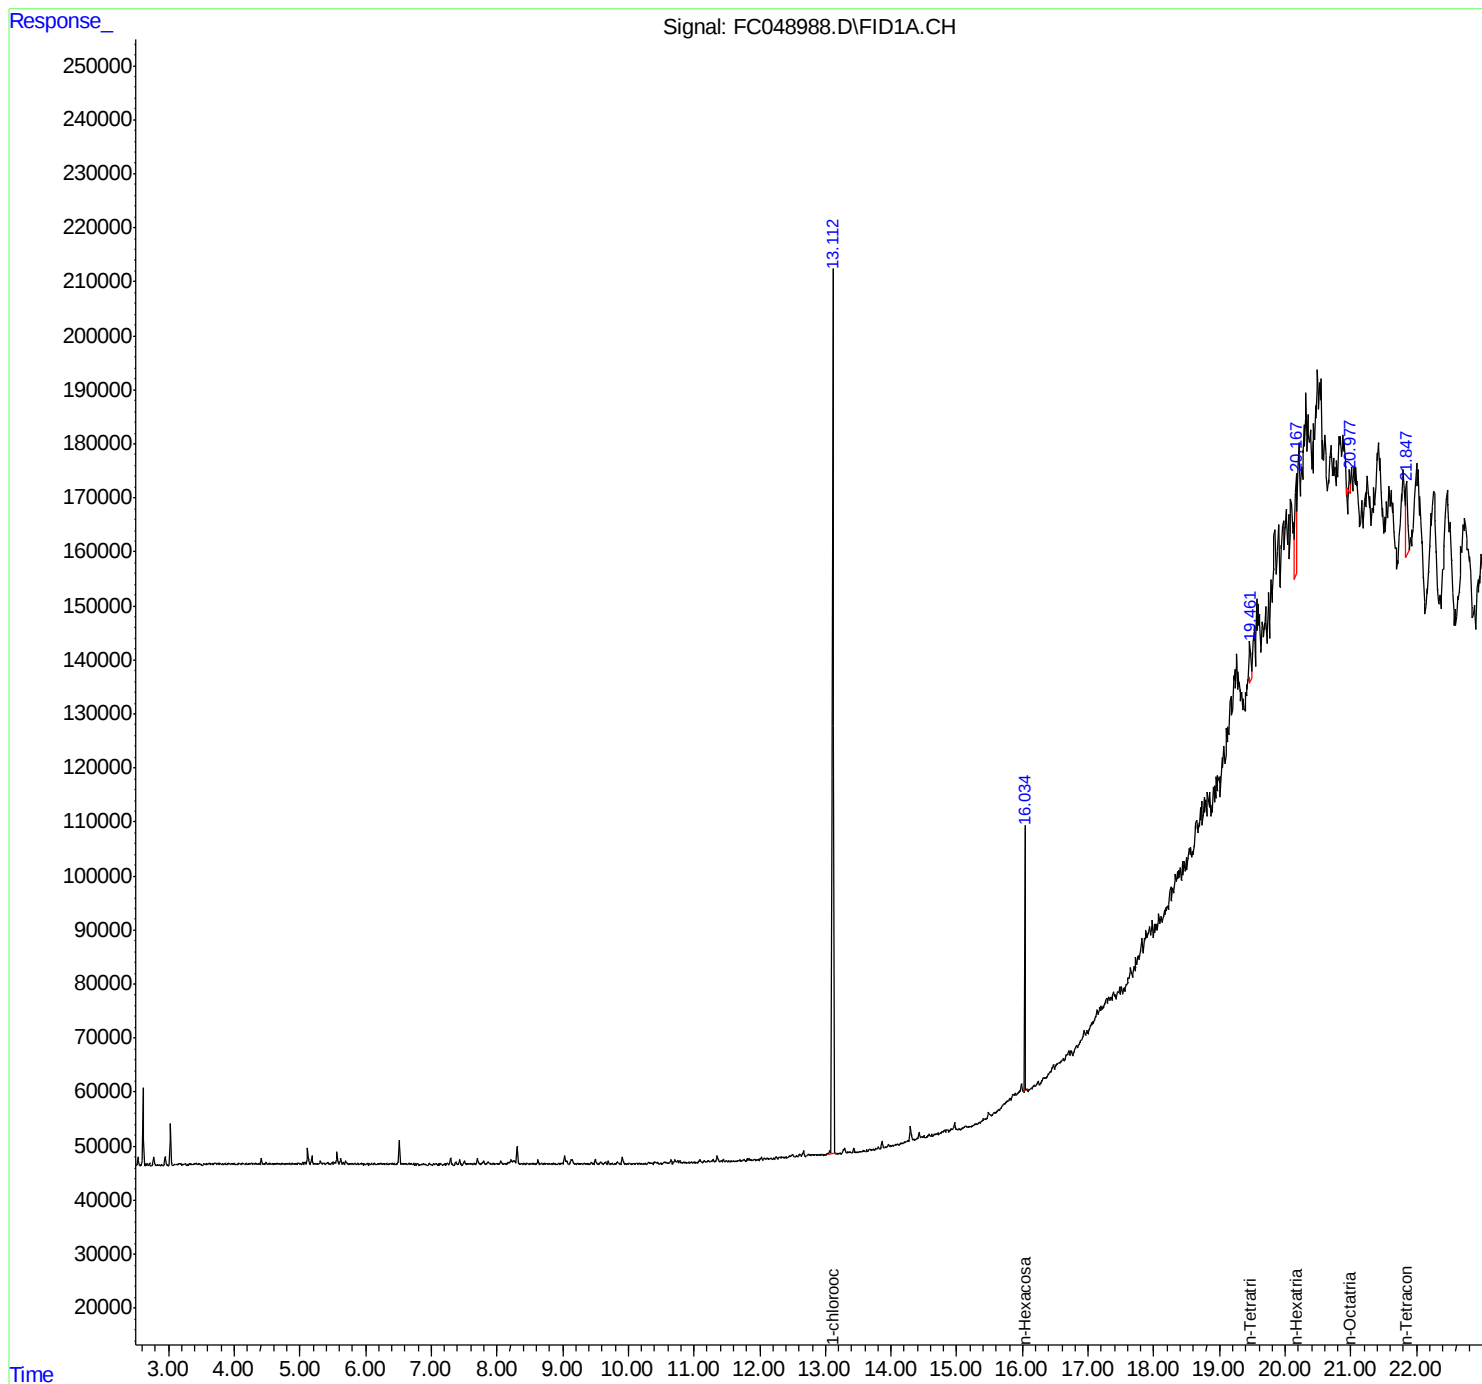


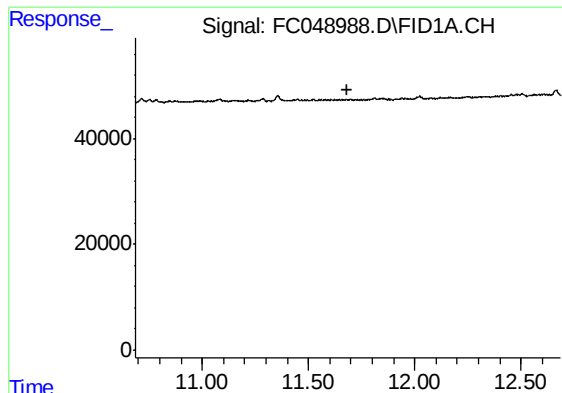

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.685 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
PB130944BL

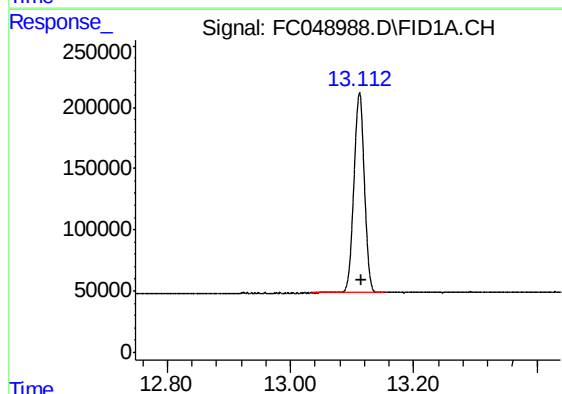


#12 1-chlorooctadecane (SURR)

R.T.: 13.112 min
Delta R.T.: -0.003 min
Response: 1939106
Conc: 19.93 ug/ml

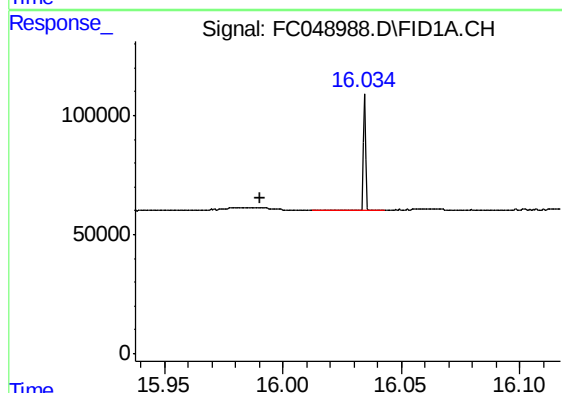


#15 n-Hexacosane (C26)

R.T.: 16.035 min
Delta R.T.: 0.044 min
Response: 28907
Conc: 0.25 ug/ml

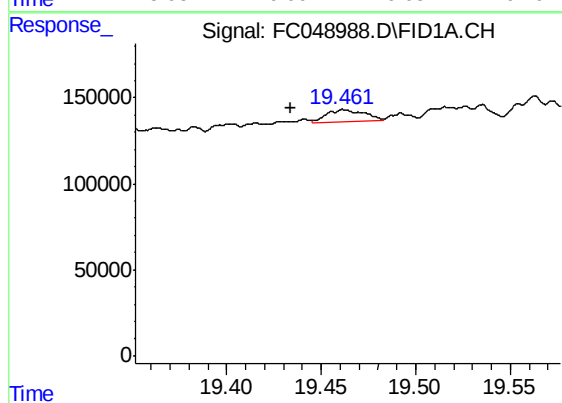

#19 n-Tetratriacontane (C34)


R.T.: 19.462 min
Delta R.T.: 0.028 min
Response: 98366
Conc: 0.95 ug/ml

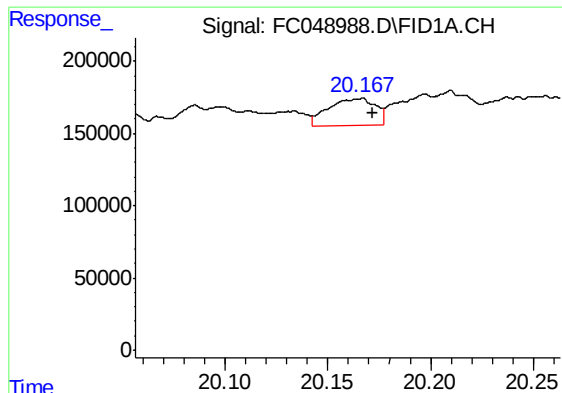

#20 n-Hexatriacontane (C36)


R.T.: 20.166 min
Delta R.T.: -0.006 min
Response: 298310
Conc: 3.00 ug/ml

Instrument :
FID_C
ClientSampleId :
PB130944BL

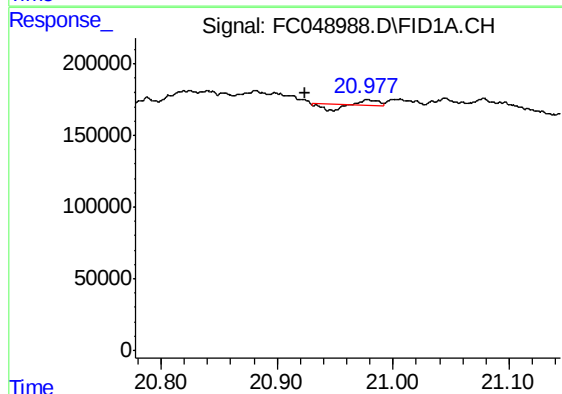

#21 n-Octatriacontane (C38)

R.T.: 20.978 min
Delta R.T.: 0.054 min
Response: 8771
Conc: 0.09 ug/ml

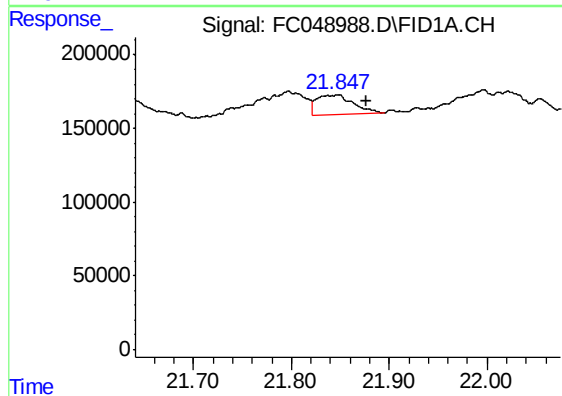

#22 n-Tetracontane (C40)

R.T.: 21.848 min
Delta R.T.: -0.029 min
Response: 346201
Conc: 3.63 ug/ml