

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC081524AL\
 Data File : FC067002.D
 Signal(s) : FID1A.ch
 Acq On : 15 Aug 2024 09:50
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 16 02:03:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 081224.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 15:57:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) T n-Heneicosane (C21)	13.115	132647	0.995 ug/ml
13) T n-Docosane (C22)	13.699	75391	0.572 ug/ml
14) T n-Tetracosane (C24)	14.802	62998	0.486 ug/ml
15) T n-Hexacosane (C26)	15.838	183158	1.444 ug/ml
16) T n-Octacosane (C28)	16.719f	61947	0.499 ug/ml
17) T n-Tricontane (C30)	17.597f	86801	0.691 ug/ml
19) T n-Tetratriacontane (C34)	19.241	288273	2.404 ug/ml
20) T n-Hexatriacontane (C36)	20.014	68031	0.603 ug/ml
21) T n-Octatriacontane (C38)	20.738	63496	0.583 ug/ml
22) T n-Tetracontane (C40)	21.606	172313	1.687 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC081524AL\
Data File : FC067002.D
Signal(s) : FID1A.ch
Acq On : 15 Aug 2024 09:50
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 16 02:03:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 081224.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 15:57:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

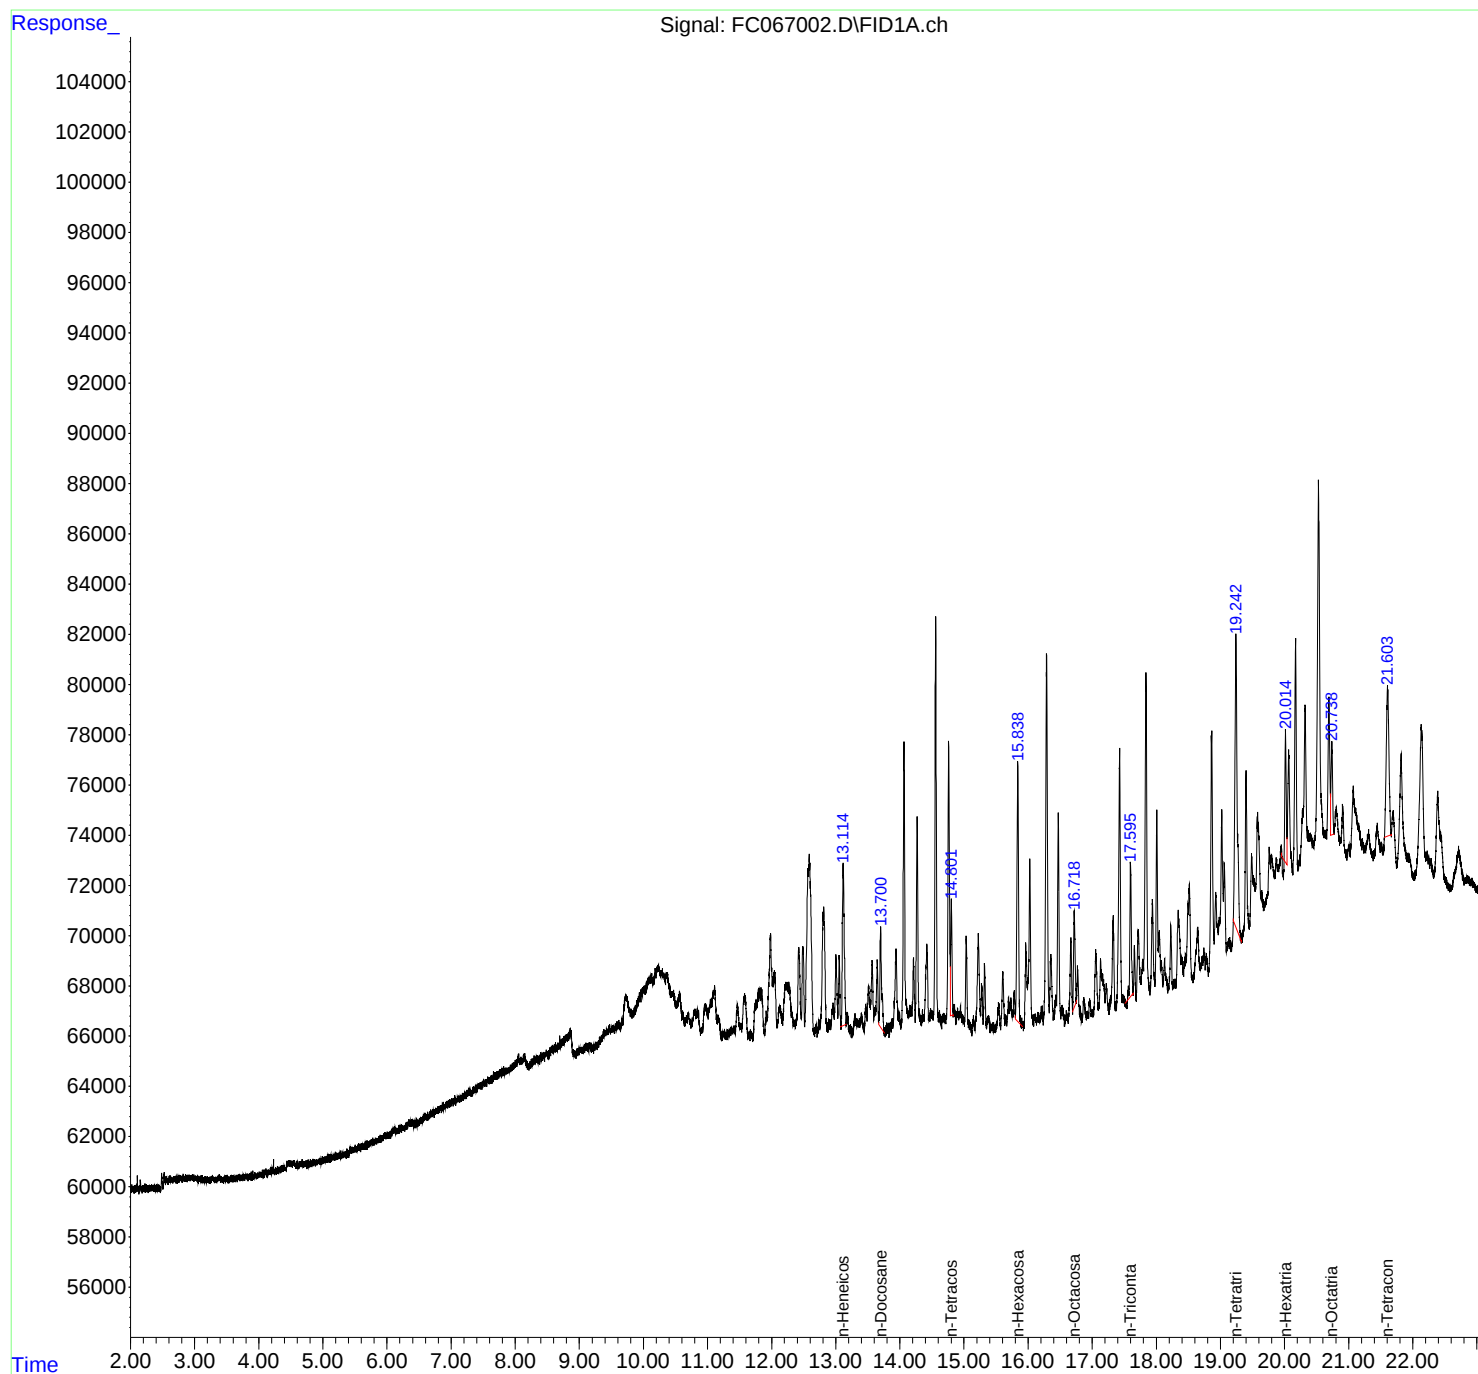


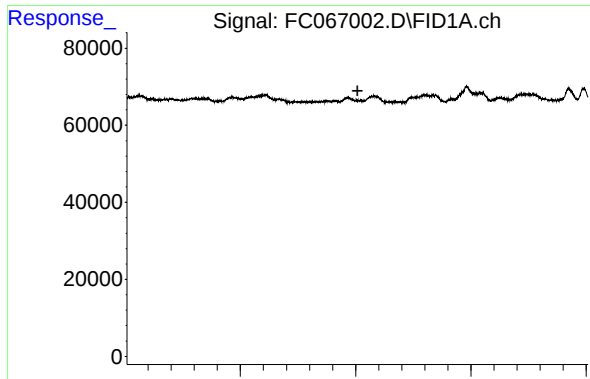

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.508 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

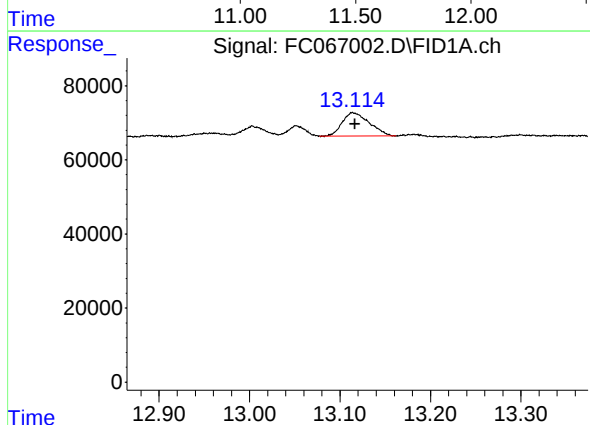


#11 n-Heneicosane (C21)

R.T.: 13.115 min
Delta R.T.: -0.001 min
Response: 132647
Conc: 1.00 ug/ml

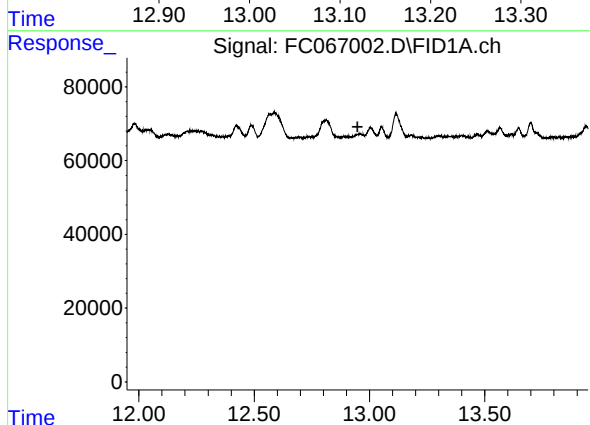


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.948 min
Response: 0
Conc: N.D.

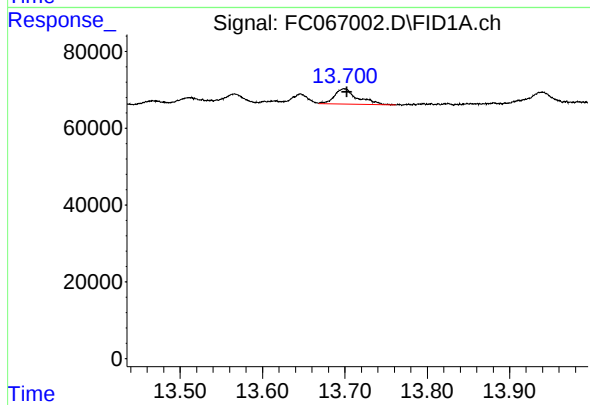

#13 n-Docosane (C22)


R.T.: 13.699 min
Delta R.T.: -0.003 min
Response: 75391
Conc: 0.57 ug/ml

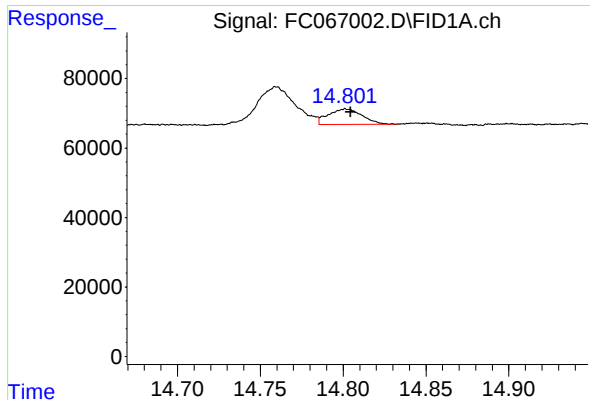

#14 n-Tetracosane (C24)


R.T.: 14.802 min
Delta R.T.: -0.003 min
Response: 62998
Conc: 0.49 ug/ml

Instrument :
FID_C
ClientSampleId :

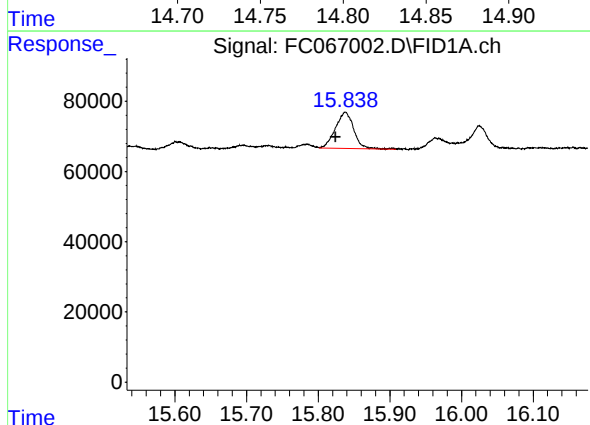


#15 n-Hexacosane (C26)

R.T.: 15.838 min
Delta R.T.: 0.014 min
Response: 183158
Conc: 1.44 ug/ml

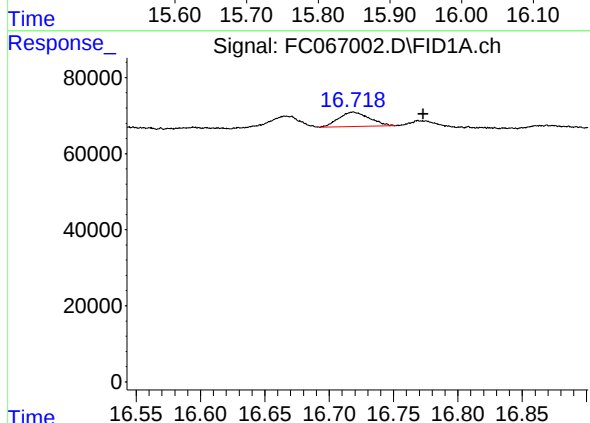


#16 n-Octacosane (C28)

R.T.: 16.719 min
Delta R.T.: -0.055 min
Response: 61947
Conc: 0.50 ug/ml

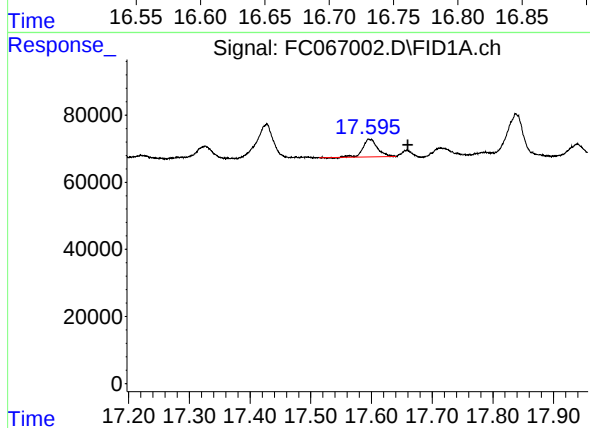

#17 n-Tricontane (C30)


R.T.: 17.597 min
Delta R.T.: -0.063 min
Response: 86801
Conc: 0.69 ug/ml

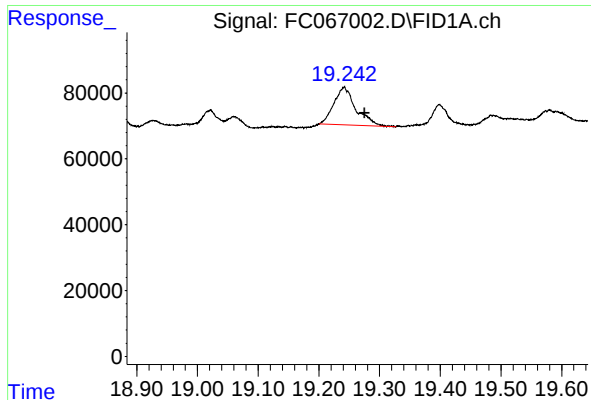

#19 n-Tetratriacontane (C34)


R.T.: 19.241 min
Delta R.T.: -0.034 min
Response: 288273
Conc: 2.40 ug/ml

Instrument :
FID_C
ClientSampleId :

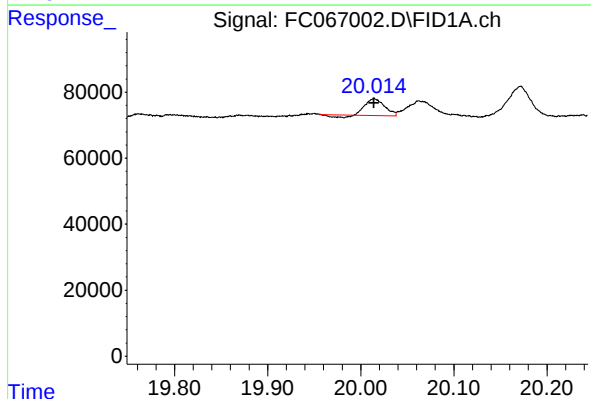


#20 n-Hexatriacontane (C36)

R.T.: 20.014 min
Delta R.T.: 0.000 min
Response: 68031
Conc: 0.60 ug/ml

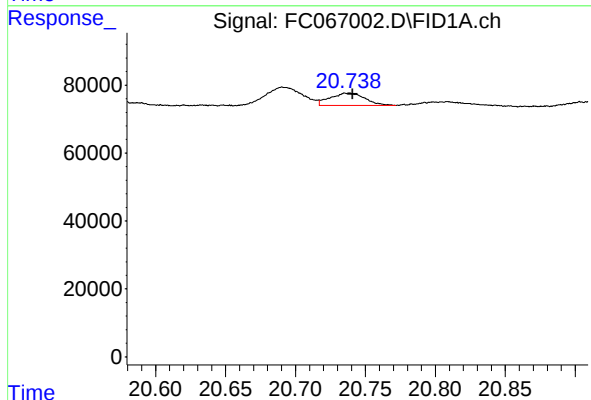

#21 n-Octatriacontane (C38)

R.T.: 20.738 min
Delta R.T.: -0.003 min
Response: 63496
Conc: 0.58 ug/ml

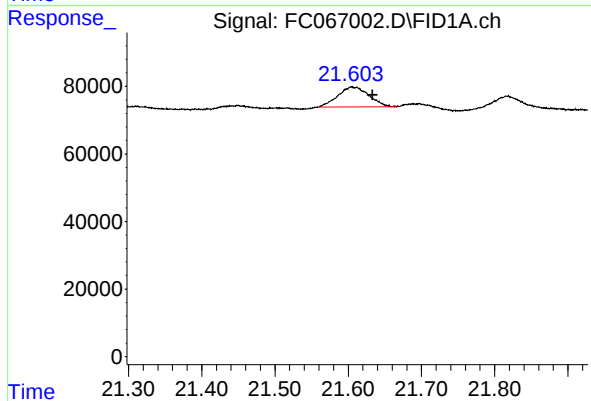

#22 n-Tetracontane (C40)

R.T.: 21.606 min
Delta R.T.: -0.027 min
Response: 172313
Conc: 1.69 ug/ml