

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC081722AL\
 Data File : FC061176.D
 Signal(s) : FID1A.ch
 Acq On : 17 Aug 2022 22:57
 Operator : YP/AJ
 Sample : N4124-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 18 00:27:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 072522.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 25 19:40:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	11.994	2771610	20.878 ug/ml
Spiked Amount 50.000		Recovery =	41.76%
Target Compounds			
17) T n-Tricontane (C30)	16.559	246831	1.763 ug/ml
18) T n-Dotriacontane (C32)	17.399	82560	0.612 ug/ml
19) T n-Tetratriacontane (C34)	18.162	124081	0.989 ug/ml
20) T n-Hexatriacontane (C36)	18.879	86699	0.709 ug/ml
21) T n-Octatriacontane (C38)	19.562	53788	0.456 ug/ml
22) T n-Tetracontane (C40)	20.210	140386	1.220 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC081722AL\
Data File : FC061176.D
Signal(s) : FID1A.ch
Acq On : 17 Aug 2022 22:57
Operator : YP/AJ
Sample : N4124-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 18 00:27:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 072522.M
Quant Title : GC Extractables
QLast Update : Mon Jul 25 19:40:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

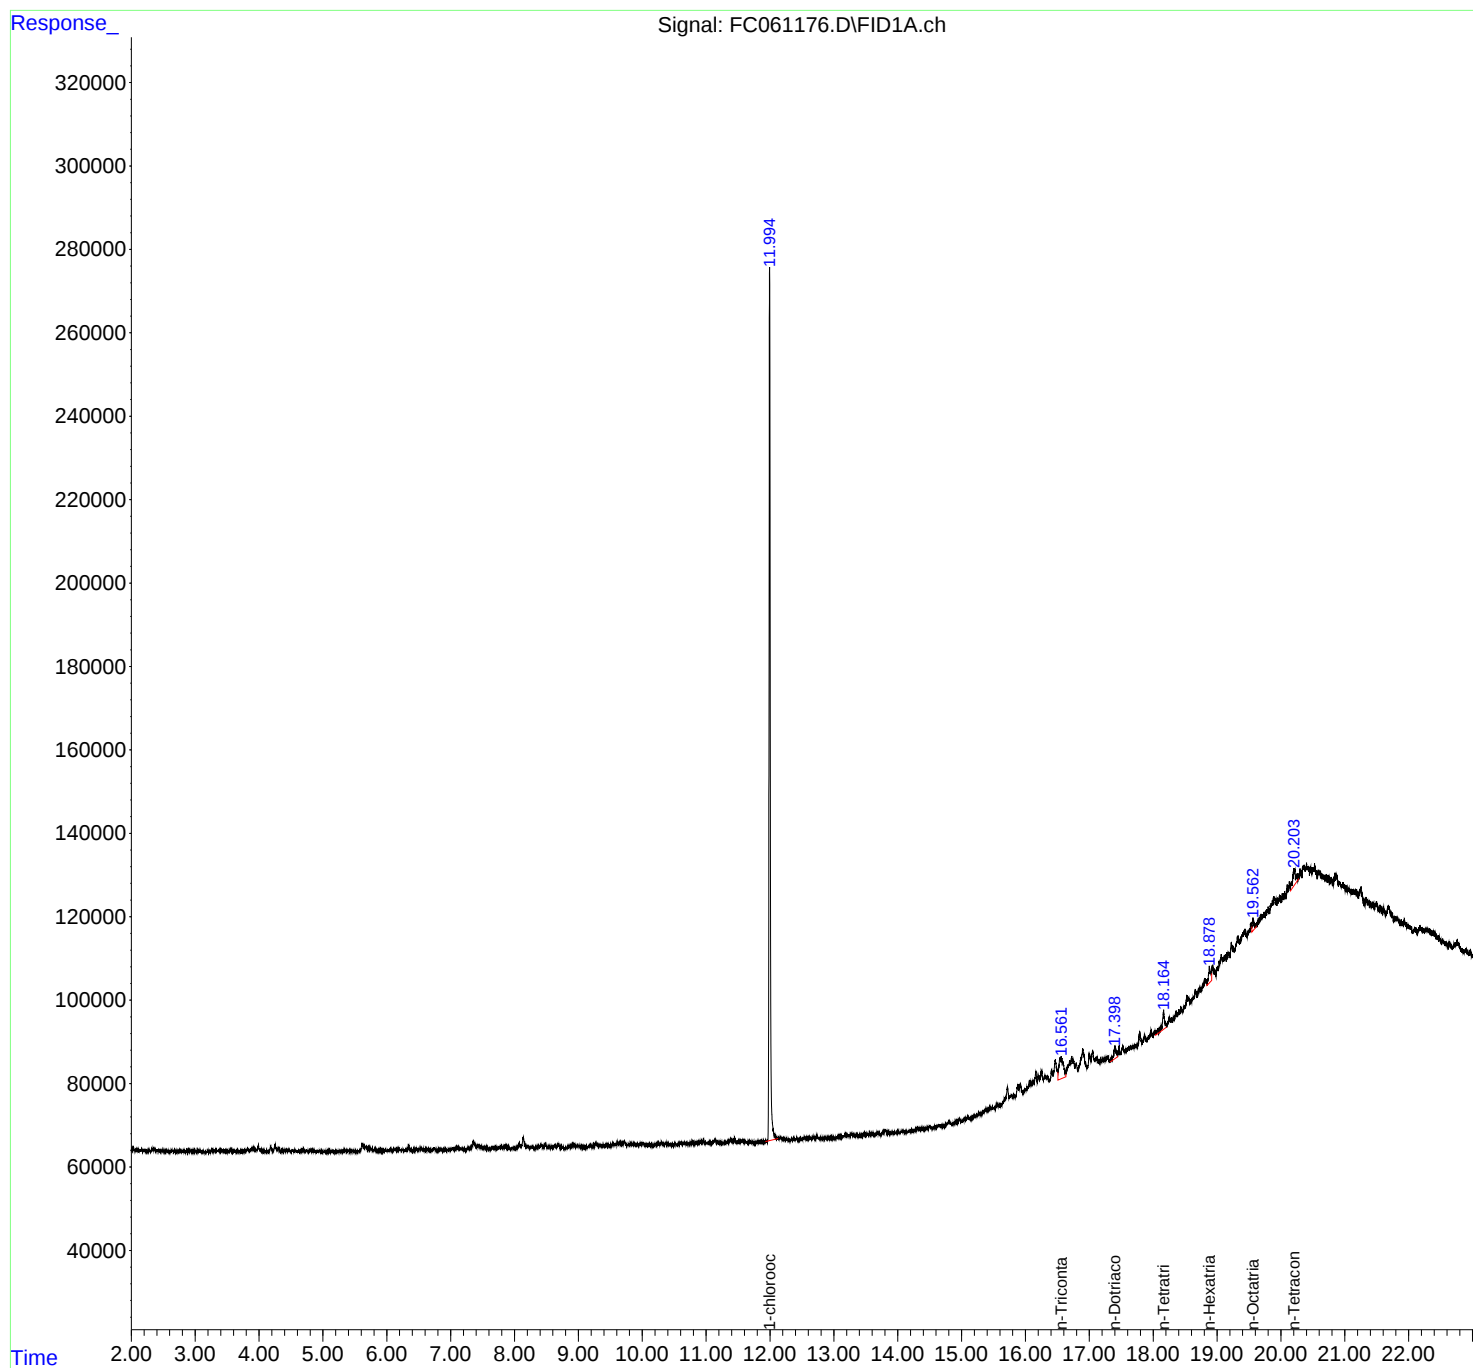


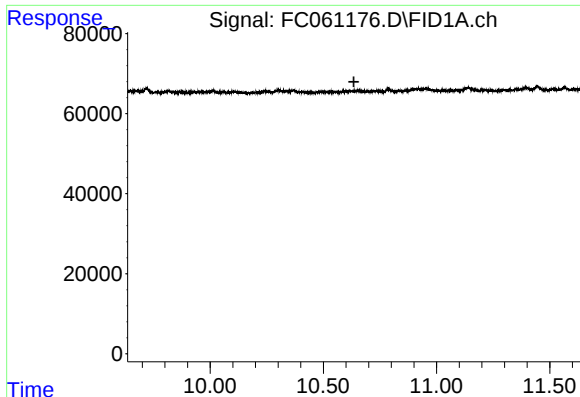

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.635 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

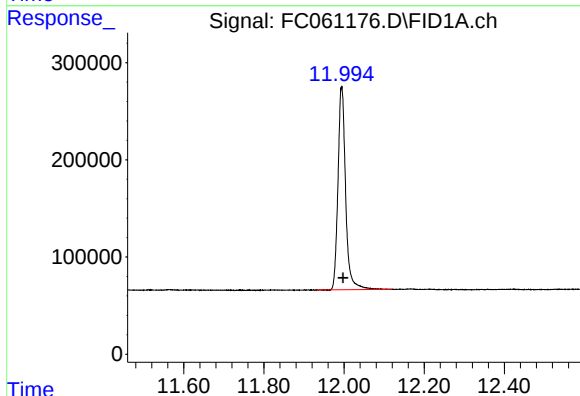


#12 1-chlorooctadecane (SURR)

R.T.: 11.994 min
Delta R.T.: -0.004 min
Response: 2771610
Conc: 20.88 ug/ml

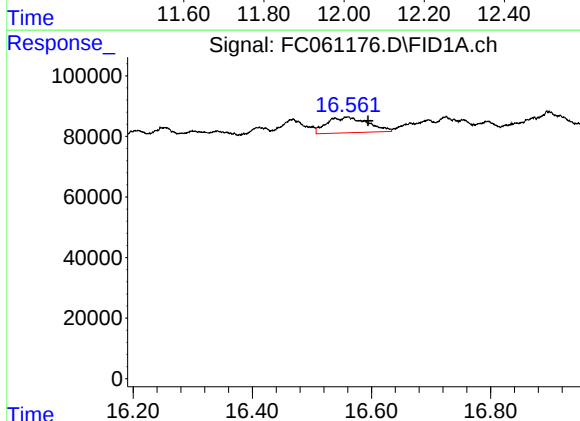


#17 n-Tricontane (C30)

R.T.: 16.559 min
Delta R.T.: -0.035 min
Response: 246831
Conc: 1.76 ug/ml

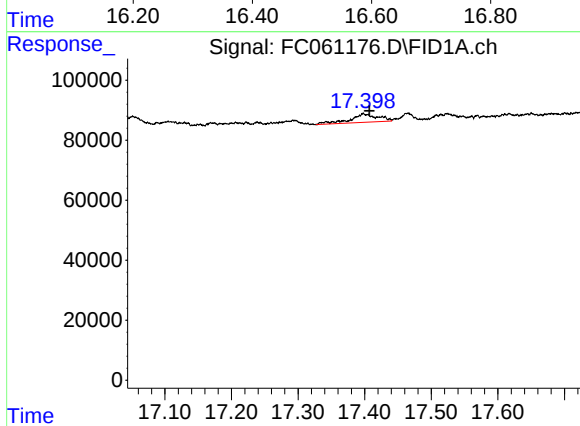

#18 n-Dotriacontane (C32)


R.T.: 17.399 min
Delta R.T.: -0.008 min
Response: 82560
Conc: 0.61 ug/ml

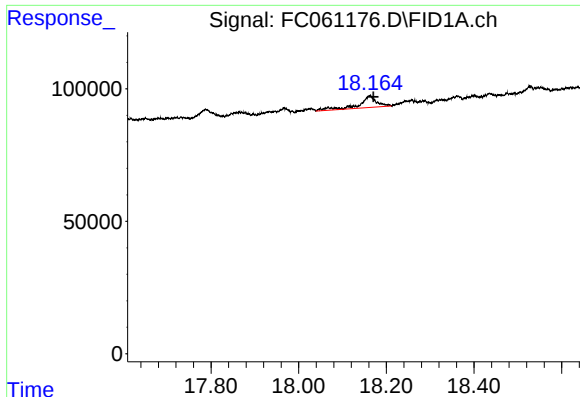

#19 n-Tetratriacontane (C34)


R.T.: 18.162 min
Delta R.T.: -0.009 min
Response: 124081
Conc: 0.99 ug/ml

Instrument :
FID_C
ClientSampleId :

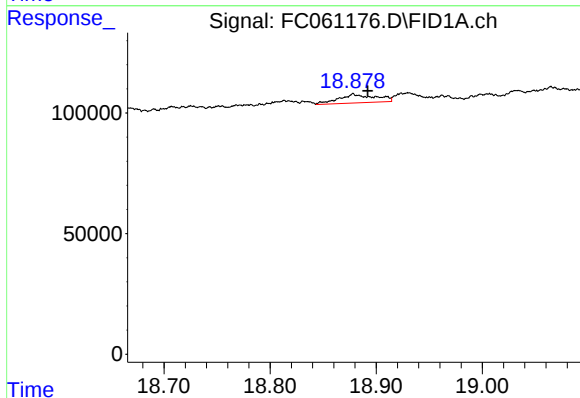


#20 n-Hexatriacontane (C36)

R.T.: 18.879 min
Delta R.T.: -0.013 min
Response: 86699
Conc: 0.71 ug/ml

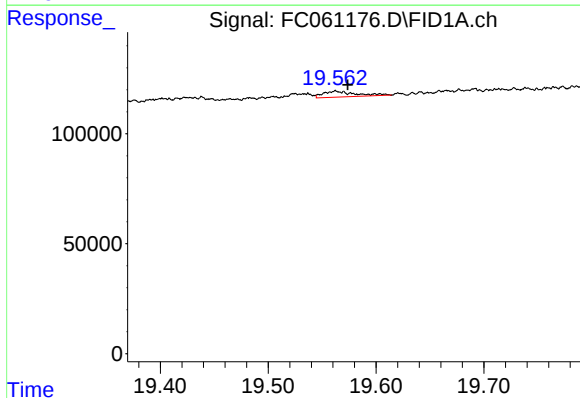

#21 n-Octatriacontane (C38)

R.T.: 19.562 min
Delta R.T.: -0.012 min
Response: 53788
Conc: 0.46 ug/ml

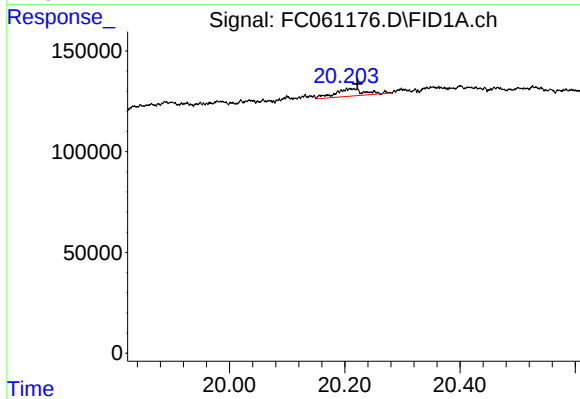

#22 n-Tetracontane (C40)

R.T.: 20.210 min
Delta R.T.: -0.012 min
Response: 140386
Conc: 1.22 ug/ml