

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC082420AL\
 Data File : FC049184.D
 Signal(s) : FID1A.CH
 Acq On : 25 Aug 2020 2:20
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Aug 25 02:57:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 080720.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 08 02:38:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T n-Dotriacontane (C32)	18.655	65054	0.602 ug/ml
20) T n-Hexatriacontane (C36)	20.138	307277	3.090 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC082420AL\
Data File : FC049184.D
Signal(s) : FID1A.CH
Acq On : 25 Aug 2020 2:20
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 25 02:57:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 080720.M
Quant Title : GC Extractables
QLast Update : Sat Aug 08 02:38:47 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

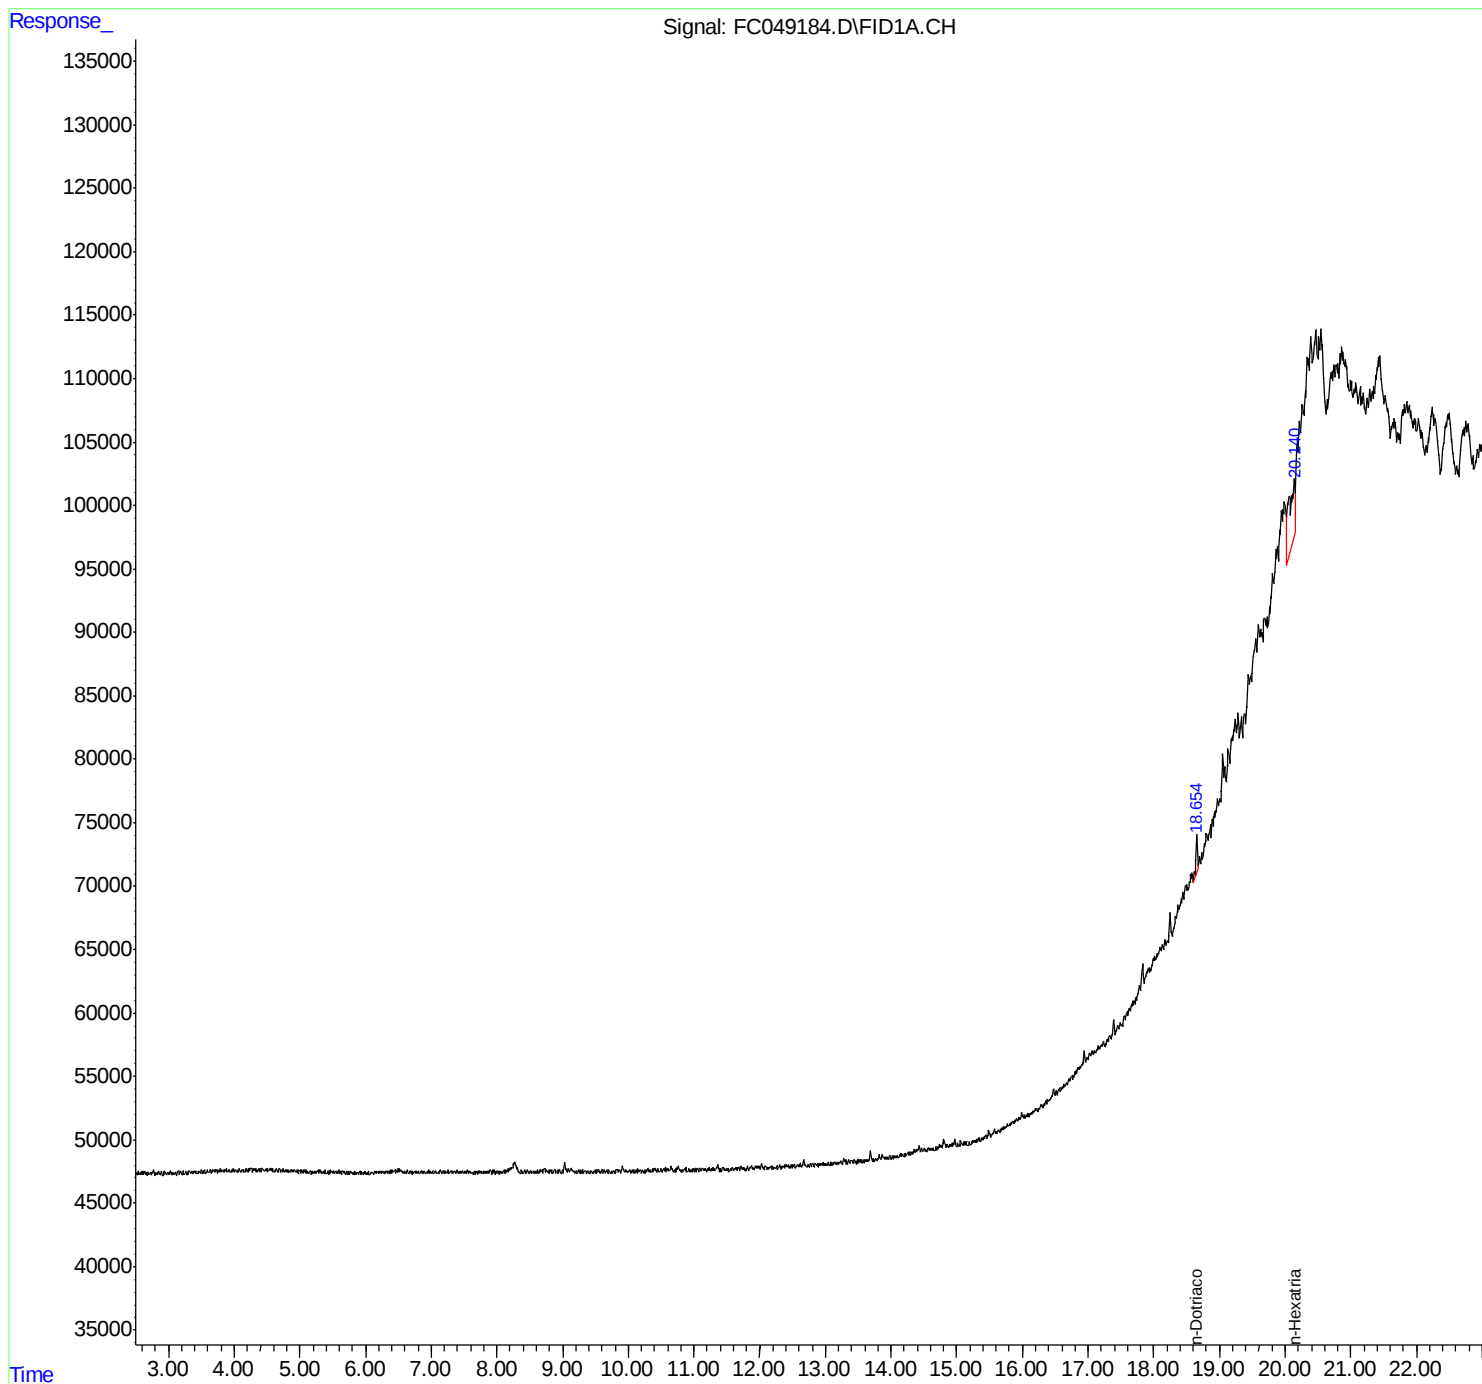


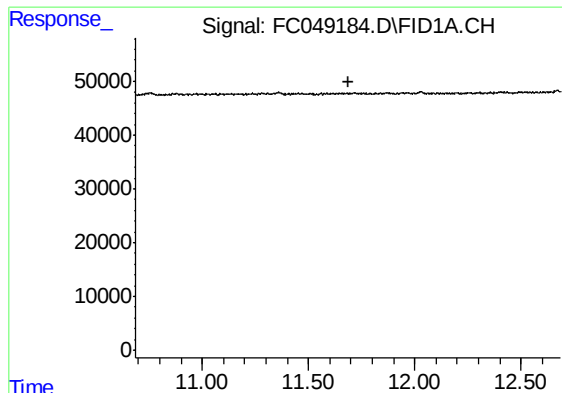

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.685 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
I.BLK

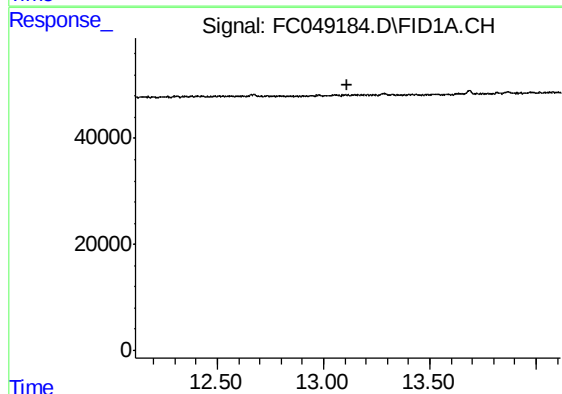


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.115 min
Response: 0
Conc: N.D.

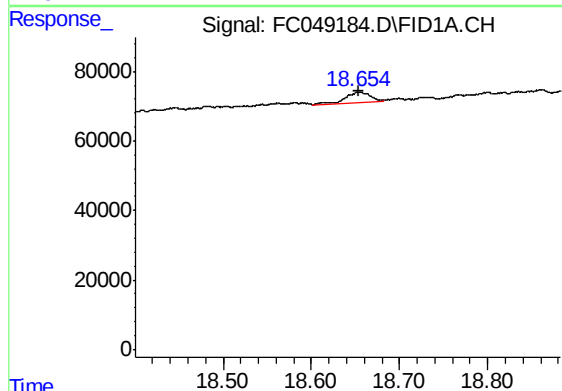

#18 n-Dotriacontane (C32)

R.T.: 18.655 min
Delta R.T.: 0.001 min
Response: 65054
Conc: 0.60 ug/ml

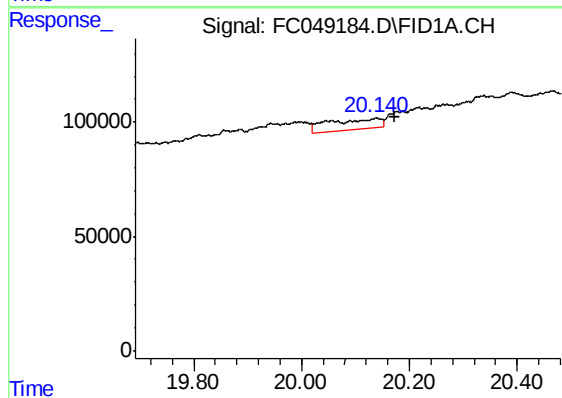

#20 n-Hexatriacontane (C36)

R.T.: 20.138 min
Delta R.T.: -0.033 min
Response: 307277
Conc: 3.09 ug/ml