

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC082622AL\
 Data File : FC061312.D
 Signal(s) : FID1A.ch
 Acq On : 26 Aug 2022 14:02
 Operator : YP/AJ
 Sample : PB143702BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 27 01:54:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:32:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.073	4325098	30.883 ug/ml
Spiked Amount 50.000		Recovery =	61.77%
Target Compounds			
4) T n-Dodecane (C12)	6.489	172510	1.114 ug/ml
6) T n-Tetradecane (C14)	8.282	69680	0.445 ug/ml
17) T n-Tricontane (C30)	17.772	56723	0.411 ug/ml
18) T n-Dotriacontane (C32)	18.604	71748	0.654 ug/ml
19) T n-Tetratriacontane (C34)	19.386	60424	0.783 ug/ml
20) T n-Hexatriacontane (C36)	20.125	36453	0.646 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC082622AL\
Data File : FC061312.D
Signal(s) : FID1A.ch
Acq On : 26 Aug 2022 14:02
Operator : YP/AJ
Sample : PB143702BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 27 01:54:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:32:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

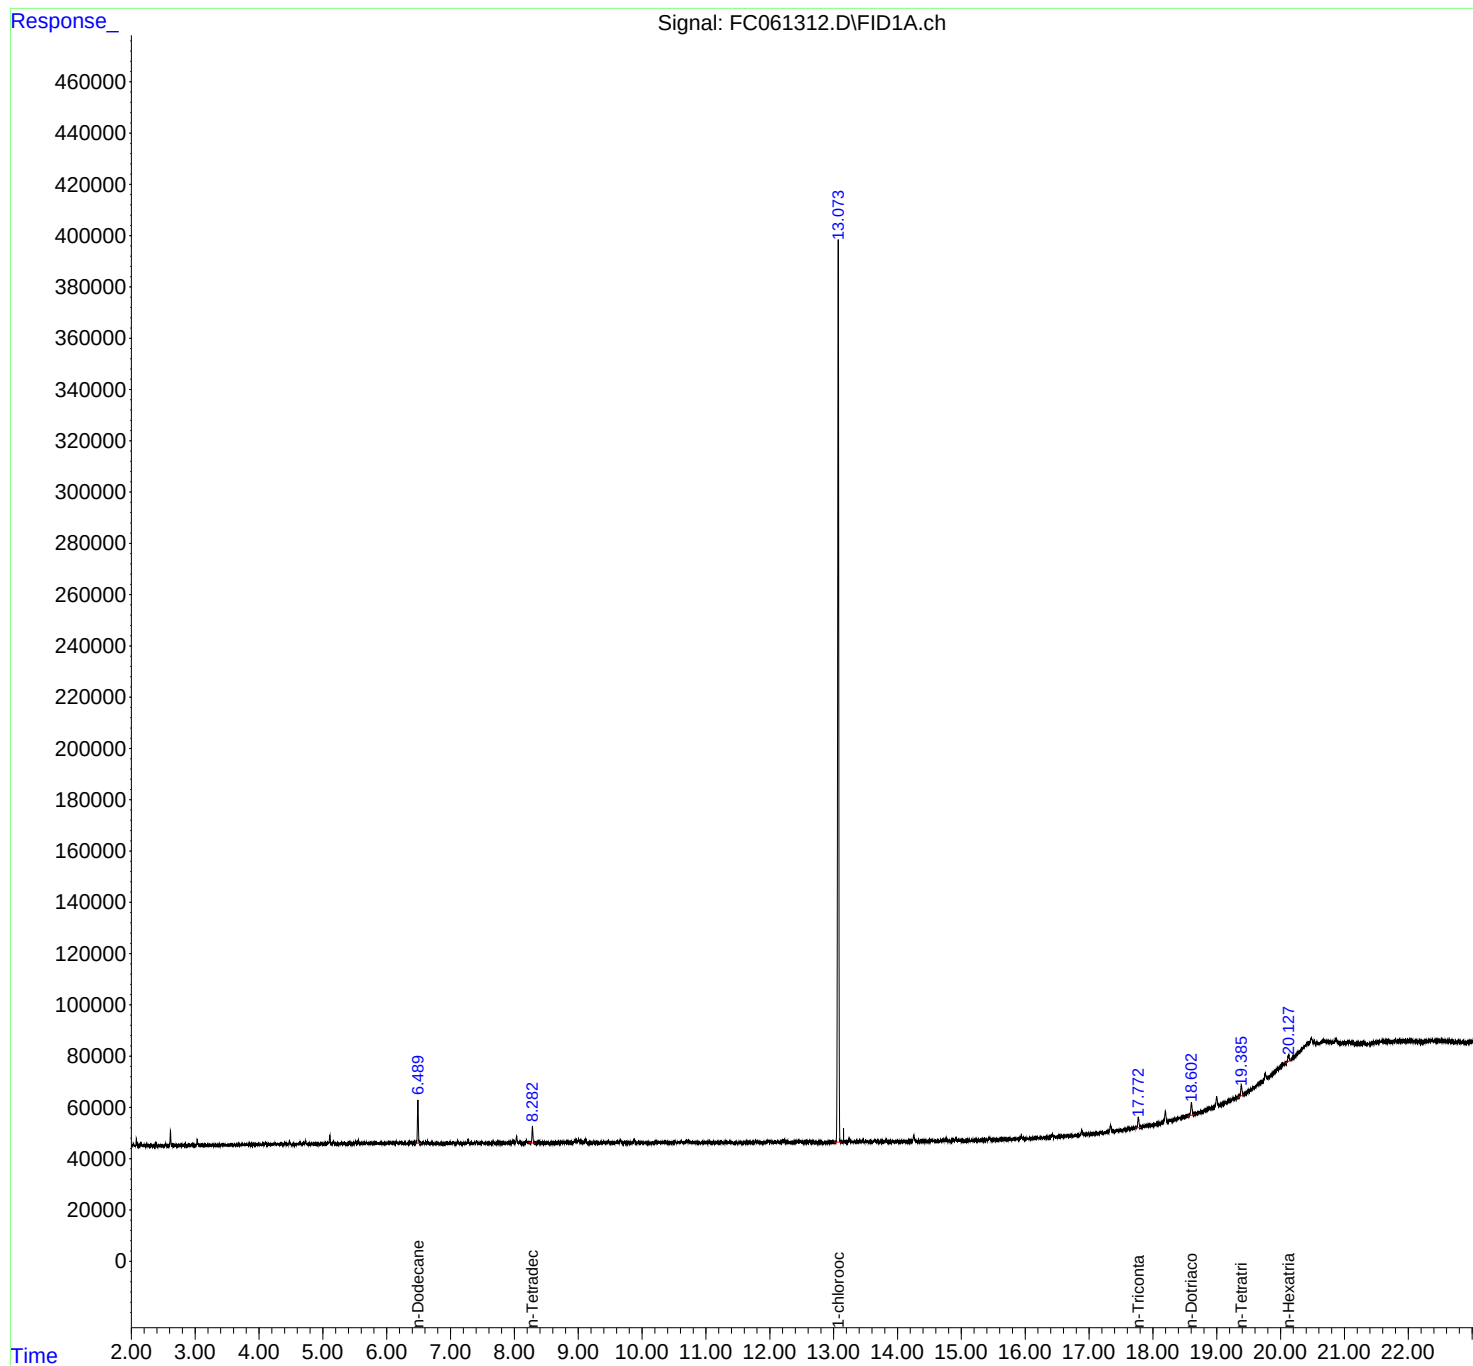


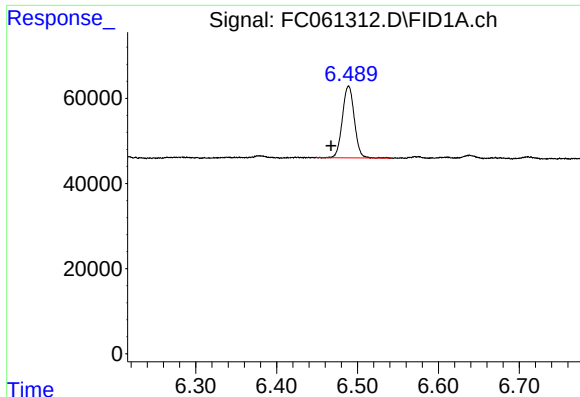

#4 n-Dodecane (C12)


R.T.: 6.489 min
Delta R.T.: 0.022 min
Response: 172510
Conc: 1.11 ug/ml

Instrument :
FID_C
ClientSampleId :

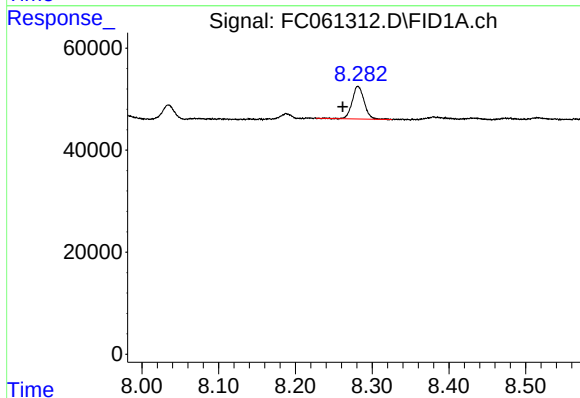


#6 n-Tetradecane (C14)

R.T.: 8.282 min
Delta R.T.: 0.020 min
Response: 69680
Conc: 0.45 ug/ml

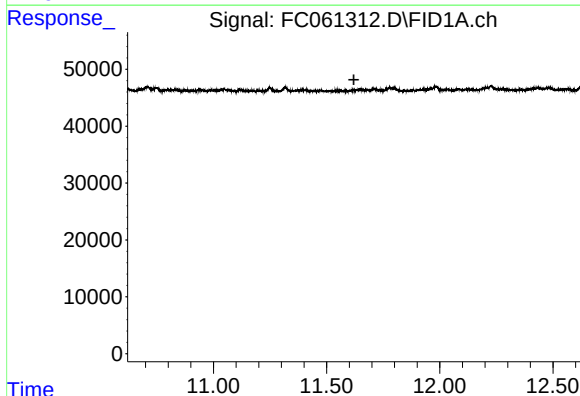


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.621 min
Response: 0
Conc: N.D.

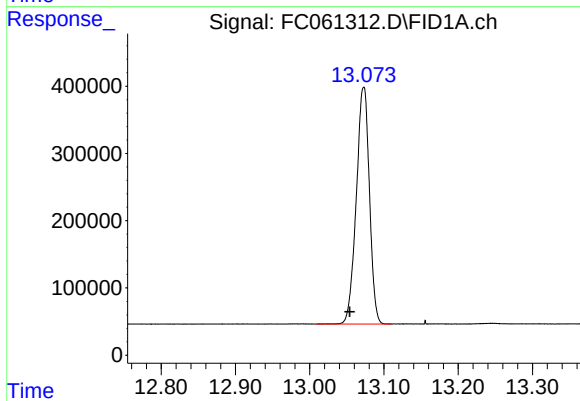

#12 1-chlorooctadecane (SURR)


R.T.: 13.073 min
Delta R.T.: 0.018 min
Response: 4325098
Conc: 30.88 ug/ml

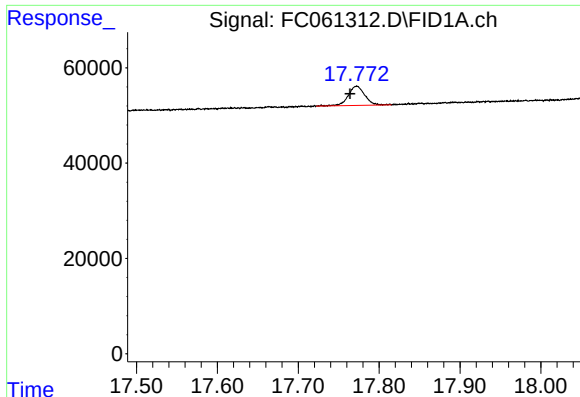

#17 n-Tricontane (C30)


R.T.: 17.772 min
Delta R.T.: 0.008 min
Response: 56723
Conc: 0.41 ug/ml

Instrument :
FID_C
ClientSampleId :

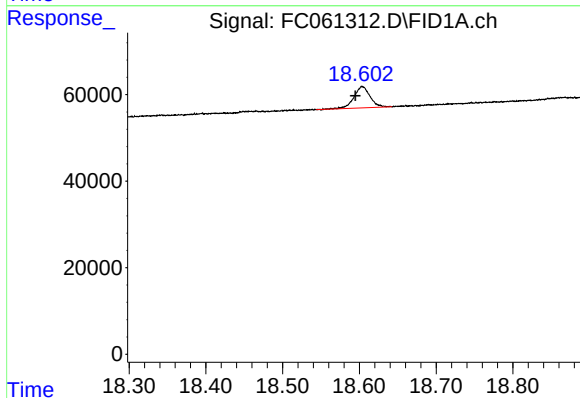


#18 n-Dotriacontane (C32)

R.T.: 18.604 min
Delta R.T.: 0.009 min
Response: 71748
Conc: 0.65 ug/ml

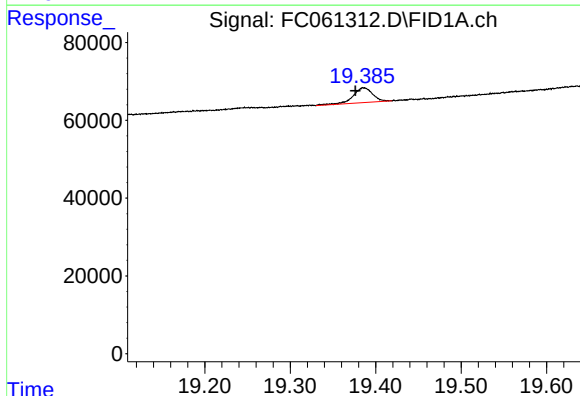

#19 n-Tetratriacontane (C34)

R.T.: 19.386 min
Delta R.T.: 0.010 min
Response: 60424
Conc: 0.78 ug/ml

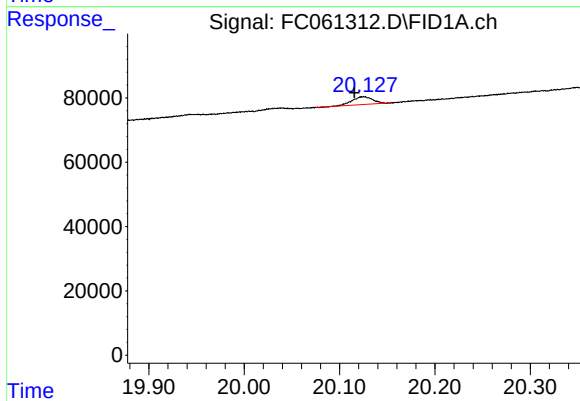

#20 n-Hexatriacontane (C36)

R.T.: 20.125 min
Delta R.T.: 0.009 min
Response: 36453
Conc: 0.65 ug/ml