

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC082824AL\
 Data File : FC067039.D
 Signal(s) : FID1A.ch
 Acq On : 28 Aug 2024 09:00
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 29 02:09:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 081224.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 15:57:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
19) T n-Tetratriacontane (C34)	19.283	16026	0.134 ug/ml
20) T n-Hexatriacontane (C36)	20.077f	60557	0.536 ug/ml
21) T n-Octatriacontane (C38)	20.763	457867	4.203 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC082824AL\
Data File : FC067039.D
Signal(s) : FID1A.ch
Acq On : 28 Aug 2024 09:00
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 29 02:09:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 081224.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 15:57:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

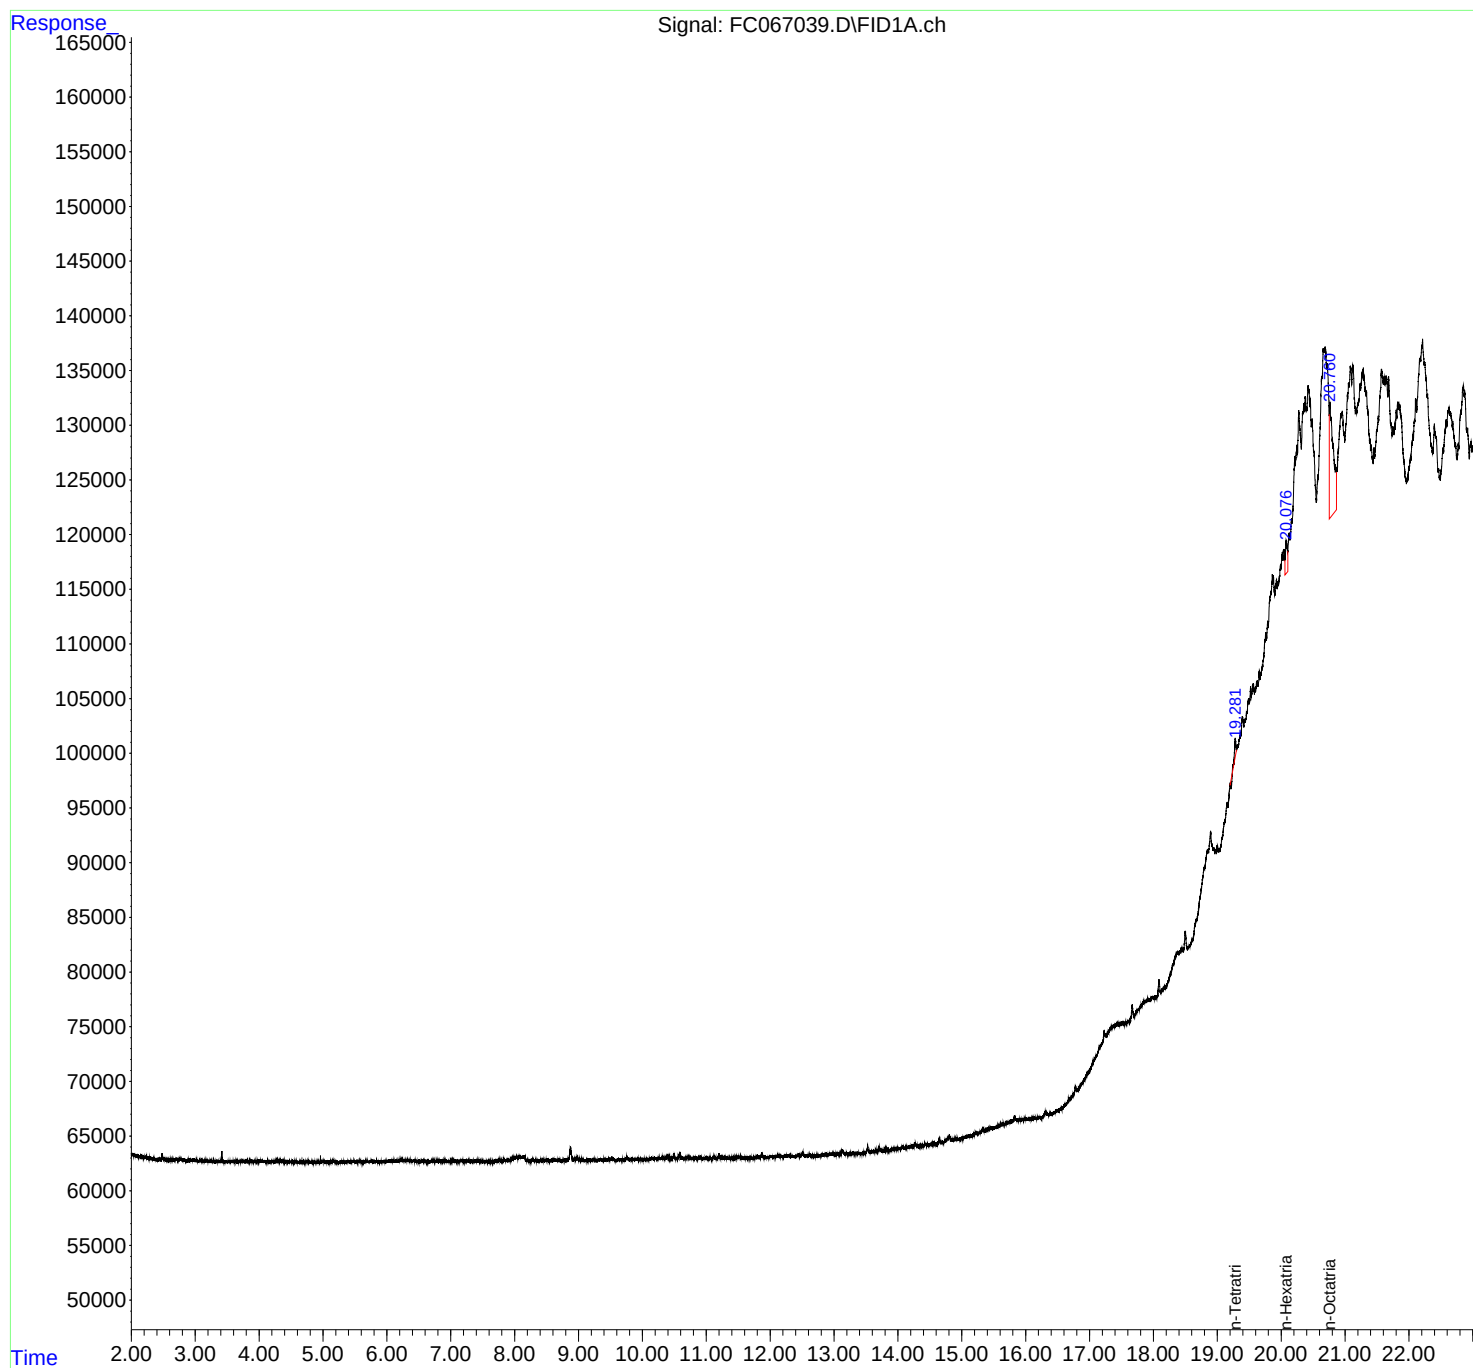


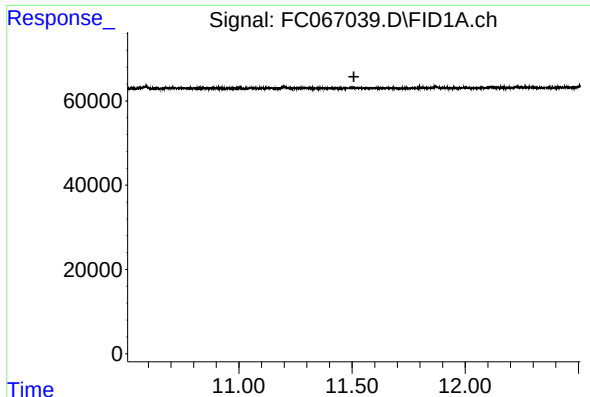

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.508 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

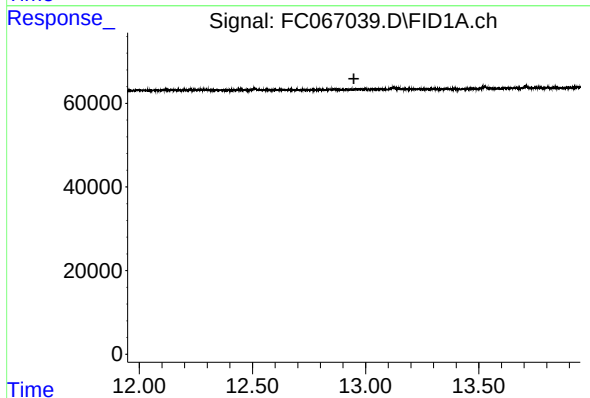


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.948 min
Response: 0
Conc: N.D.

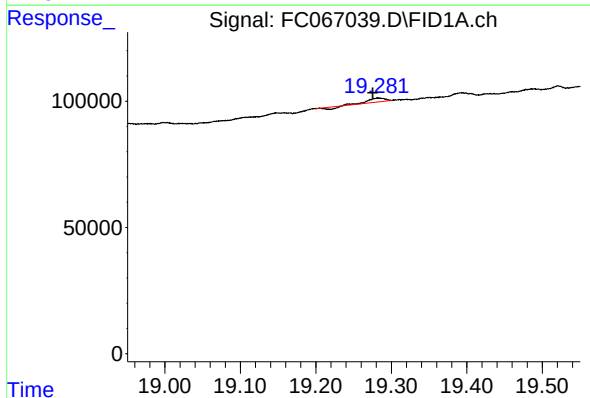


#19 n-Tetratriacontane (C34)

R.T.: 19.283 min
Delta R.T.: 0.008 min
Response: 16026
Conc: 0.13 ug/ml

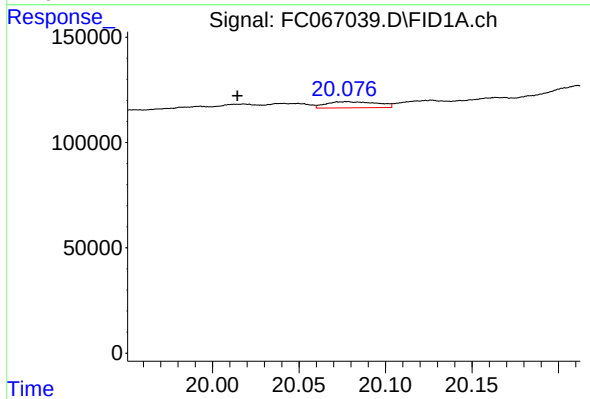

#20 n-Hexatriacontane (C36)

R.T.: 20.077 min
Delta R.T.: 0.063 min
Response: 60557
Conc: 0.54 ug/ml

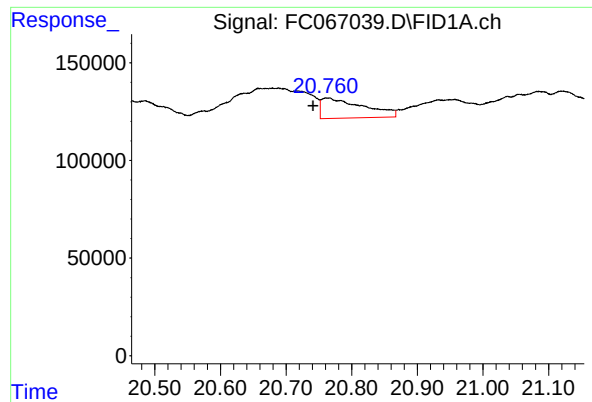

#21 n-Octatriacontane (C38)

R.T.: 20.763 min
Delta R.T.: 0.022 min
Response: 457867
Conc: 4.20 ug/ml

Instrument :

FID_C

ClientSampleId :