

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082825AL\
Data File : FE055571.D
Signal(s) : FID1B.ch
Acq On : 29 Aug 2025 00:12
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 29 03:34:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 082825.M
Quant Title : GC Extractables
QLast Update : Thu Aug 28 12:04:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.238	135790	0.919 ug/ml
18) T	n-Dotriacontane (C32)	19.072	209804	1.429 ug/ml
19) T	n-Tetratriacontane (C34)	19.858	147623	1.045 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082825AL\
Data File : FE055571.D
Signal(s) : FID1B.ch
Acq On : 29 Aug 2025 00:12
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 29 03:34:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 082825.M
Quant Title : GC Extractables
QLast Update : Thu Aug 28 12:04:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

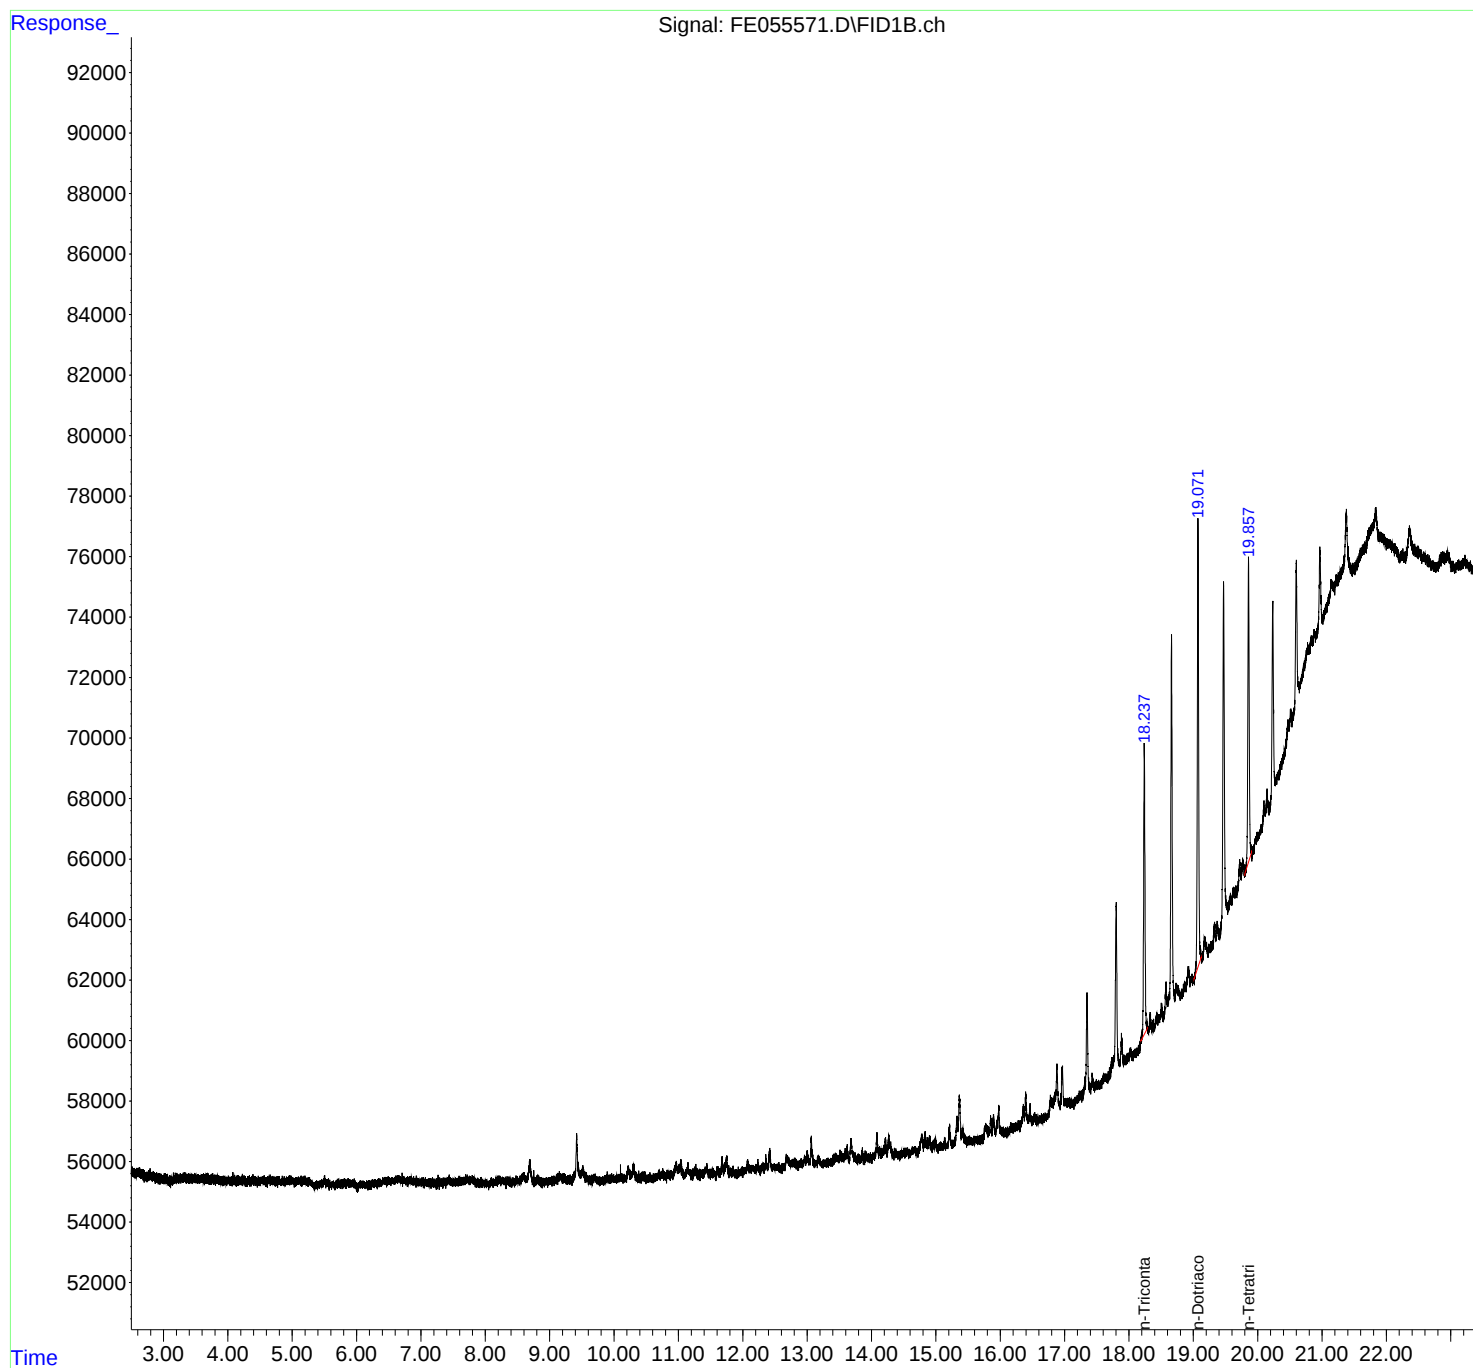


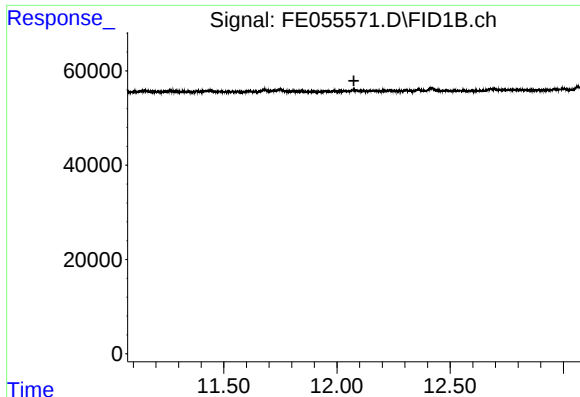

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 12.075 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

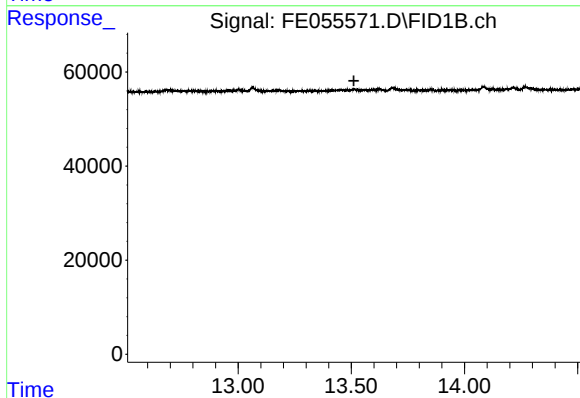


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.512 min
Response: 0
Conc: N.D.

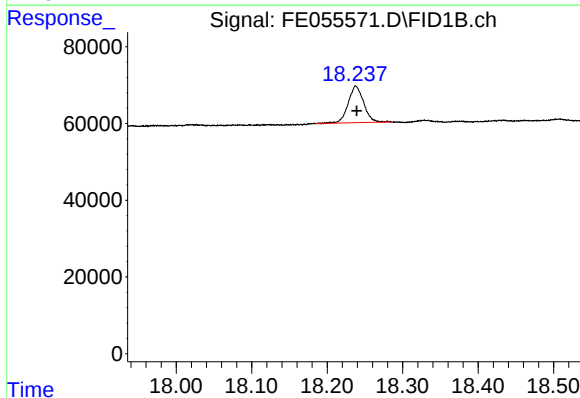


#17 n-Tricontane (C30)

R.T.: 18.238 min
Delta R.T.: 0.000 min
Response: 135790
Conc: 0.92 ug/ml

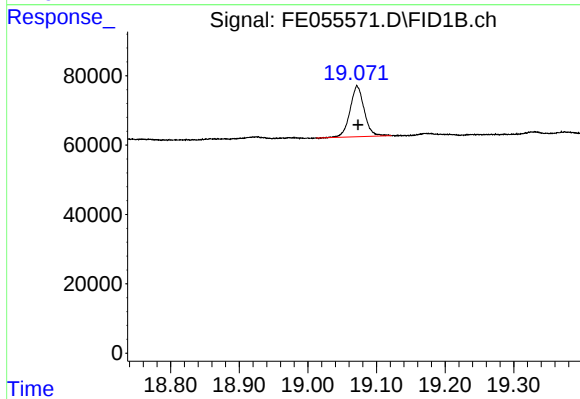

#18 n-Dotriacontane (C32)

R.T.: 19.072 min
Delta R.T.: -0.001 min
Response: 209804
Conc: 1.43 ug/ml

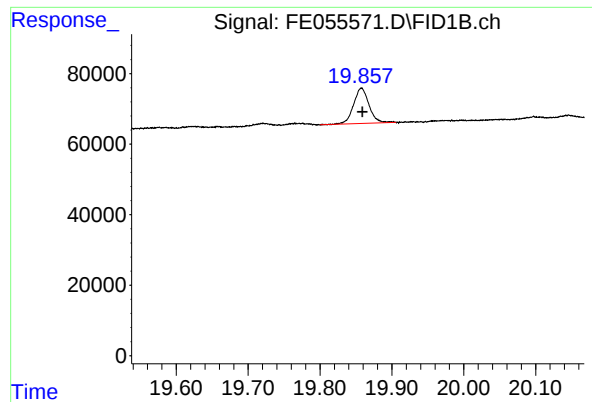

#19 n-Tetratriacontane (C34)

R.T.: 19.858 min
Delta R.T.: -0.001 min
Response: 147623
Conc: 1.04 ug/ml

Instrument :
FID_C
ClientSampleId :