

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC082922AL\
 Data File : FC061323.D
 Signal(s) : FID1A.ch
 Acq On : 29 Aug 2022 09:11
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 30 04:56:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:32:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.556f	79772	0.513 ug/ml
11) T	n-Heneicosane (C21)	13.215	416010	2.660 ug/ml
13) T	n-Docosane (C22)	13.809	227008	1.463 ug/ml
14) T	n-Tetracosane (C24)	14.917	155513	1.005 ug/ml
15) T	n-Hexacosane (C26)	15.936	169215	1.124 ug/ml
16) T	n-Octacosane (C28)	16.884	130399	0.883 ug/ml
17) T	n-Tricontane (C30)	17.769	138342	1.002 ug/ml
18) T	n-Dotriacontane (C32)	18.597	235208	2.143 ug/ml
19) T	n-Tetratriacontane (C34)	19.383	108064	1.400 ug/ml
20) T	n-Hexatriacontane (C36)	20.121	79975	1.417 ug/ml
21) T	n-Octatriacontane (C38)	20.860	131959	2.844 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC082922AL\
Data File : FC061323.D
Signal(s) : FID1A.ch
Acq On : 29 Aug 2022 09:11
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 30 04:56:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:32:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

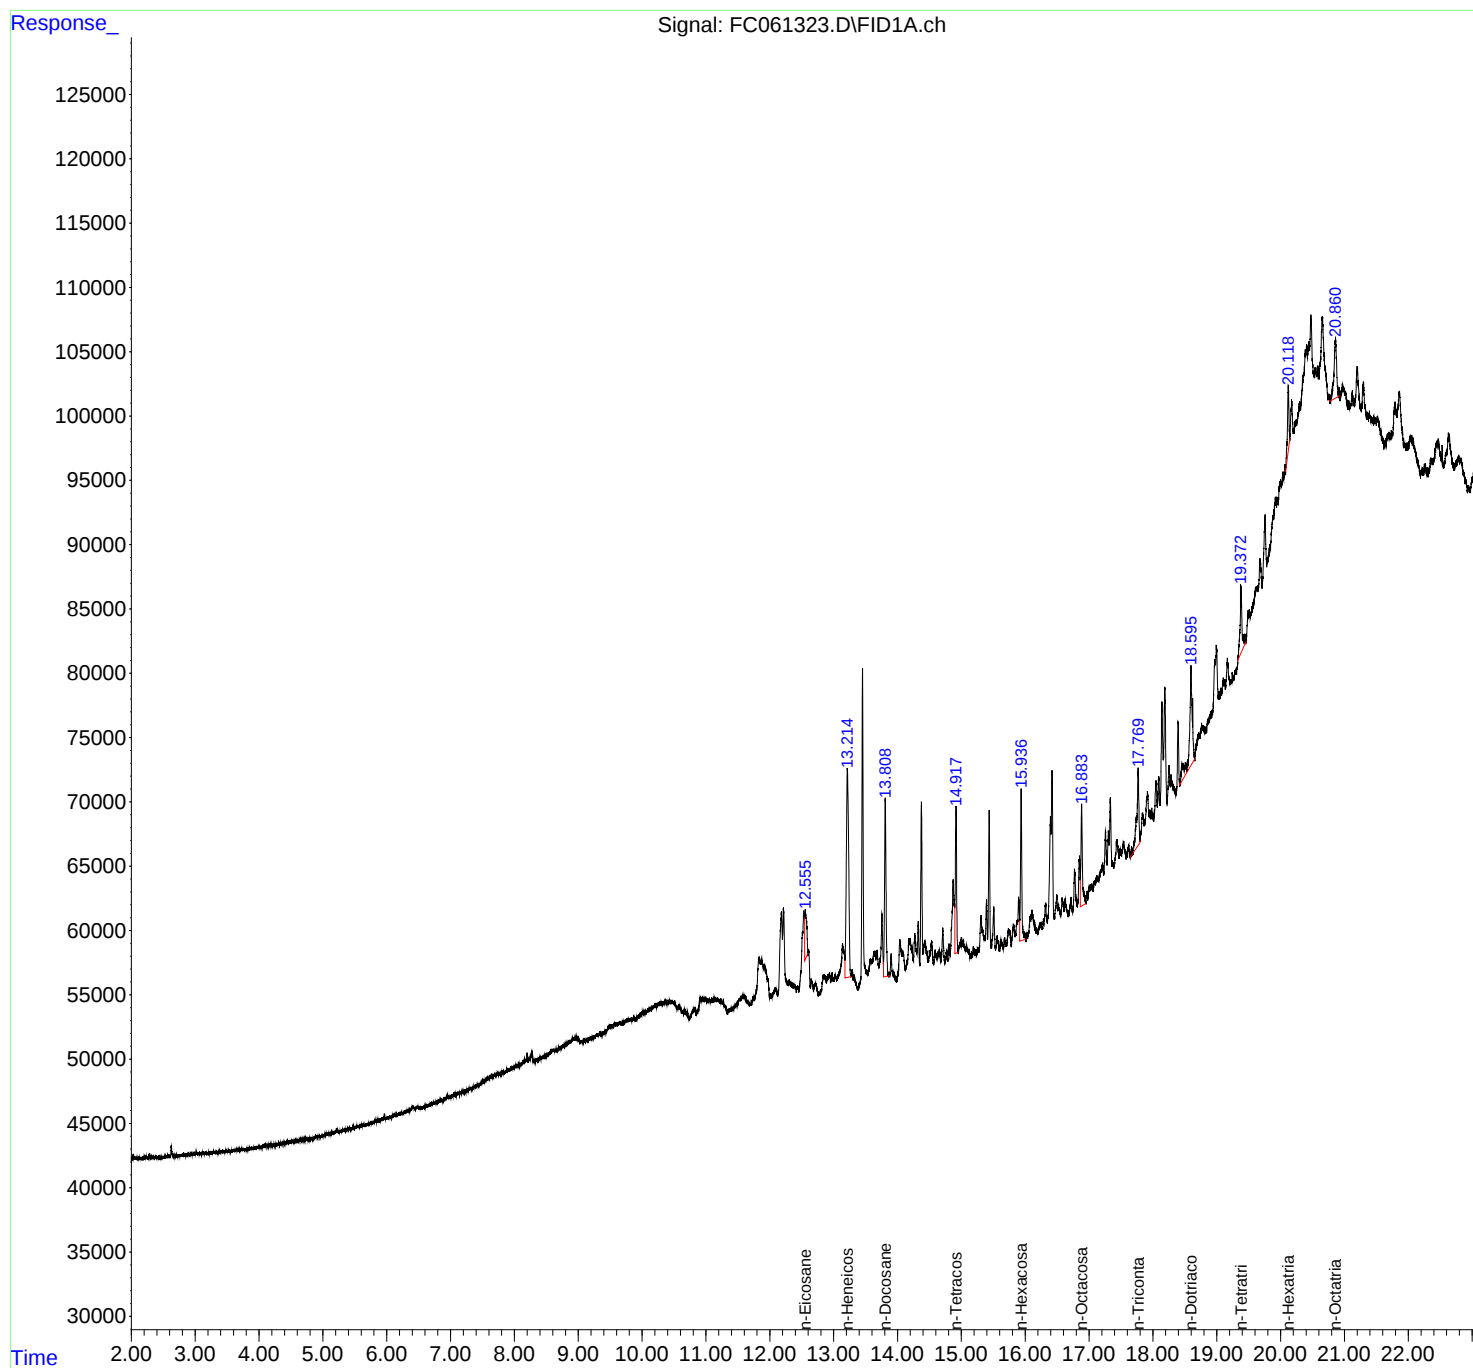


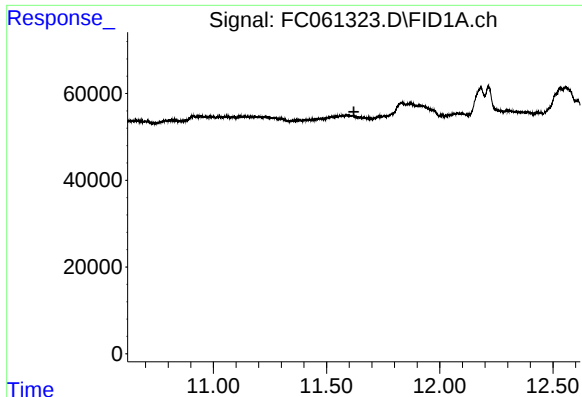

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.621 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

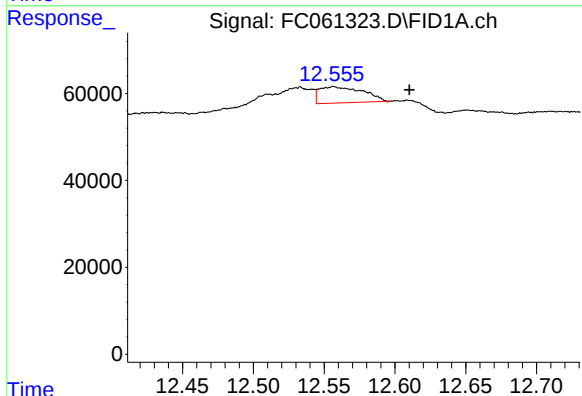


#10 n-Eicosane (C20)

R.T.: 12.556 min
Delta R.T.: -0.054 min
Response: 79772
Conc: 0.51 ug/ml

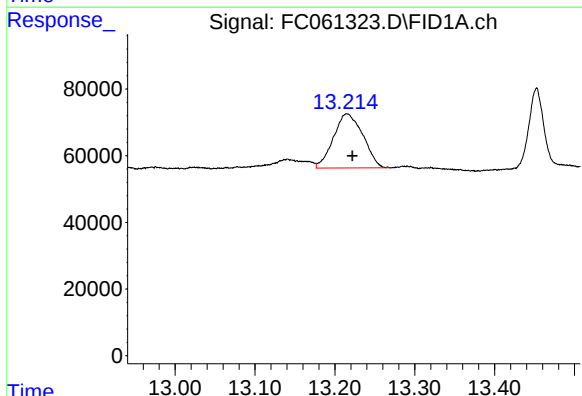


#11 n-Heneicosane (C21)

R.T.: 13.215 min
Delta R.T.: -0.007 min
Response: 416010
Conc: 2.66 ug/ml

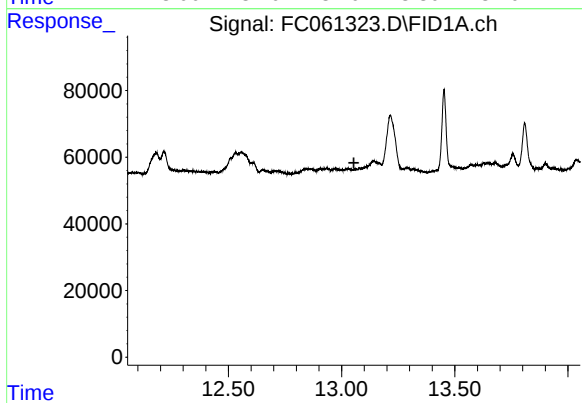

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.054 min
Response: 0
Conc: N.D.

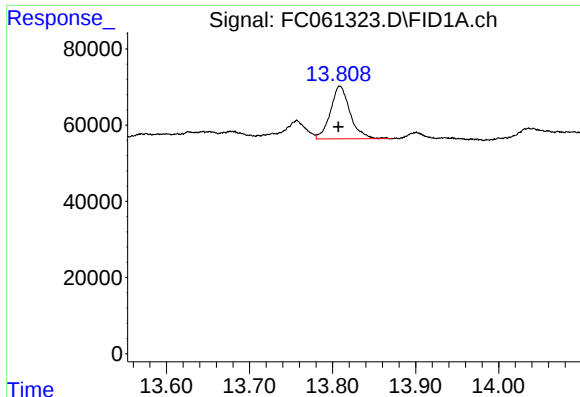

#13 n-Docosane (C22)


R.T.: 13.809 min
Delta R.T.: 0.002 min
Response: 227008
Conc: 1.46 ug/ml

Instrument :
FID_C
ClientSampleId :

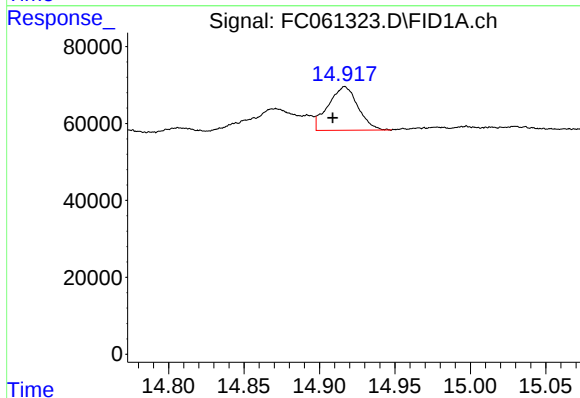


#14 n-Tetracosane (C24)

R.T.: 14.917 min
Delta R.T.: 0.008 min
Response: 155513
Conc: 1.01 ug/ml

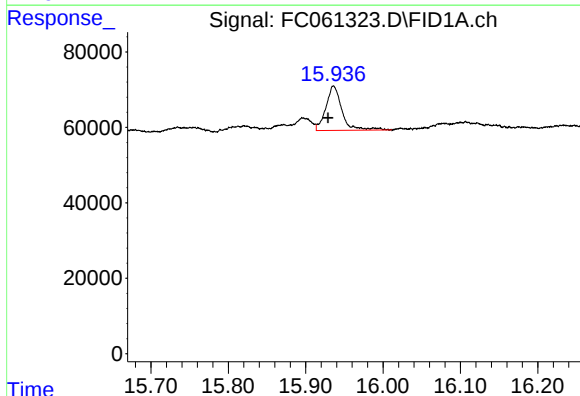


#15 n-Hexacosane (C26)

R.T.: 15.936 min
Delta R.T.: 0.007 min
Response: 169215
Conc: 1.12 ug/ml

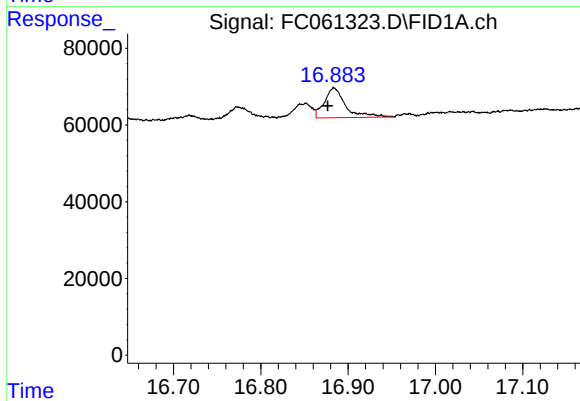

#16 n-Octacosane (C28)


R.T.: 16.884 min
Delta R.T.: 0.008 min
Response: 130399
Conc: 0.88 ug/ml

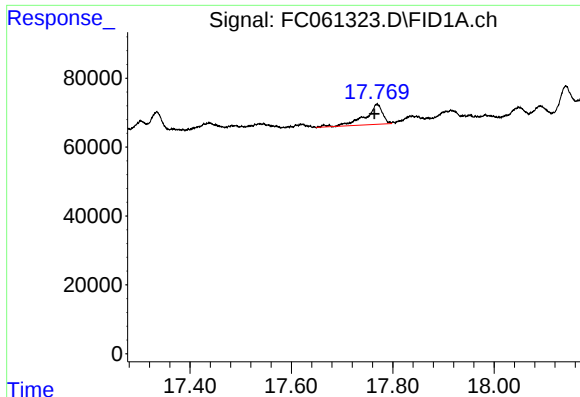

#17 n-Tricontane (C30)


R.T.: 17.769 min
Delta R.T.: 0.005 min
Response: 138342
Conc: 1.00 ug/ml

Instrument :
FID_C
ClientSampleId :

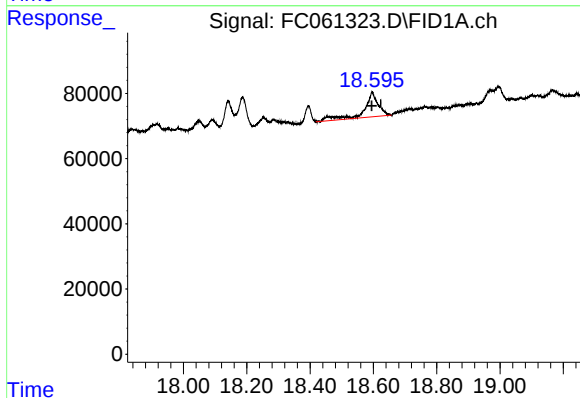


#18 n-Dotriacontane (C32)

R.T.: 18.597 min
Delta R.T.: 0.002 min
Response: 235208
Conc: 2.14 ug/ml

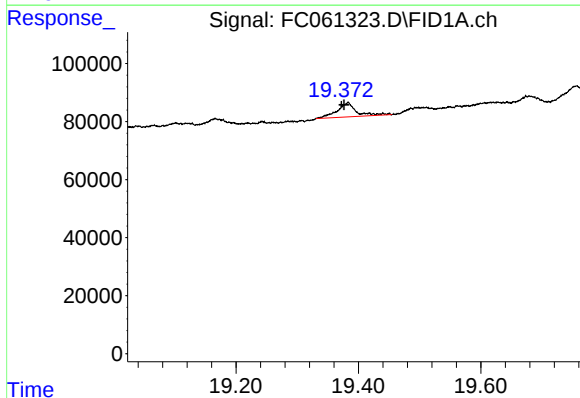


#19 n-Tetratriacontane (C34)

R.T.: 19.383 min
Delta R.T.: 0.006 min
Response: 108064
Conc: 1.40 ug/ml

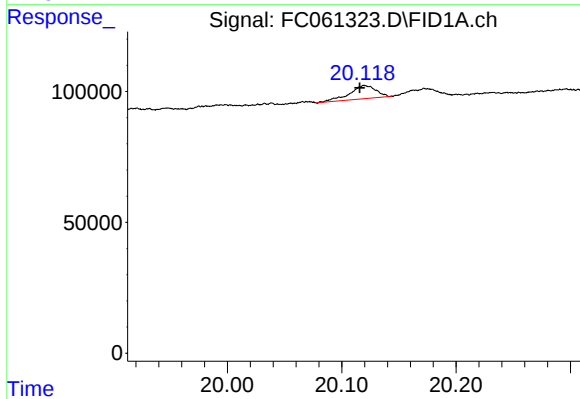

#20 n-Hexatriacontane (C36)

R.T.: 20.121 min
Delta R.T.: 0.005 min
Response: 79975
Conc: 1.42 ug/ml

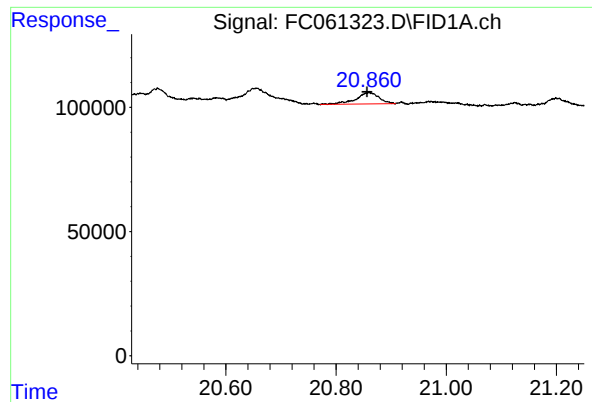

#21 n-Octatriacontane (C38)

R.T.: 20.860 min
Delta R.T.: 0.004 min
Response: 131959
Conc: 2.84 ug/ml

Instrument :
FID_C
ClientSampleId :