

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC082922AL\
 Data File : FC061327.D
 Signal(s) : FID1A.ch
 Acq On : 29 Aug 2022 12:36
 Operator : YP/AJ
 Sample : N4378-01DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 30 04:57:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 082222.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 23 05:32:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.639	845049	4.774 ug/ml
Spiked Amount 50.000		Recovery =	9.55%
12) S 1-chlorooctadecane (S...	13.070	689941	4.926 ug/ml
Spiked Amount 50.000		Recovery =	9.85%
Target Compounds			
10) T n-Eicosane (C20)	12.570	74222	0.477 ug/ml
13) T n-Docosane (C22)	13.847	135816	0.875 ug/ml
14) T n-Tetracosane (C24)	14.895	234208	1.514 ug/ml
16) T n-Octacosane (C28)	16.886	72327	0.490 ug/ml
17) T n-Tricontane (C30)	17.775	157395	1.140 ug/ml
18) T n-Dotriacontane (C32)	18.604	54706	0.498 ug/ml
19) T n-Tetratriacontane (C34)	19.388	37156	0.481 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC082922AL\
Data File : FC061327.D
Signal(s) : FID1A.ch
Acq On : 29 Aug 2022 12:36
Operator : YP/AJ
Sample : N4378-01DL 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 30 04:57:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 082222.M
Quant Title : GC Extractables
QLast Update : Tue Aug 23 05:32:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

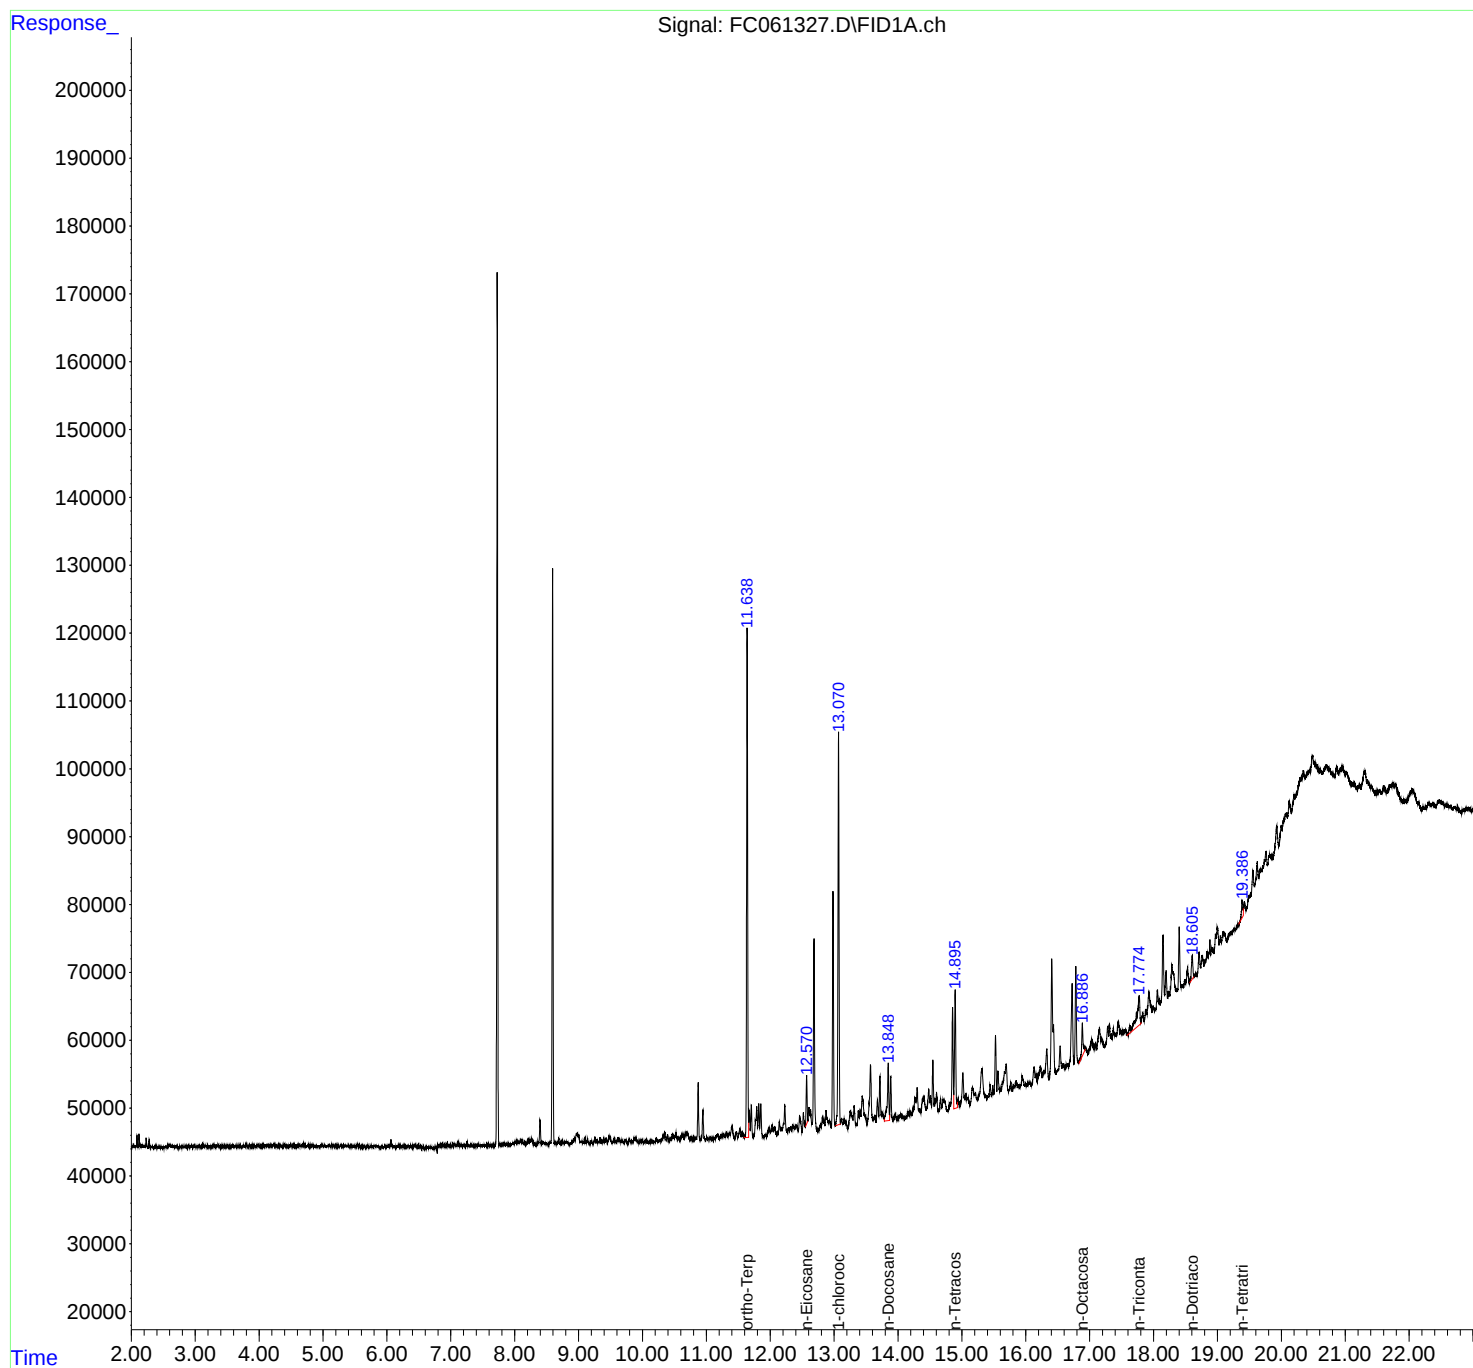


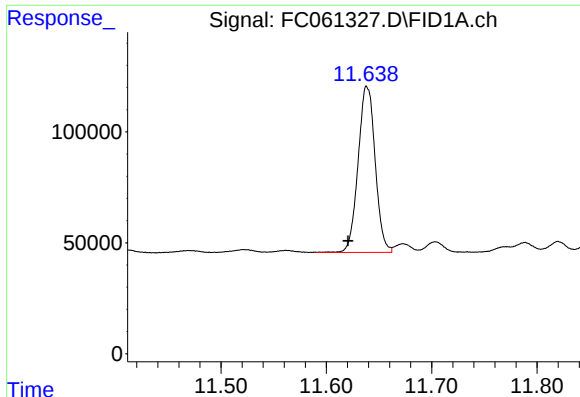

#9 ortho-Terphenyl (SURR)


R.T.: 11.639 min
Delta R.T.: 0.018 min
Response: 845049
Conc: 4.77 ug/ml

Instrument :
FID_C
ClientSampleId :

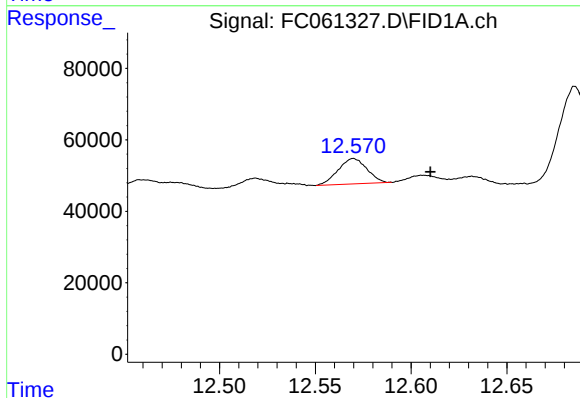


#10 n-Eicosane (C20)

R.T.: 12.570 min
Delta R.T.: -0.040 min
Response: 74222
Conc: 0.48 ug/ml

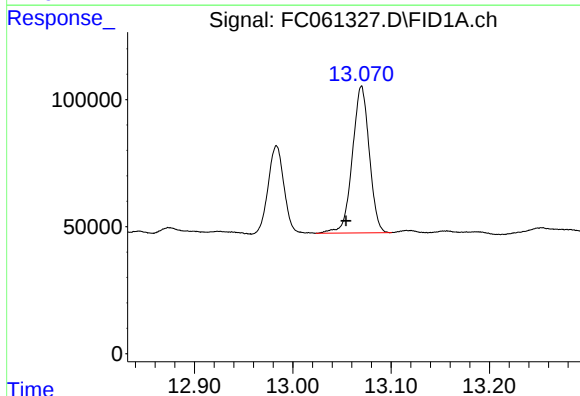


#12 1-chlorooctadecane (SURR)

R.T.: 13.070 min
Delta R.T.: 0.016 min
Response: 689941
Conc: 4.93 ug/ml

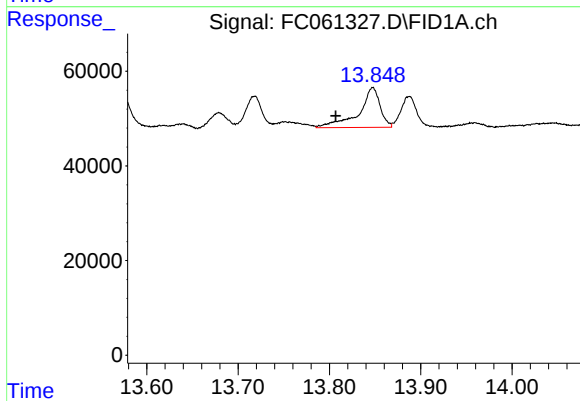

#13 n-Docosane (C22)


R.T.: 13.847 min
Delta R.T.: 0.040 min
Response: 135816
Conc: 0.88 ug/ml

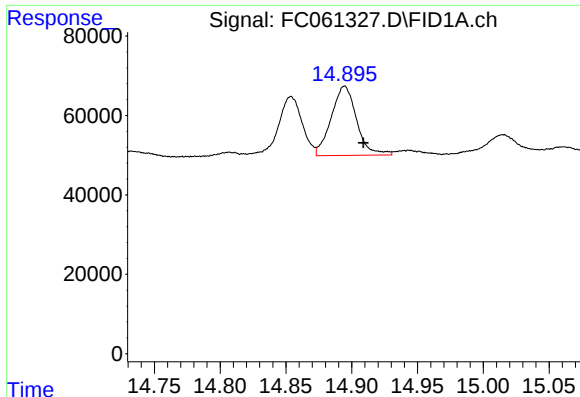

#14 n-Tetracosane (C24)


R.T.: 14.895 min
Delta R.T.: -0.014 min
Response: 234208
Conc: 1.51 ug/ml

Instrument :
FID_C
ClientSampleId :

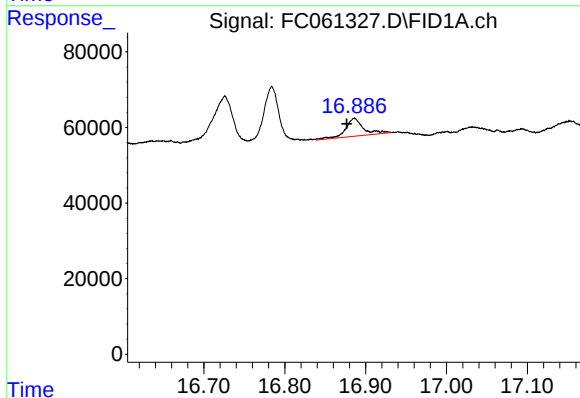


#16 n-Octacosane (C28)

R.T.: 16.886 min
Delta R.T.: 0.010 min
Response: 72327
Conc: 0.49 ug/ml

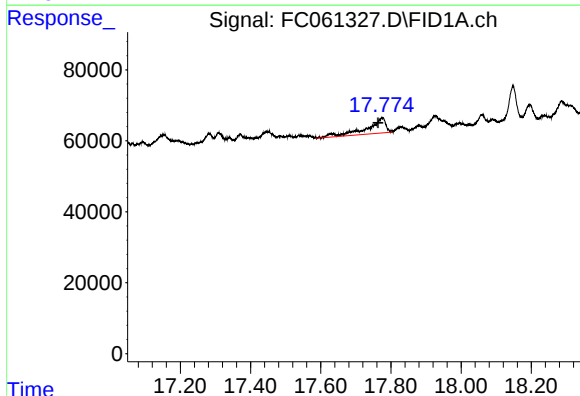


#17 n-Tricontane (C30)

R.T.: 17.775 min
Delta R.T.: 0.011 min
Response: 157395
Conc: 1.14 ug/ml

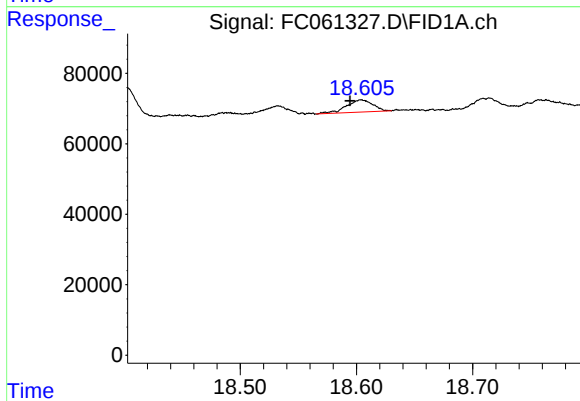

#18 n-Dotriacontane (C32)

R.T.: 18.604 min
Delta R.T.: 0.010 min
Response: 54706
Conc: 0.50 ug/ml

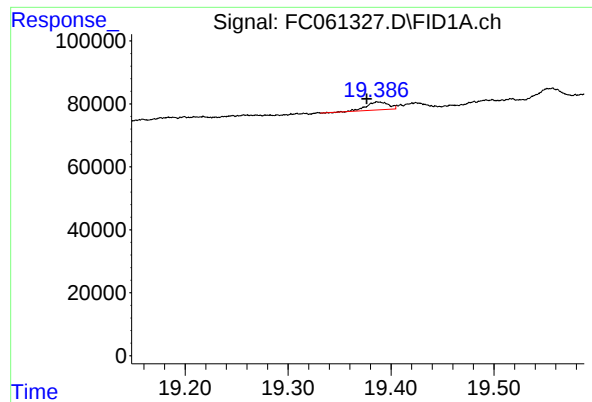

#19 n-Tetratriacontane (C34)

R.T.: 19.388 min
Delta R.T.: 0.011 min
Response: 37156
Conc: 0.48 ug/ml

Instrument :

FID_C

ClientSampleId :