

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC083022AL\  
 Data File : FC061358.D  
 Signal(s) : FID1A.ch  
 Acq On : 30 Aug 2022 16:02  
 Operator : YP/AJ  
 Sample : N4414-01DL 5X  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 FID\_C  
 ClientSampleId :  
 OK-2-082622DL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 08/31/2022  
 Supervised By :Ankita Jodhani 08/31/2022

Integration File: autoint1.e  
 Quant Time: Aug 31 03:37:20 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 082222.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Aug 23 05:32:18 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.642 | 976271     | 5.515 ug/ml  |
| Spiked Amount 50.000           |        | Recovery = | 11.03%       |
| 12) S 1-chlorooctadecane (S... | 13.073 | 883189     | 6.306 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 12.61%       |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC083022AL\  
Data File : FC061358.D  
Signal(s) : FID1A.ch  
Acq On : 30 Aug 2022 16:02  
Operator : YP/AJ  
Sample : N4414-01DL 5X  
Misc :  
ALS Vial : 8 Sample Multiplier: 1


Instrument :  
FID\_C  
ClientSampleId :  
OK-2-082622DL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/31/2022  
Supervised By :Ankita Jodhani 08/31/2022

Integration File: autoint1.e  
Quant Time: Aug 31 03:37:20 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 082222.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 23 05:32:18 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

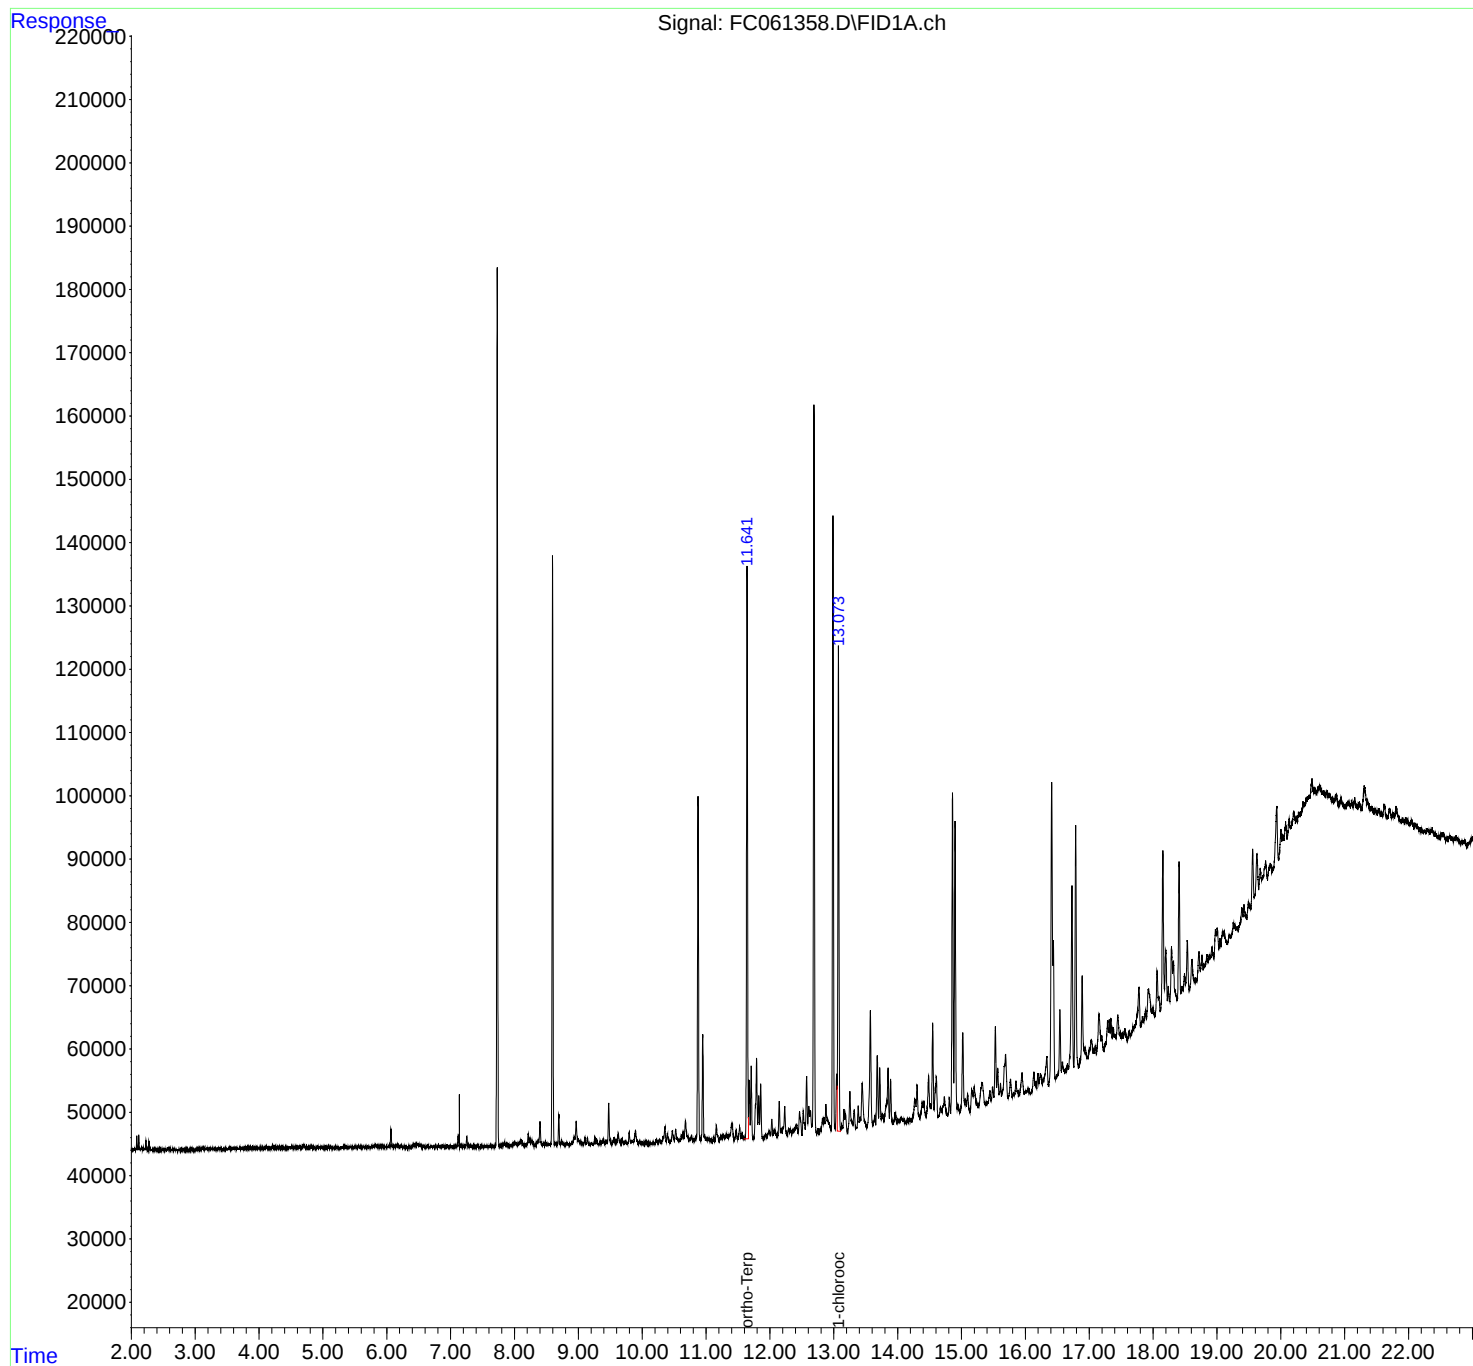

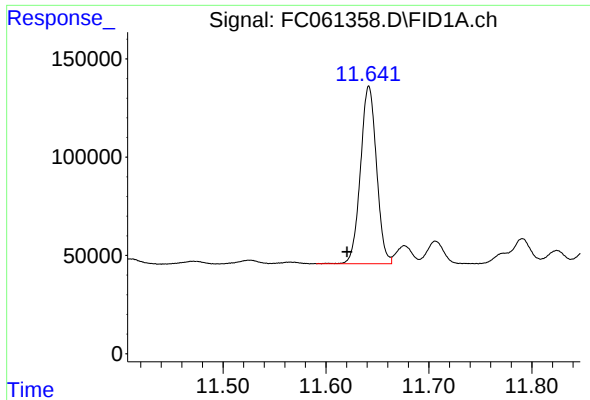


#9 ortho-Terphenyl (SURR)

R.T.: 11.642 min  
Delta R.T.: 0.021 min  
Response: 976271  
Conc: 5.51 ug/ml

Instrument :  
FID\_C  
ClientSampleId :  
OK-2-082622DL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/31/2022  
Supervised By :Ankita Jodhani 08/31/2022

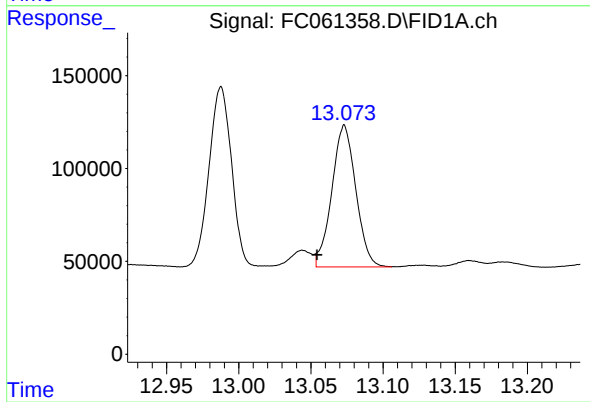

#12 1-chlorooctadecane (SURR)

R.T.: 13.073 min  
Delta R.T.: 0.019 min  
Response: 883189  
Conc: 6.31 ug/ml m