

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC083123AL\
Data File : FC064456.D
Signal(s) : FID1A.ch
Acq On : 31 Aug 2023 08:53
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 31 12:13:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 081823.M
Quant Title : GC Extractables
QLast Update : Fri Aug 18 14:31:35 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.474	33483	0.237 ug/ml
19) T	n-Tetratriacontane (C34)	19.253	35522	0.266 ug/ml
20) T	n-Hexatriacontane (C36)	19.990	19943	0.156 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC083123AL\
Data File : FC064456.D
Signal(s) : FID1A.ch
Acq On : 31 Aug 2023 08:53
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 31 12:13:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 081823.M
Quant Title : GC Extractables
QLast Update : Fri Aug 18 14:31:35 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

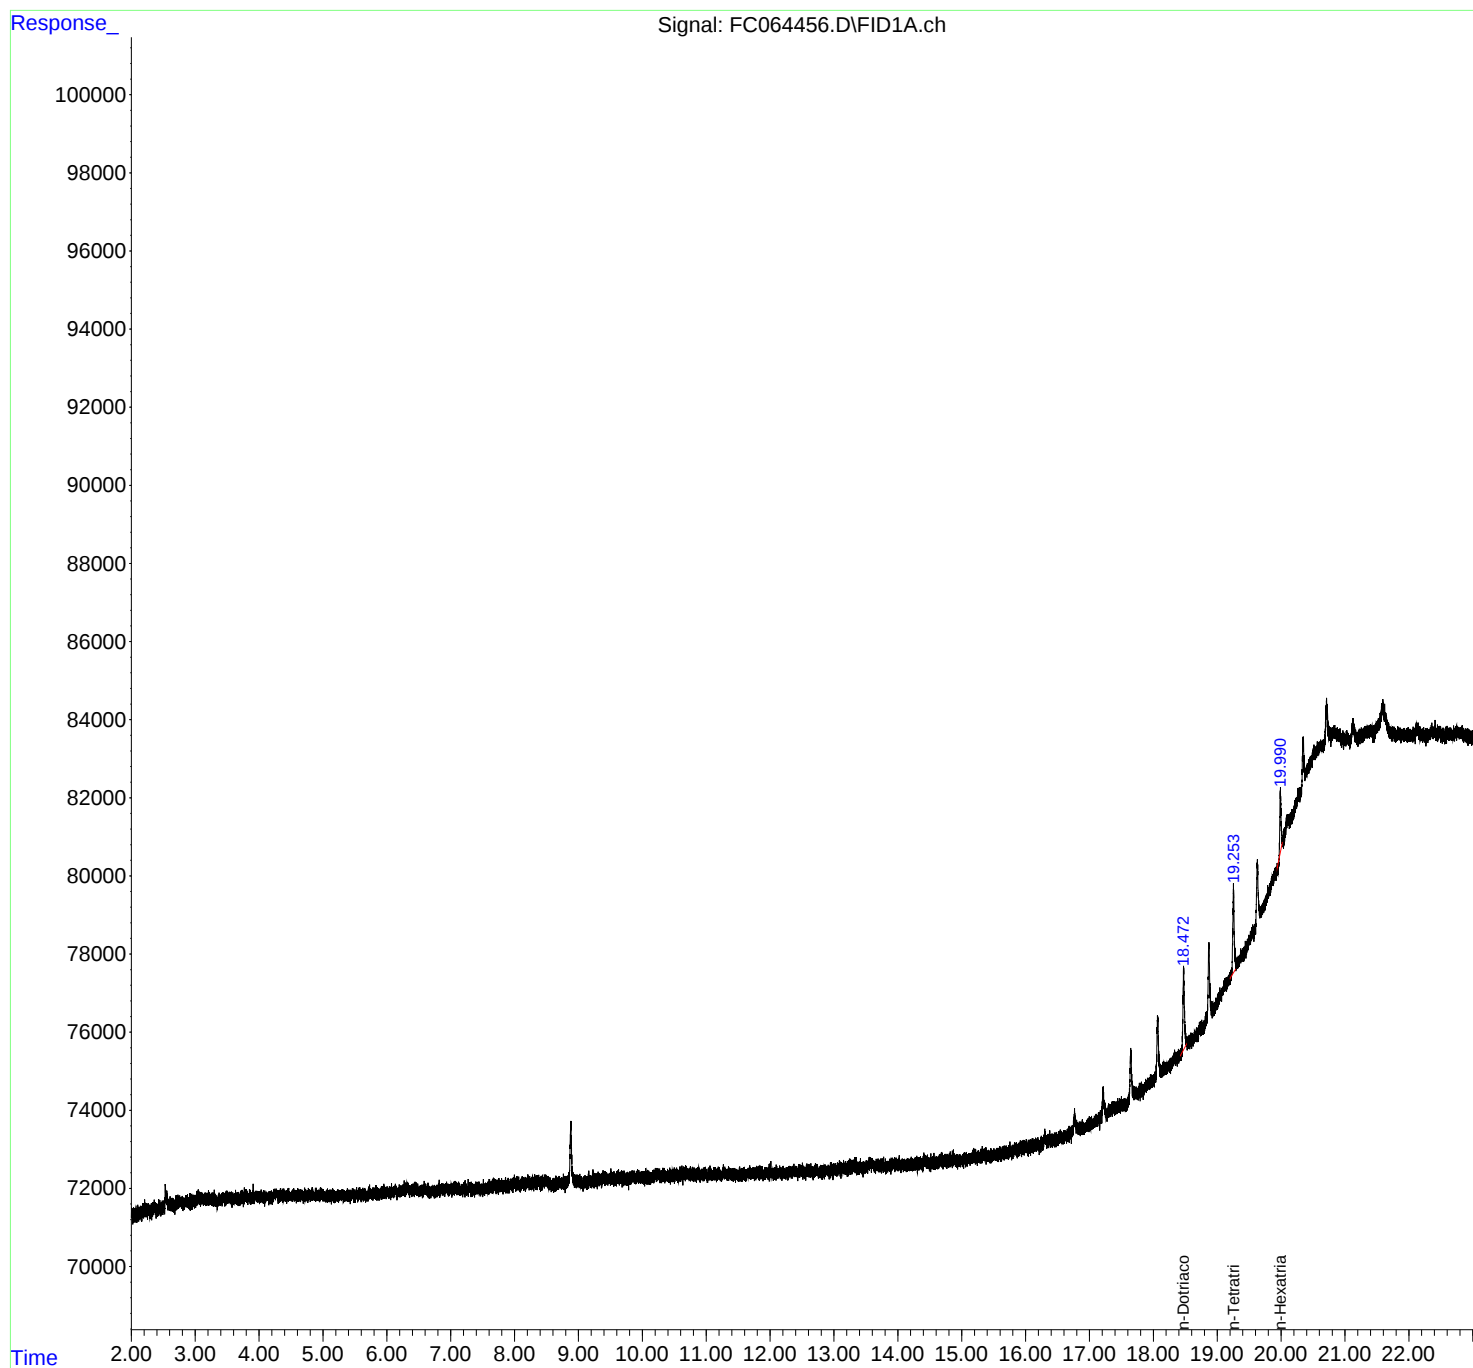


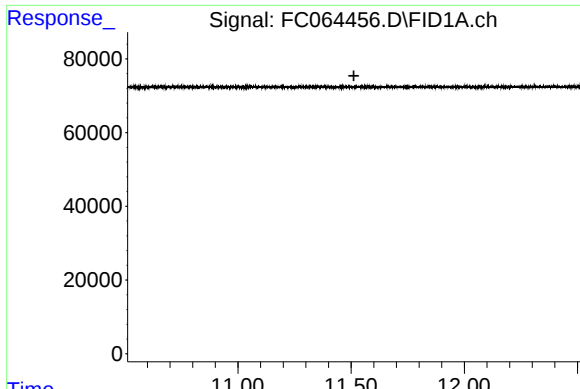

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.512 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

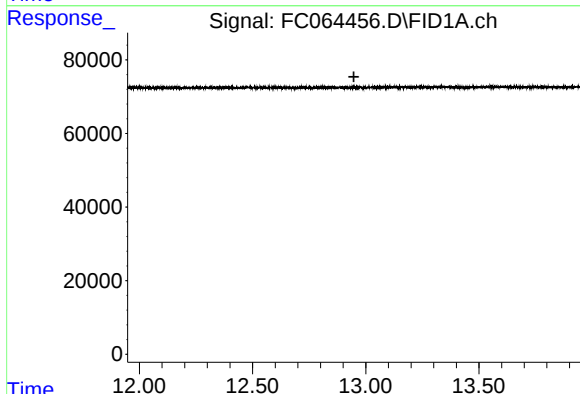


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 12.947 min
Response: 0
Conc: N.D.

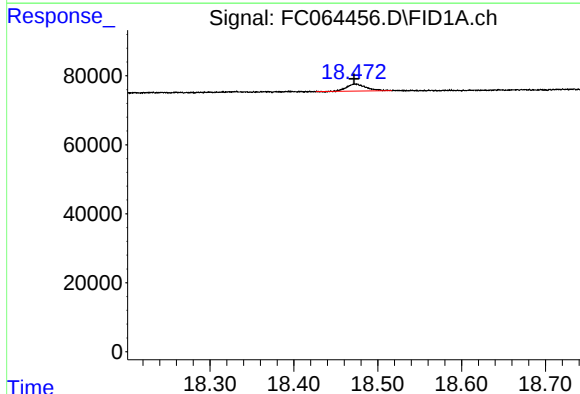


#18 n-Dotriacontane (C32)

R.T.: 18.474 min
Delta R.T.: 0.002 min
Response: 33483
Conc: 0.24 ug/ml

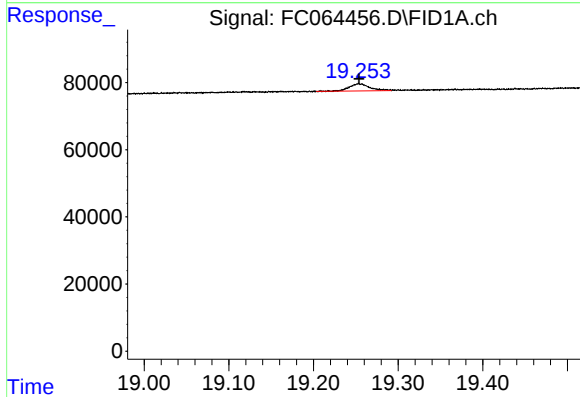

#19 n-Tetratriacontane (C34)

R.T.: 19.253 min
Delta R.T.: 0.000 min
Response: 35522
Conc: 0.27 ug/ml

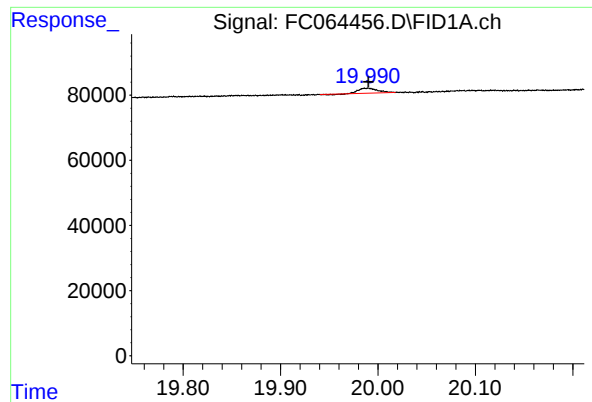

#20 n-Hexatriacontane (C36)

R.T.: 19.990 min
Delta R.T.: 0.000 min
Response: 19943
Conc: 0.16 ug/ml

Instrument :

FID_C

ClientSampleId :