

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC083123AL\
 Data File : FC064462.D
 Signal(s) : FID1A.ch
 Acq On : 31 Aug 2023 13:08
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 01 00:17:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 081823.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 18 14:31:35 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.647	30730	0.210 ug/ml
18) T	n-Dotriacontane (C32)	18.471	24256	0.172 ug/ml
19) T	n-Tetratriacontane (C34)	19.254	59634	0.446 ug/ml
20) T	n-Hexatriacontane (C36)	19.997	82713	0.646 ug/ml
21) T	n-Octatriacontane (C38)	20.667	925320	7.535 ug/ml
22) T	n-Tetracontane (C40)	21.559	978628	8.427 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC083123AL\
Data File : FC064462.D
Signal(s) : FID1A.ch
Acq On : 31 Aug 2023 13:08
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 01 00:17:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 081823.M
Quant Title : GC Extractables
QLast Update : Fri Aug 18 14:31:35 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

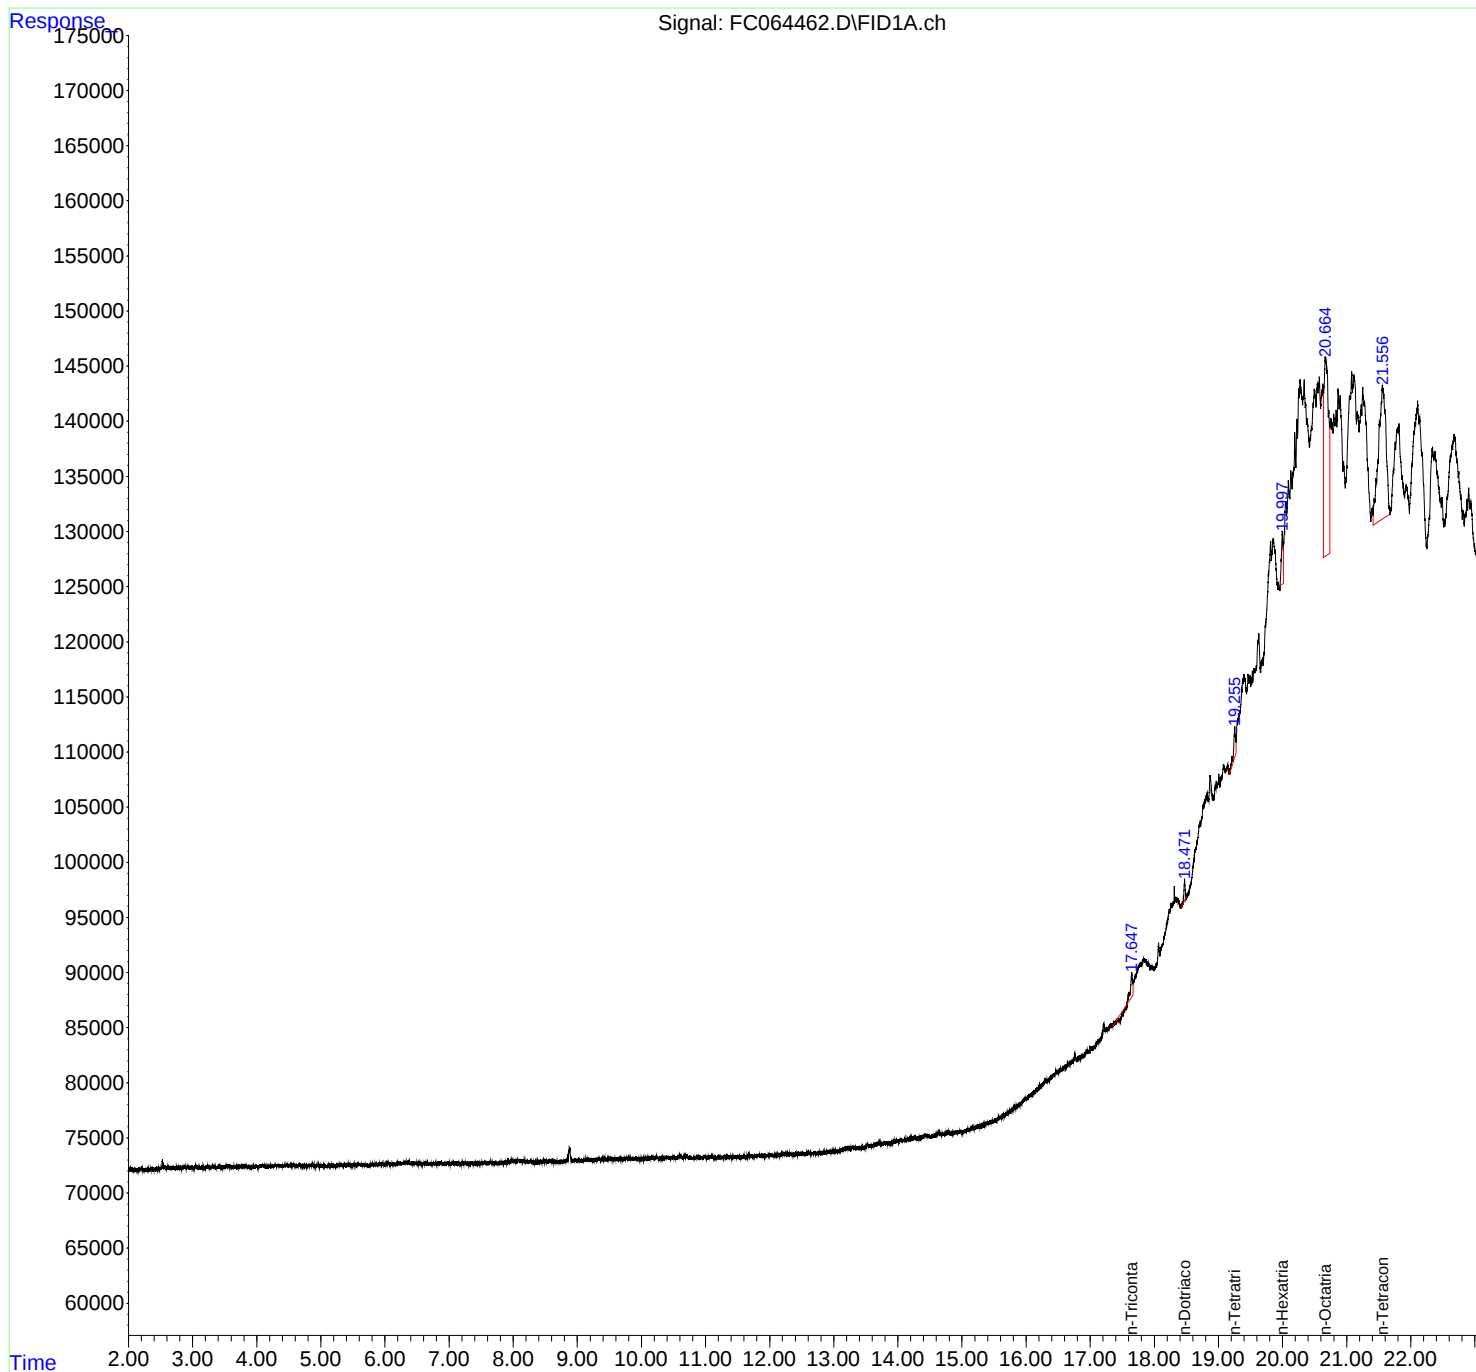


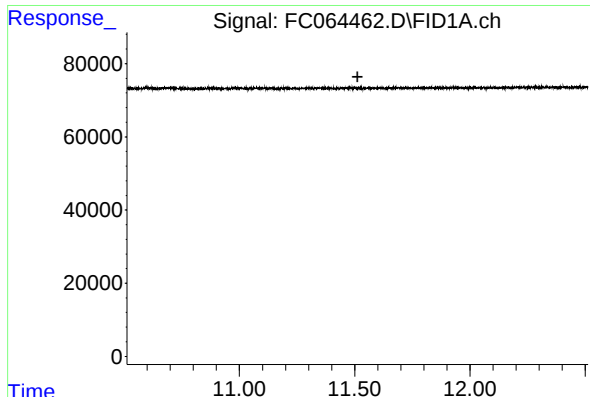

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.512 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

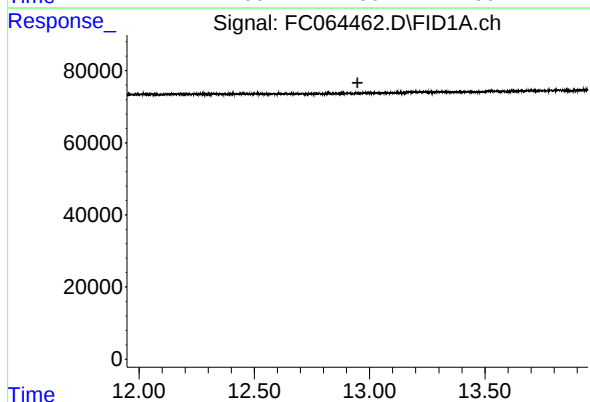


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.947 min
Response: 0
Conc: N.D.

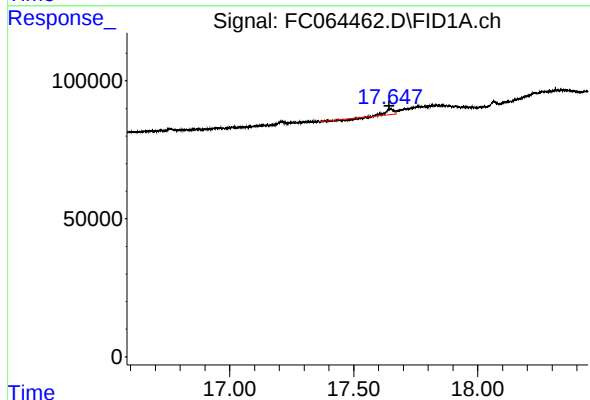


#17 n-Tricontane (C30)

R.T.: 17.647 min
Delta R.T.: 0.003 min
Response: 30730
Conc: 0.21 ug/ml

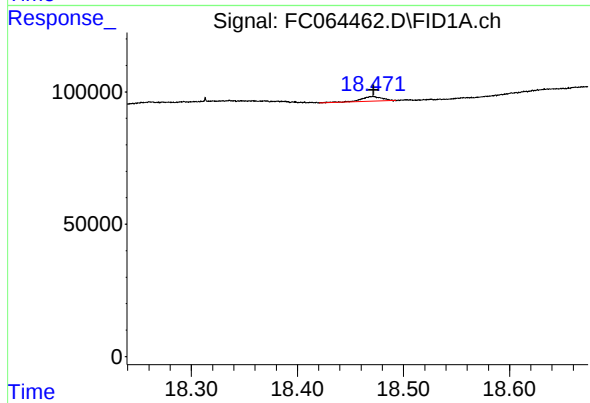

#18 n-Dotriacontane (C32)


R.T.: 18.471 min
Delta R.T.: -0.001 min
Response: 24256
Conc: 0.17 ug/ml

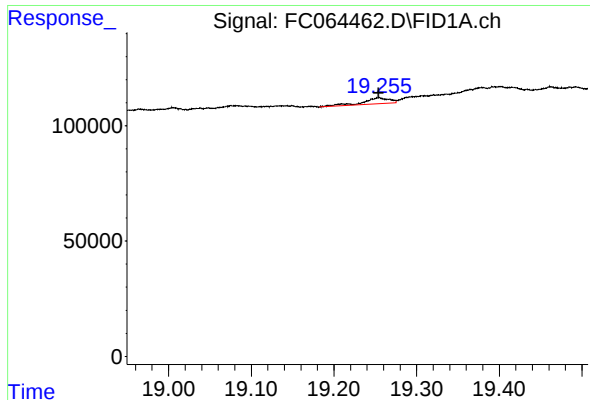

#19 n-Tetratriacontane (C34)


R.T.: 19.254 min
Delta R.T.: 0.000 min
Response: 59634
Conc: 0.45 ug/ml

Instrument :
FID_C
ClientSampleId :

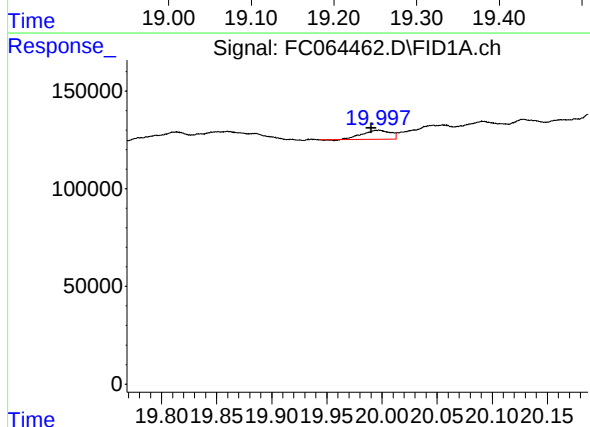


#20 n-Hexatriacontane (C36)

R.T.: 19.997 min
Delta R.T.: 0.007 min
Response: 82713
Conc: 0.65 ug/ml

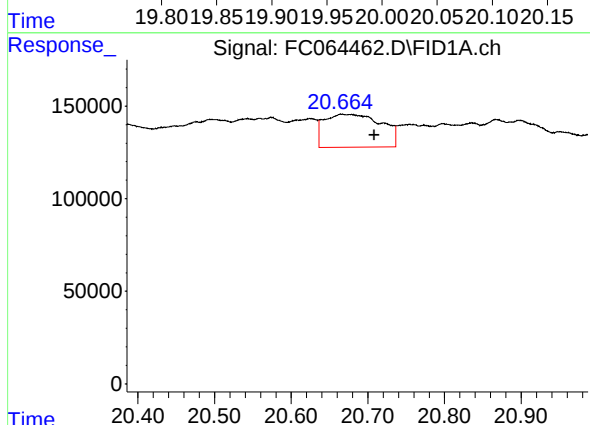

#21 n-Octatriacontane (C38)

R.T.: 20.667 min
Delta R.T.: -0.042 min
Response: 925320
Conc: 7.54 ug/ml

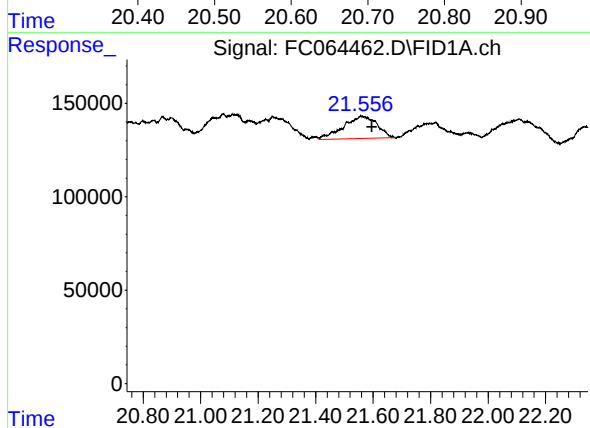

#22 n-Tetracontane (C40)

R.T.: 21.559 min
Delta R.T.: -0.037 min
Response: 978628
Conc: 8.43 ug/ml