

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC090222AL\
Data File : FC061420.D
Signal(s) : FID1A.ch
Acq On : 02 Sep 2022 09:35
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 05 01:17:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 082222.M
Quant Title : GC Extractables
QLast Update : Wed Aug 31 11:58:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.562	111143	0.715 ug/ml
11) T	n-Heneicosane (C21)	13.178	130991	0.837 ug/ml
13) T	n-Docosane (C22)	13.765	110698	0.713 ug/ml
14) T	n-Tetracosane (C24)	14.868	65254	0.422 ug/ml
15) T	n-Hexacosane (C26)	15.889	64475	0.428 ug/ml
16) T	n-Octacosane (C28)	16.839	83845	0.568 ug/ml
17) T	n-Tricontane (C30)	17.727	91165	0.660 ug/ml
18) T	n-Dotriacontane (C32)	18.554	188850	1.720 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC090222AL\
Data File : FC061420.D
Signal(s) : FID1A.ch
Acq On : 02 Sep 2022 09:35
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 05 01:17:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 082222.M
Quant Title : GC Extractables
QLast Update : Wed Aug 31 11:58:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

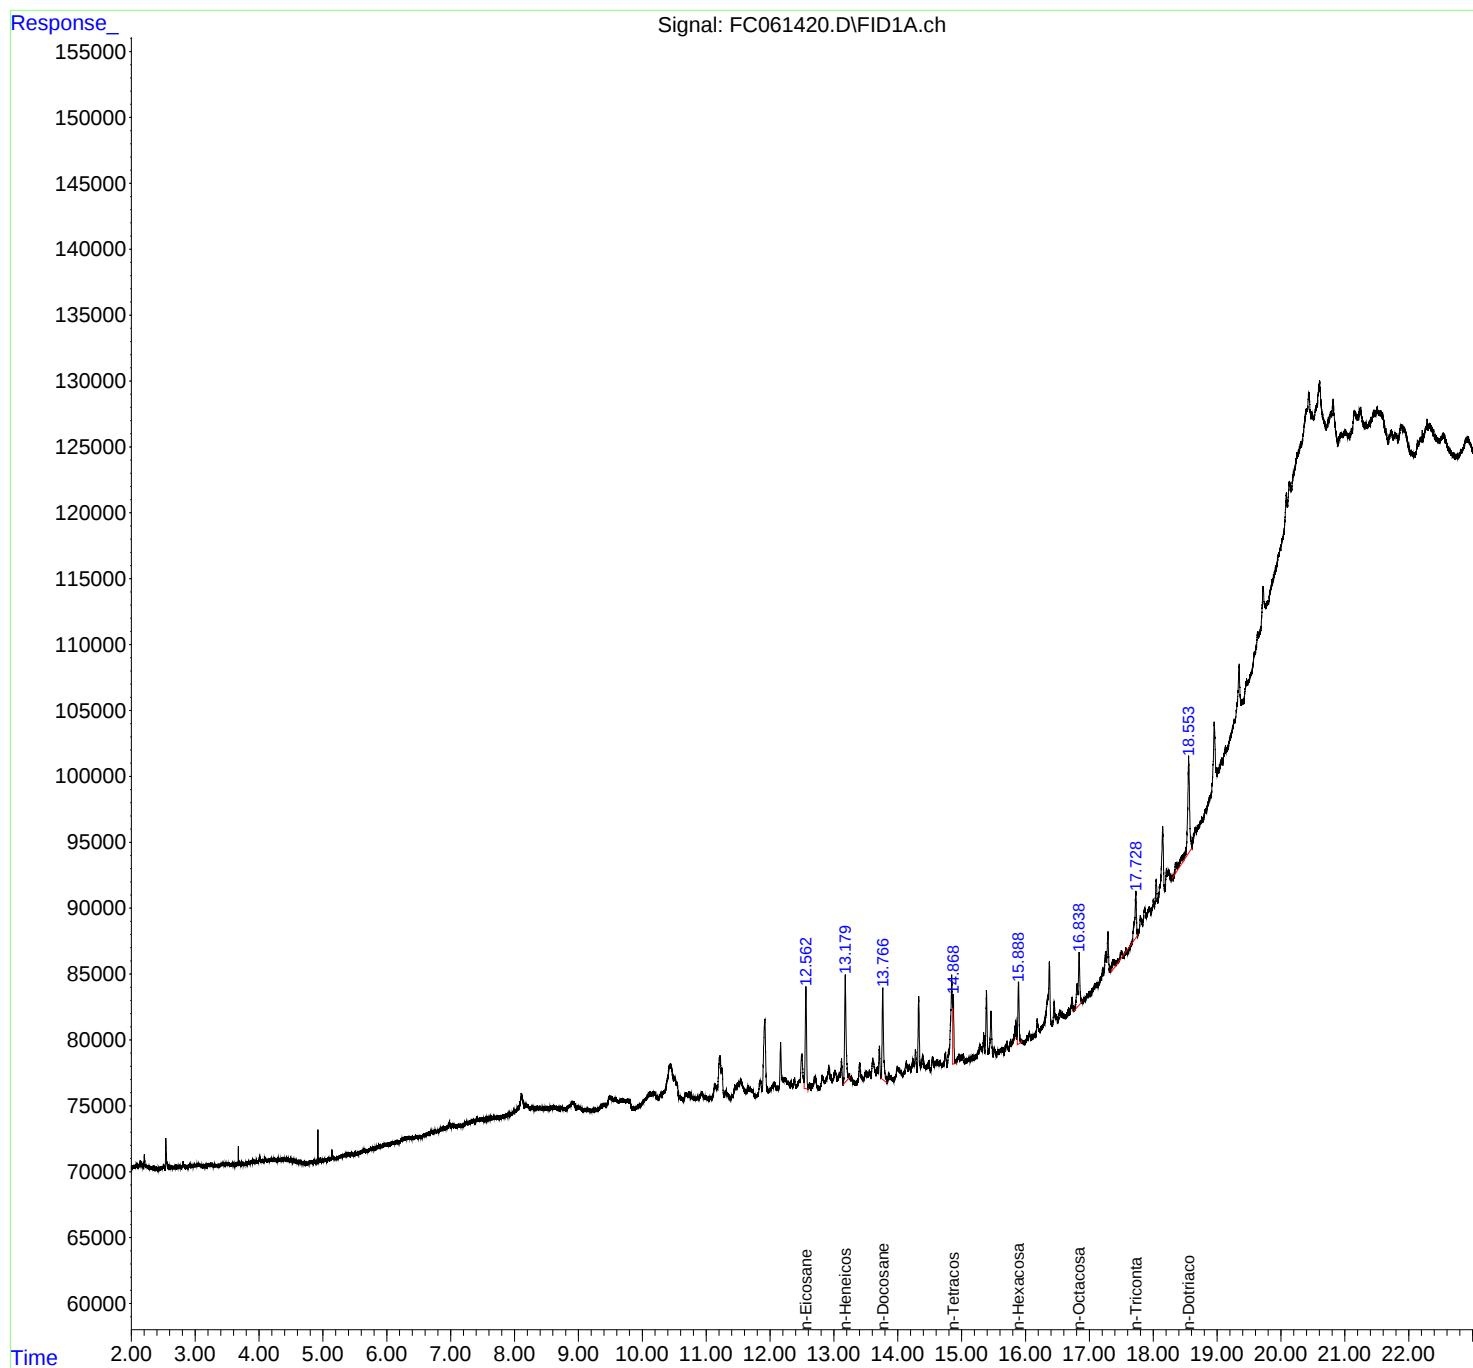


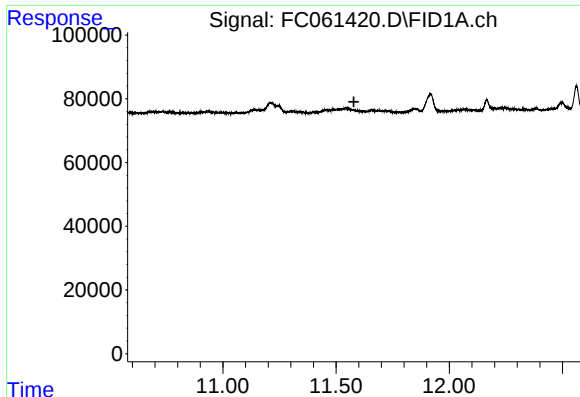

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.578 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

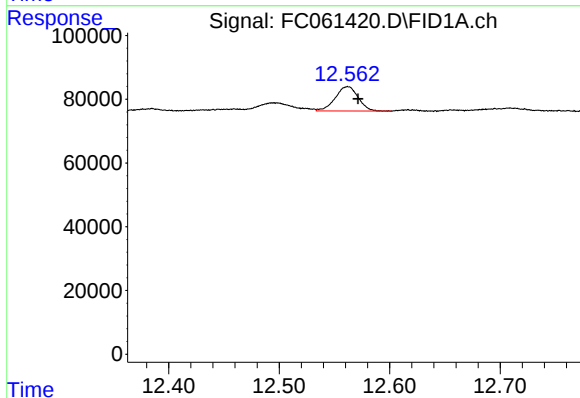


#10 n-Eicosane (C20)

R.T.: 12.562 min
Delta R.T.: -0.010 min
Response: 111143
Conc: 0.71 ug/ml

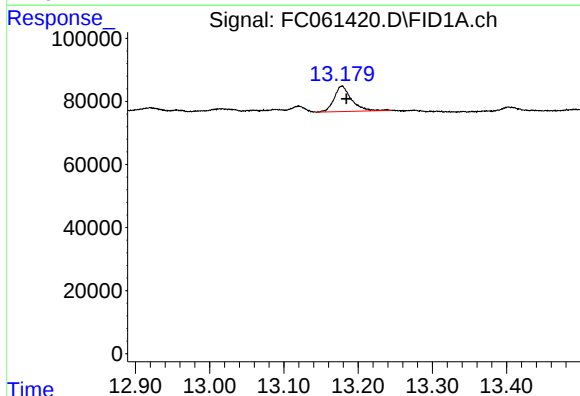


#11 n-Heneicosane (C21)

R.T.: 13.178 min
Delta R.T.: -0.006 min
Response: 130991
Conc: 0.84 ug/ml

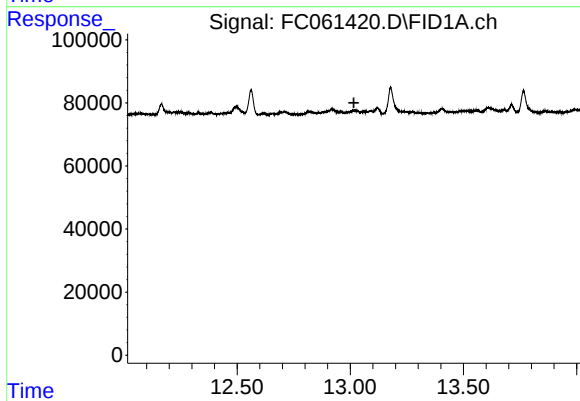

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.016 min
Response: 0
Conc: N.D.

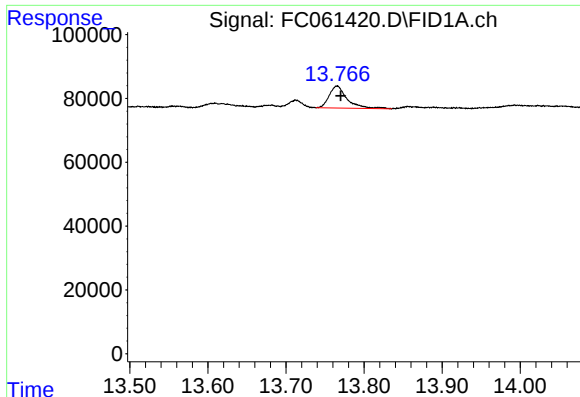

#13 n-Docosane (C22)


R.T.: 13.765 min
Delta R.T.: -0.005 min
Response: 110698
Conc: 0.71 ug/ml

Instrument :
FID_C
ClientSampleId :

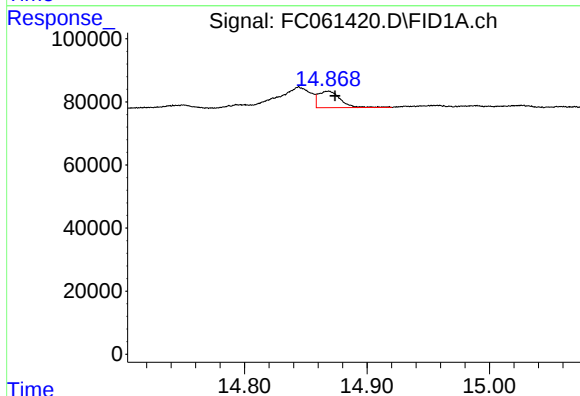


#14 n-Tetracosane (C24)

R.T.: 14.868 min
Delta R.T.: -0.006 min
Response: 65254
Conc: 0.42 ug/ml

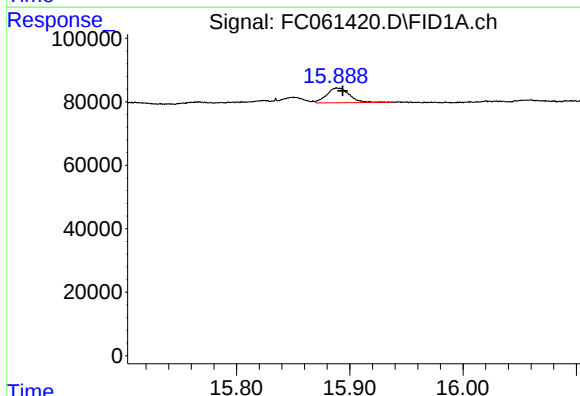


#15 n-Hexacosane (C26)

R.T.: 15.889 min
Delta R.T.: -0.004 min
Response: 64475
Conc: 0.43 ug/ml

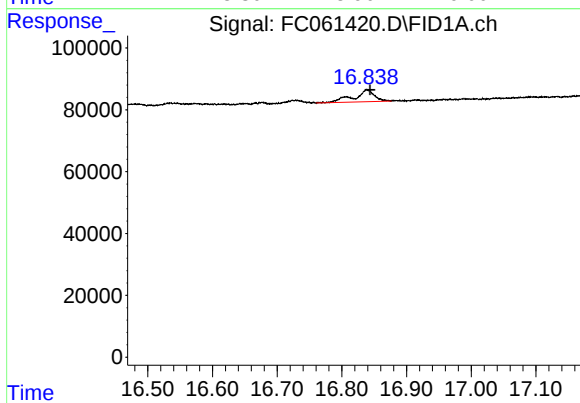

#16 n-Octacosane (C28)


R.T.: 16.839 min
Delta R.T.: -0.004 min
Response: 83845
Conc: 0.57 ug/ml

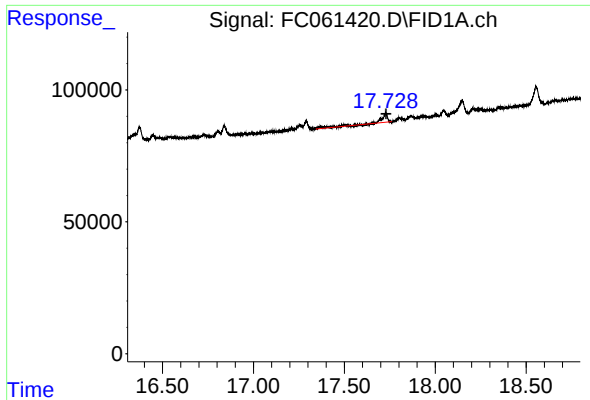

#17 n-Tricontane (C30)

R.T.: 17.727 min
Delta R.T.: -0.003 min
Response: 91165
Conc: 0.66 ug/ml

Instrument :
FID_C
ClientSampleId :

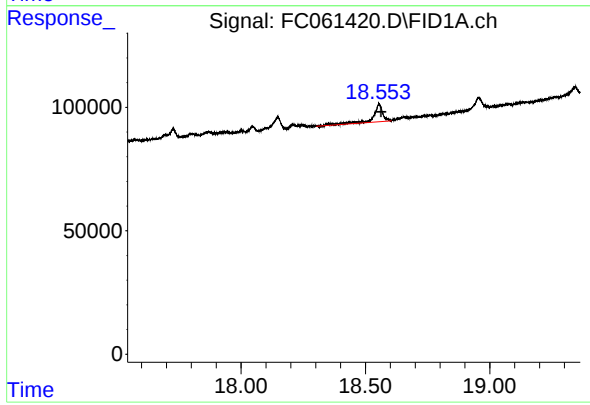

#18 n-Dotriacontane (C32)

R.T.: 18.554 min
Delta R.T.: -0.008 min
Response: 188850
Conc: 1.72 ug/ml