

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC090523AL\
 Data File : FC064489.D
 Signal(s) : FID1A.ch
 Acq On : 05 Sep 2023 08:43
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 06 00:18:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 081823.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 18 14:31:35 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.645	14583	0.100 ug/ml
18) T	n-Dotriacontane (C32)	18.476	8350	0.059 ug/ml
19) T	n-Tetratriacontane (C34)	19.253	19619	0.147 ug/ml
20) T	n-Hexatriacontane (C36)	20.000	20258	0.158 ug/ml
21) T	n-Octatriacontane (C38)	20.769f	56995	0.464 ug/ml
22) T	n-Tetracontane (C40)	21.592	194419	1.674 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC090523AL\
Data File : FC064489.D
Signal(s) : FID1A.ch
Acq On : 05 Sep 2023 08:43
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 06 00:18:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 081823.M
Quant Title : GC Extractables
QLast Update : Fri Aug 18 14:31:35 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

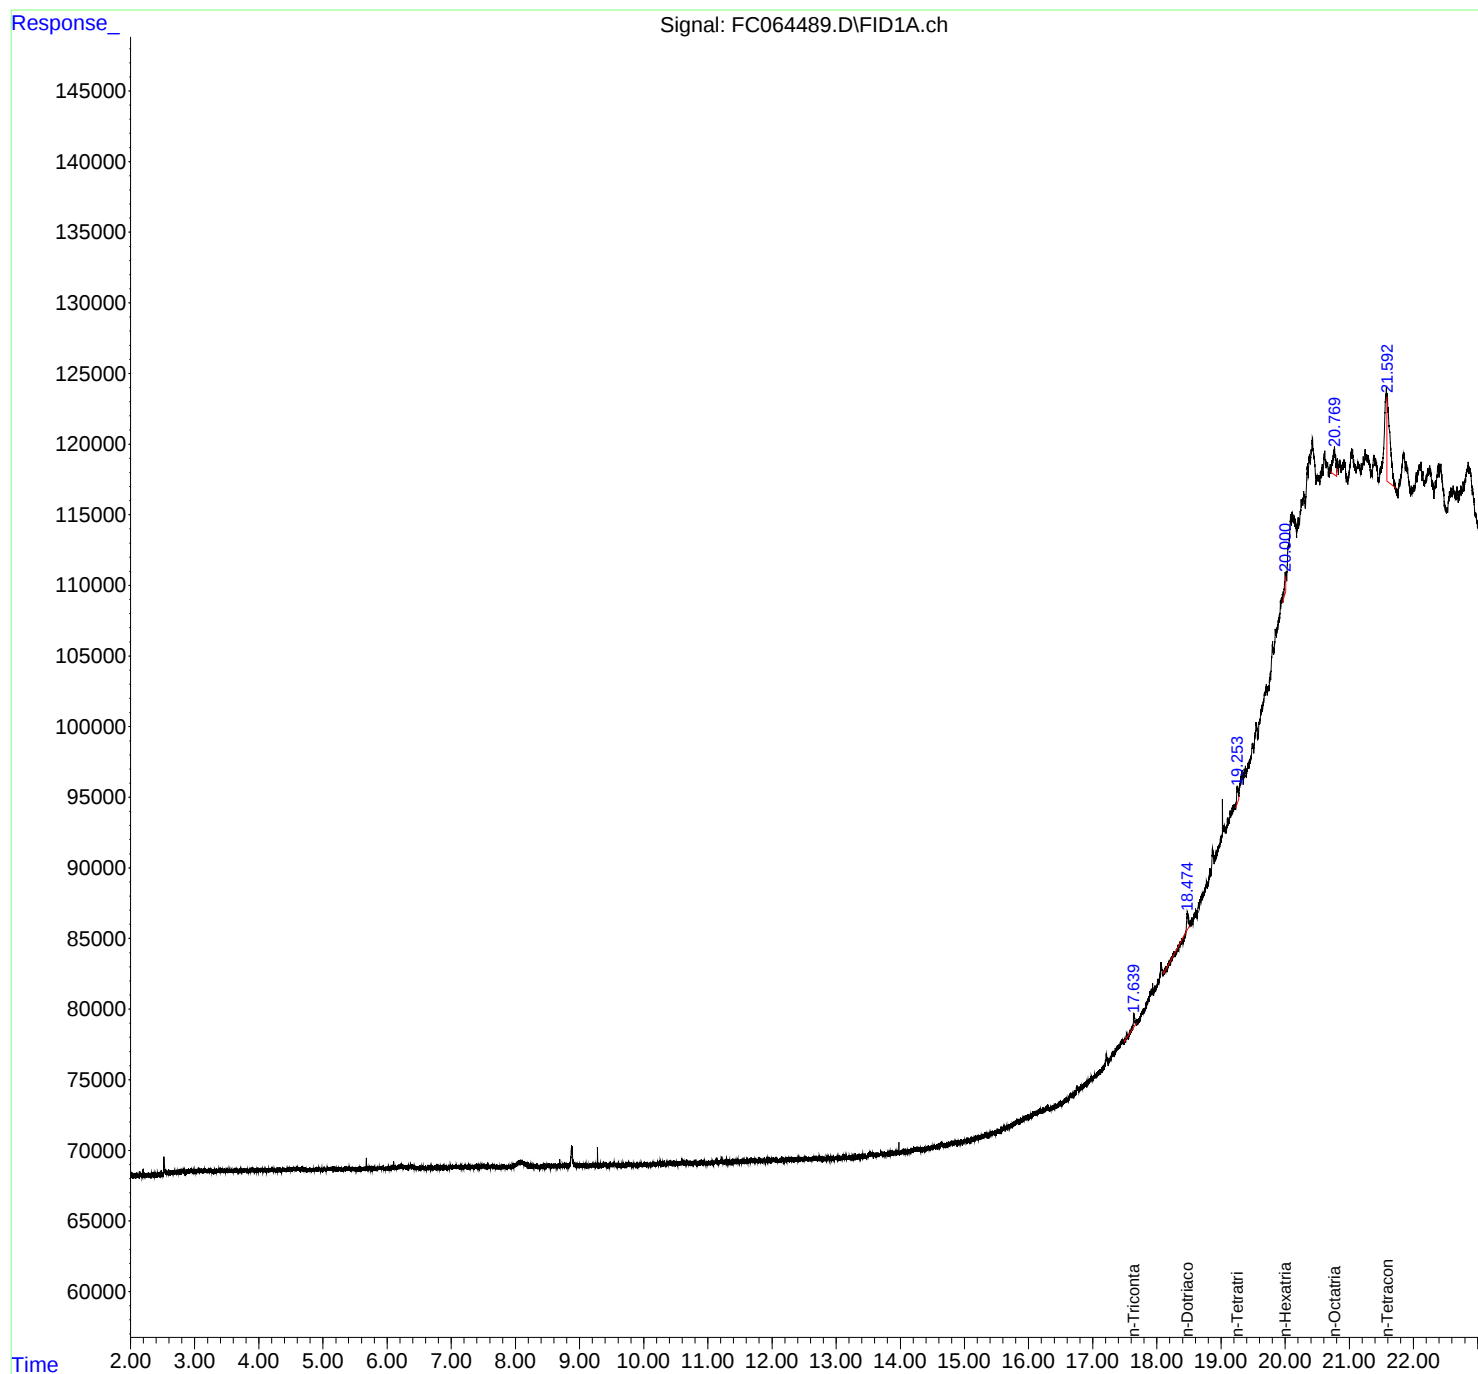


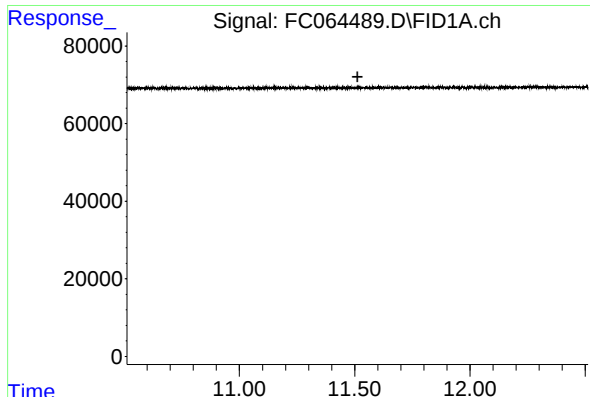

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.512 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

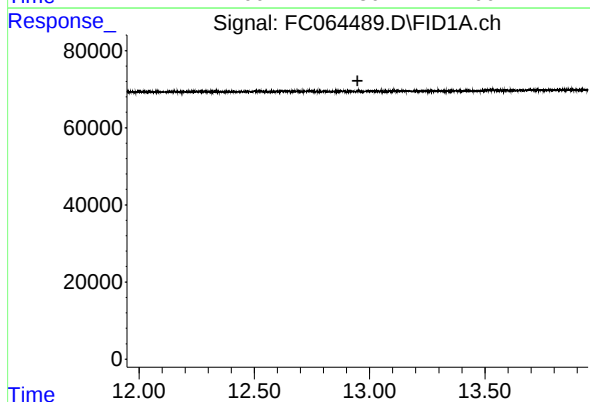


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.947 min
Response: 0
Conc: N.D.

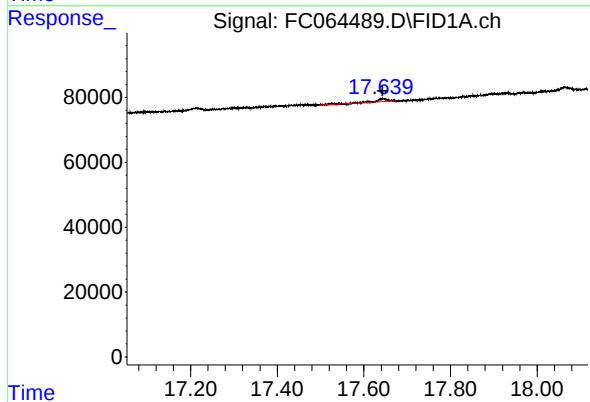


#17 n-Tricontane (C30)

R.T.: 17.645 min
Delta R.T.: 0.001 min
Response: 14583
Conc: 0.10 ug/ml

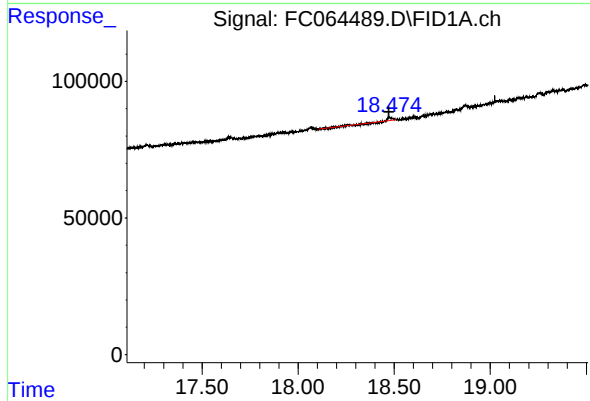

#18 n-Dotriacontane (C32)


R.T.: 18.476 min
Delta R.T.: 0.004 min
Response: 8350
Conc: 0.06 ug/ml

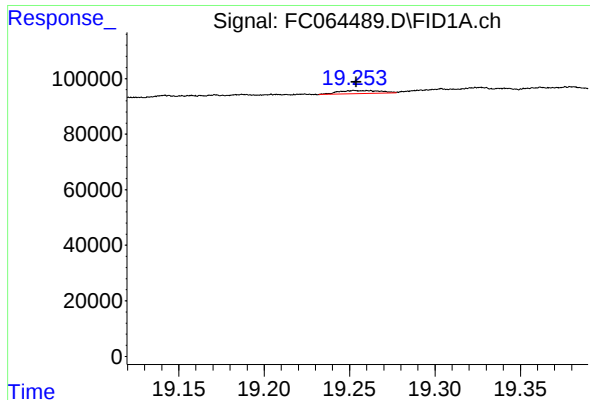

#19 n-Tetratriacontane (C34)


R.T.: 19.253 min
Delta R.T.: -0.001 min
Response: 19619
Conc: 0.15 ug/ml

Instrument :
FID_C
ClientSampleId :

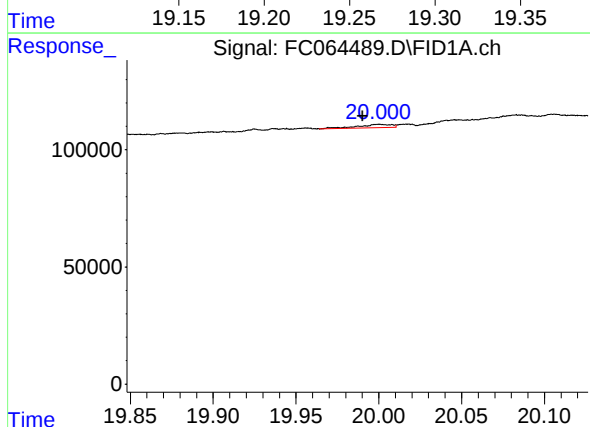


#20 n-Hexatriacontane (C36)

R.T.: 20.000 min
Delta R.T.: 0.010 min
Response: 20258
Conc: 0.16 ug/ml

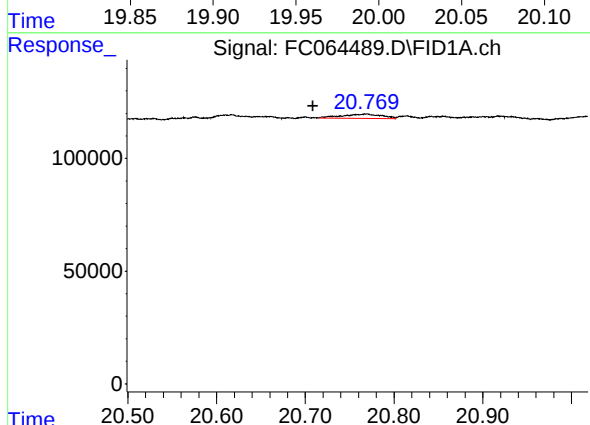

#21 n-Octatriacontane (C38)

R.T.: 20.769 min
Delta R.T.: 0.060 min
Response: 56995
Conc: 0.46 ug/ml

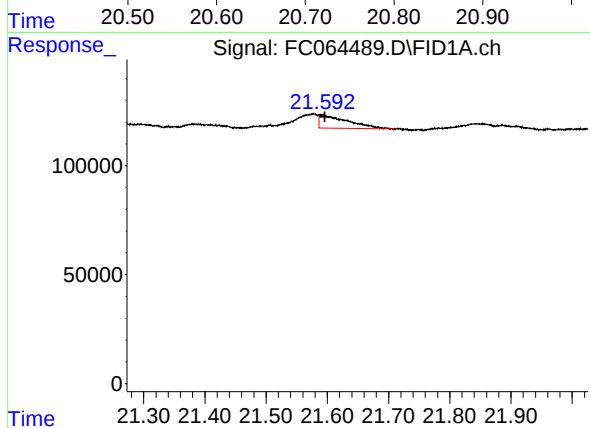

#22 n-Tetracontane (C40)

R.T.: 21.592 min
Delta R.T.: -0.004 min
Response: 194419
Conc: 1.67 ug/ml