

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC090523AL\
Data File : FC064497.D
Signal(s) : FID1A.ch
Acq On : 05 Sep 2023 15:40
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 06 00:18:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 081823.M
Quant Title : GC Extractables
QLast Update : Fri Aug 18 14:31:35 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.474	45615	0.323 ug/ml
19) T	n-Tetratriacontane (C34)	19.256	102534	0.767 ug/ml
20) T	n-Hexatriacontane (C36)	19.994	23539	0.184 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC090523AL\
Data File : FC064497.D
Signal(s) : FID1A.ch
Acq On : 05 Sep 2023 15:40
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 06 00:18:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 081823.M
Quant Title : GC Extractables
QLast Update : Fri Aug 18 14:31:35 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

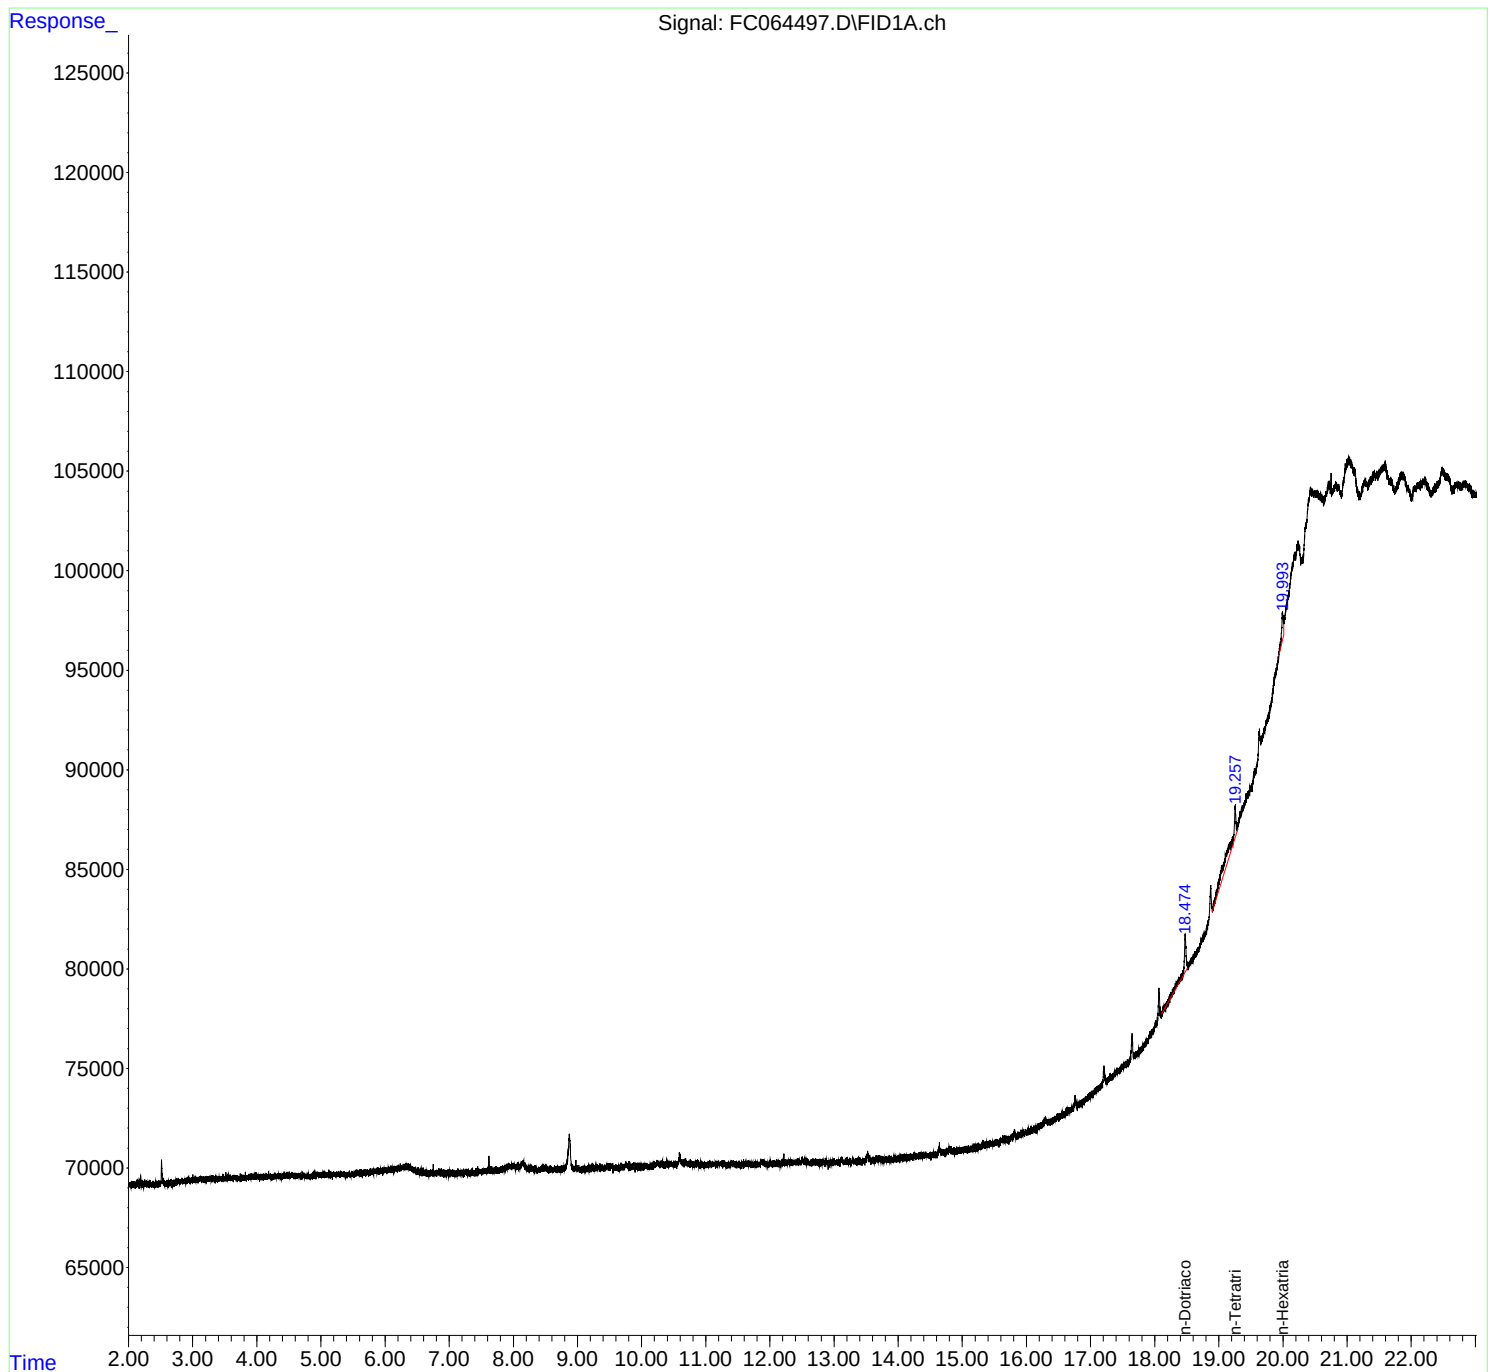


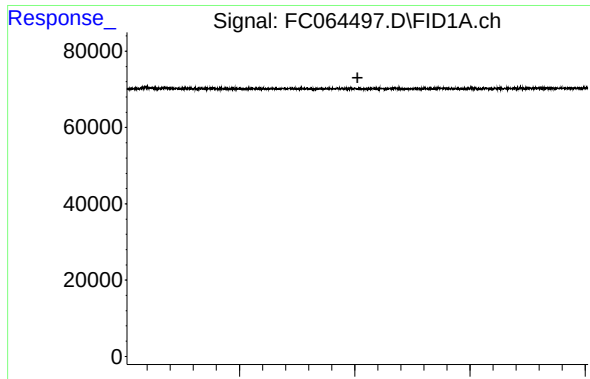

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.512 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

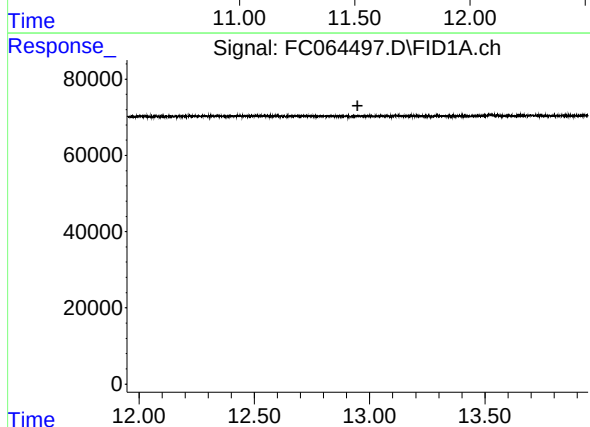


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.947 min
Response: 0
Conc: N.D.

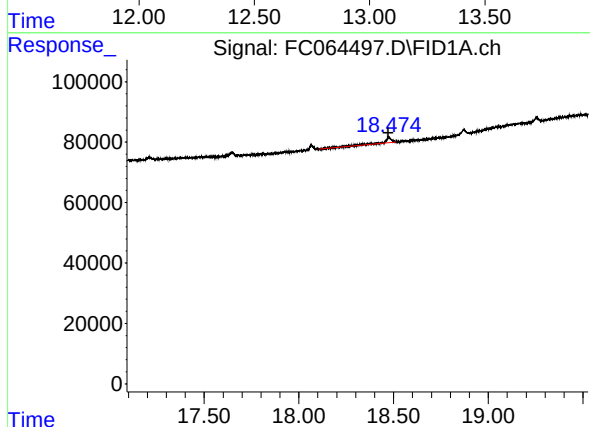


#18 n-Dotriacontane (C32)

R.T.: 18.474 min
Delta R.T.: 0.002 min
Response: 45615
Conc: 0.32 ug/ml

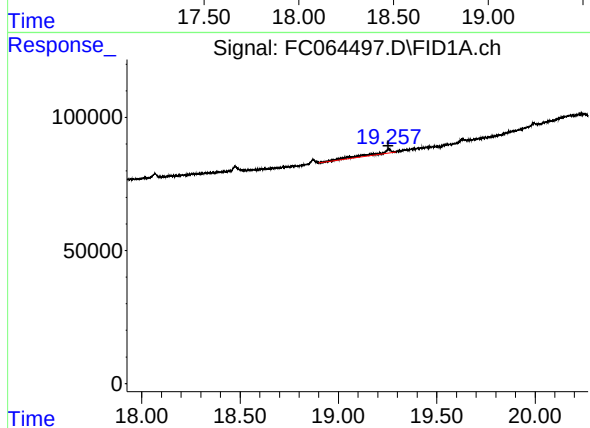

#19 n-Tetratriacontane (C34)

R.T.: 19.256 min
Delta R.T.: 0.002 min
Response: 102534
Conc: 0.77 ug/ml

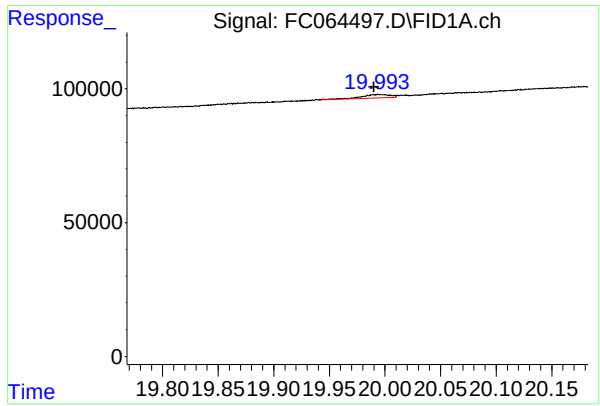

#20 n-Hexatriacontane (C36)

R.T.: 19.994 min
Delta R.T.: 0.004 min
Response: 23539
Conc: 0.18 ug/ml

Instrument :

FID_C

ClientSampleId :