

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC090922AL\
Data File : FC061463.D
Signal(s) : FID1A.ch
Acq On : 09 Sep 2022 09:33
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 12 03:02:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 082222.M
Quant Title : GC Extractables
QLast Update : Wed Aug 31 11:58:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.556	97915	0.630 ug/ml
11) T	n-Heneicosane (C21)	13.173	111094	0.710 ug/ml
13) T	n-Docosane (C22)	13.762	89463	0.577 ug/ml
14) T	n-Tetracosane (C24)	14.841	187041	1.209 ug/ml
15) T	n-Hexacosane (C26)	15.886	64567	0.429 ug/ml
18) T	n-Dotriacontane (C32)	18.555	77377	0.705 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC090922AL\
Data File : FC061463.D
Signal(s) : FID1A.ch
Acq On : 09 Sep 2022 09:33
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 12 03:02:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 082222.M
Quant Title : GC Extractables
QLast Update : Wed Aug 31 11:58:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

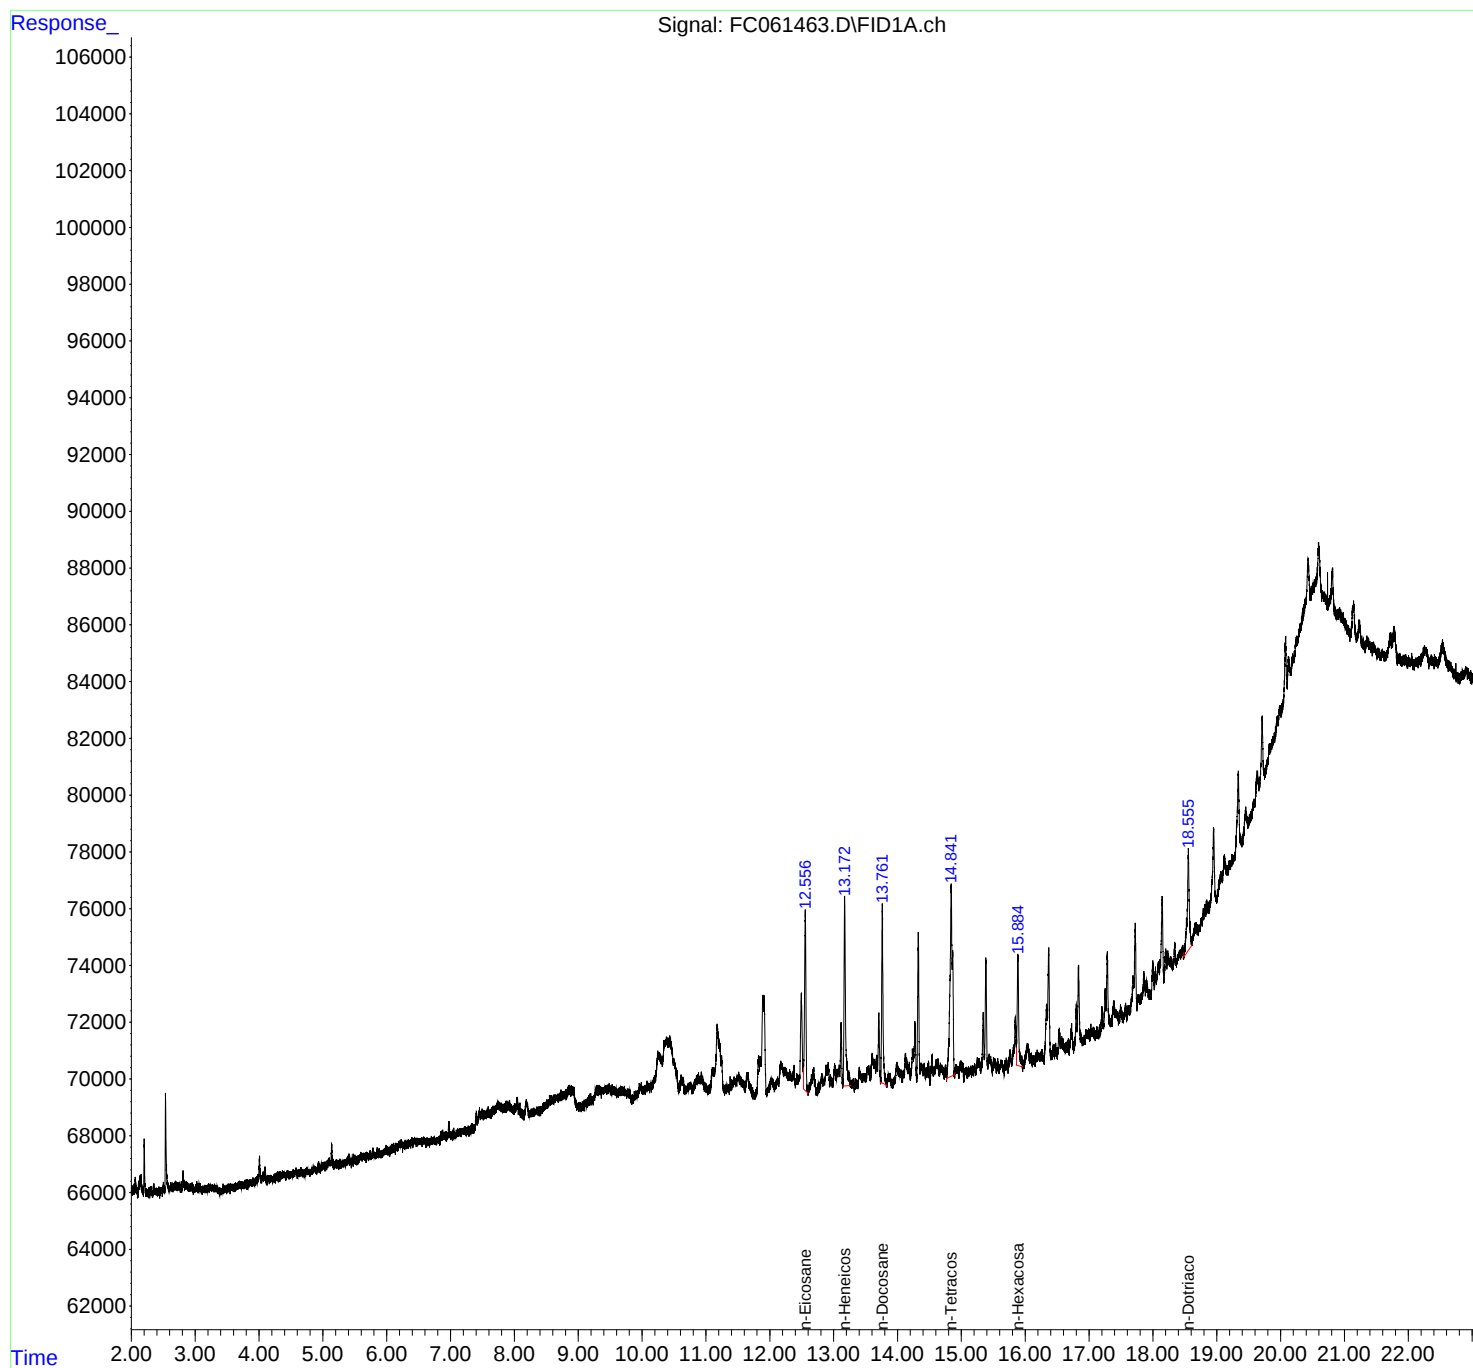


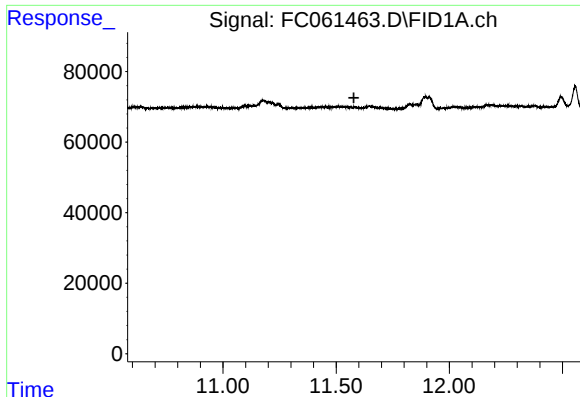

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.578 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

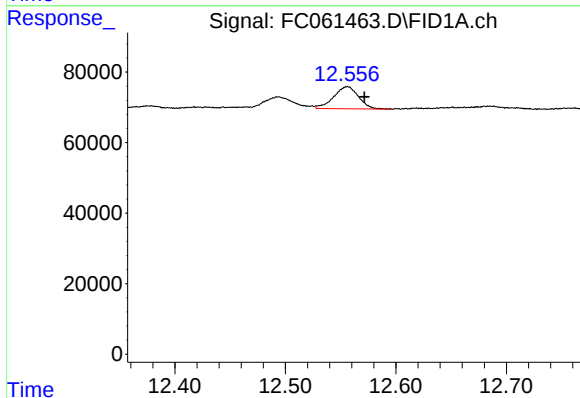


#10 n-Eicosane (C20)

R.T.: 12.556 min
Delta R.T.: -0.016 min
Response: 97915
Conc: 0.63 ug/ml

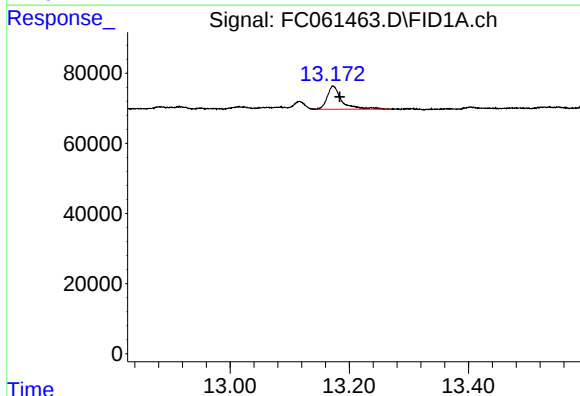


#11 n-Heneicosane (C21)

R.T.: 13.173 min
Delta R.T.: -0.011 min
Response: 111094
Conc: 0.71 ug/ml

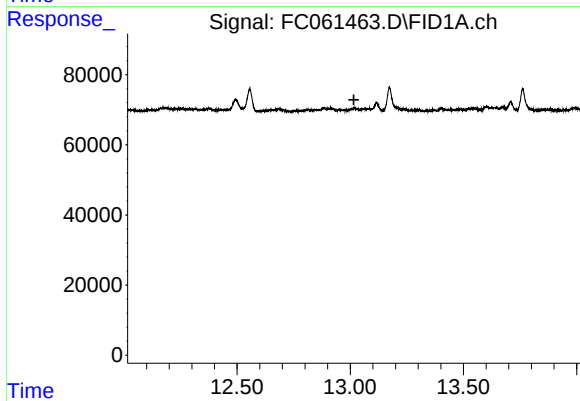

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.016 min
Response: 0
Conc: N.D.

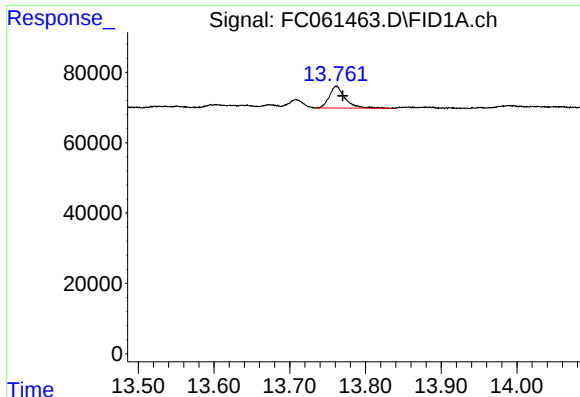

#13 n-Docosane (C22)


R.T.: 13.762 min
Delta R.T.: -0.008 min
Response: 89463
Conc: 0.58 ug/ml

Instrument :
FID_C
ClientSampleId :

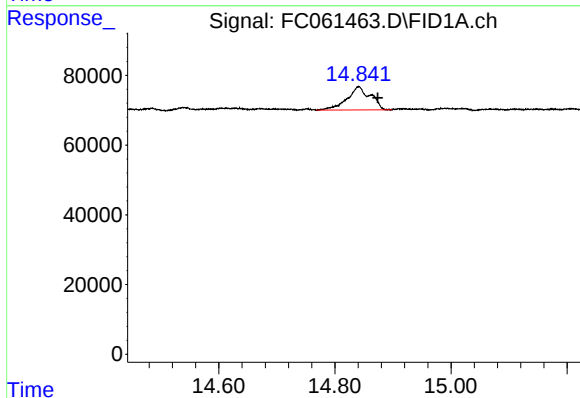


#14 n-Tetracosane (C24)

R.T.: 14.841 min
Delta R.T.: -0.033 min
Response: 187041
Conc: 1.21 ug/ml

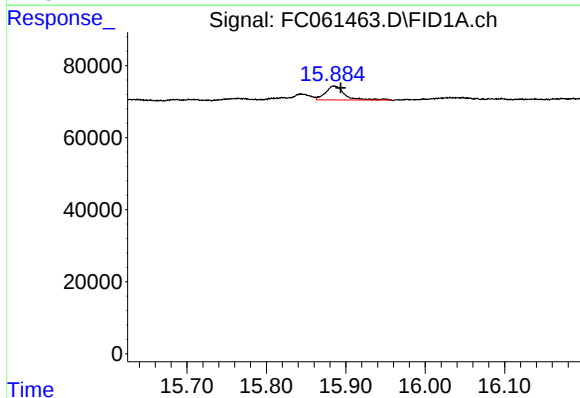

#15 n-Hexacosane (C26)

R.T.: 15.886 min
Delta R.T.: -0.008 min
Response: 64567
Conc: 0.43 ug/ml

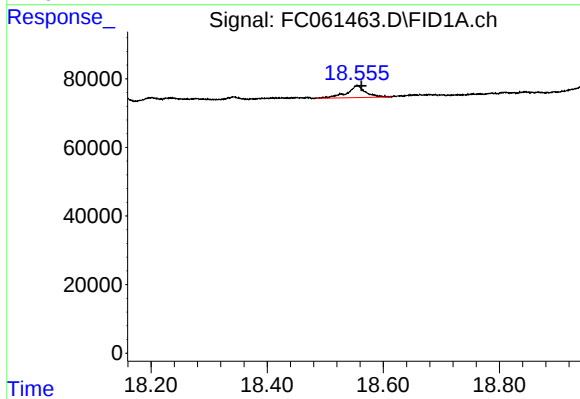

#18 n-Dotriacontane (C32)

R.T.: 18.555 min
Delta R.T.: -0.007 min
Response: 77377
Conc: 0.70 ug/ml