

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC091123AL\
 Data File : FC064530.D
 Signal(s) : FID1A.ch
 Acq On : 11 Sep 2023 11:16
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 12 02:54:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 081823.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 18 14:31:35 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) T n-Heneicosane (C21)	13.095	98027	0.587 ug/ml
13) T n-Docosane (C22)	13.686	150390	0.922 ug/ml
14) T n-Tetracosane (C24)	14.790	122399	0.769 ug/ml
15) T n-Hexacosane (C26)	15.807	96327	0.623 ug/ml
16) T n-Octacosane (C28)	16.753	64227	0.434 ug/ml
17) T n-Tricontane (C30)	17.637	43924	0.301 ug/ml
18) T n-Dotriacontane (C32)	18.466	122983	0.871 ug/ml
19) T n-Tetratriacontane (C34)	19.247	61579	0.461 ug/ml
20) T n-Hexatriacontane (C36)	19.987	43945	0.343 ug/ml
22) T n-Tetracontane (C40)	21.577	49822	0.429 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC091123AL\
Data File : FC064530.D
Signal(s) : FID1A.ch
Acq On : 11 Sep 2023 11:16
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 12 02:54:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 081823.M
Quant Title : GC Extractables
QLast Update : Fri Aug 18 14:31:35 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

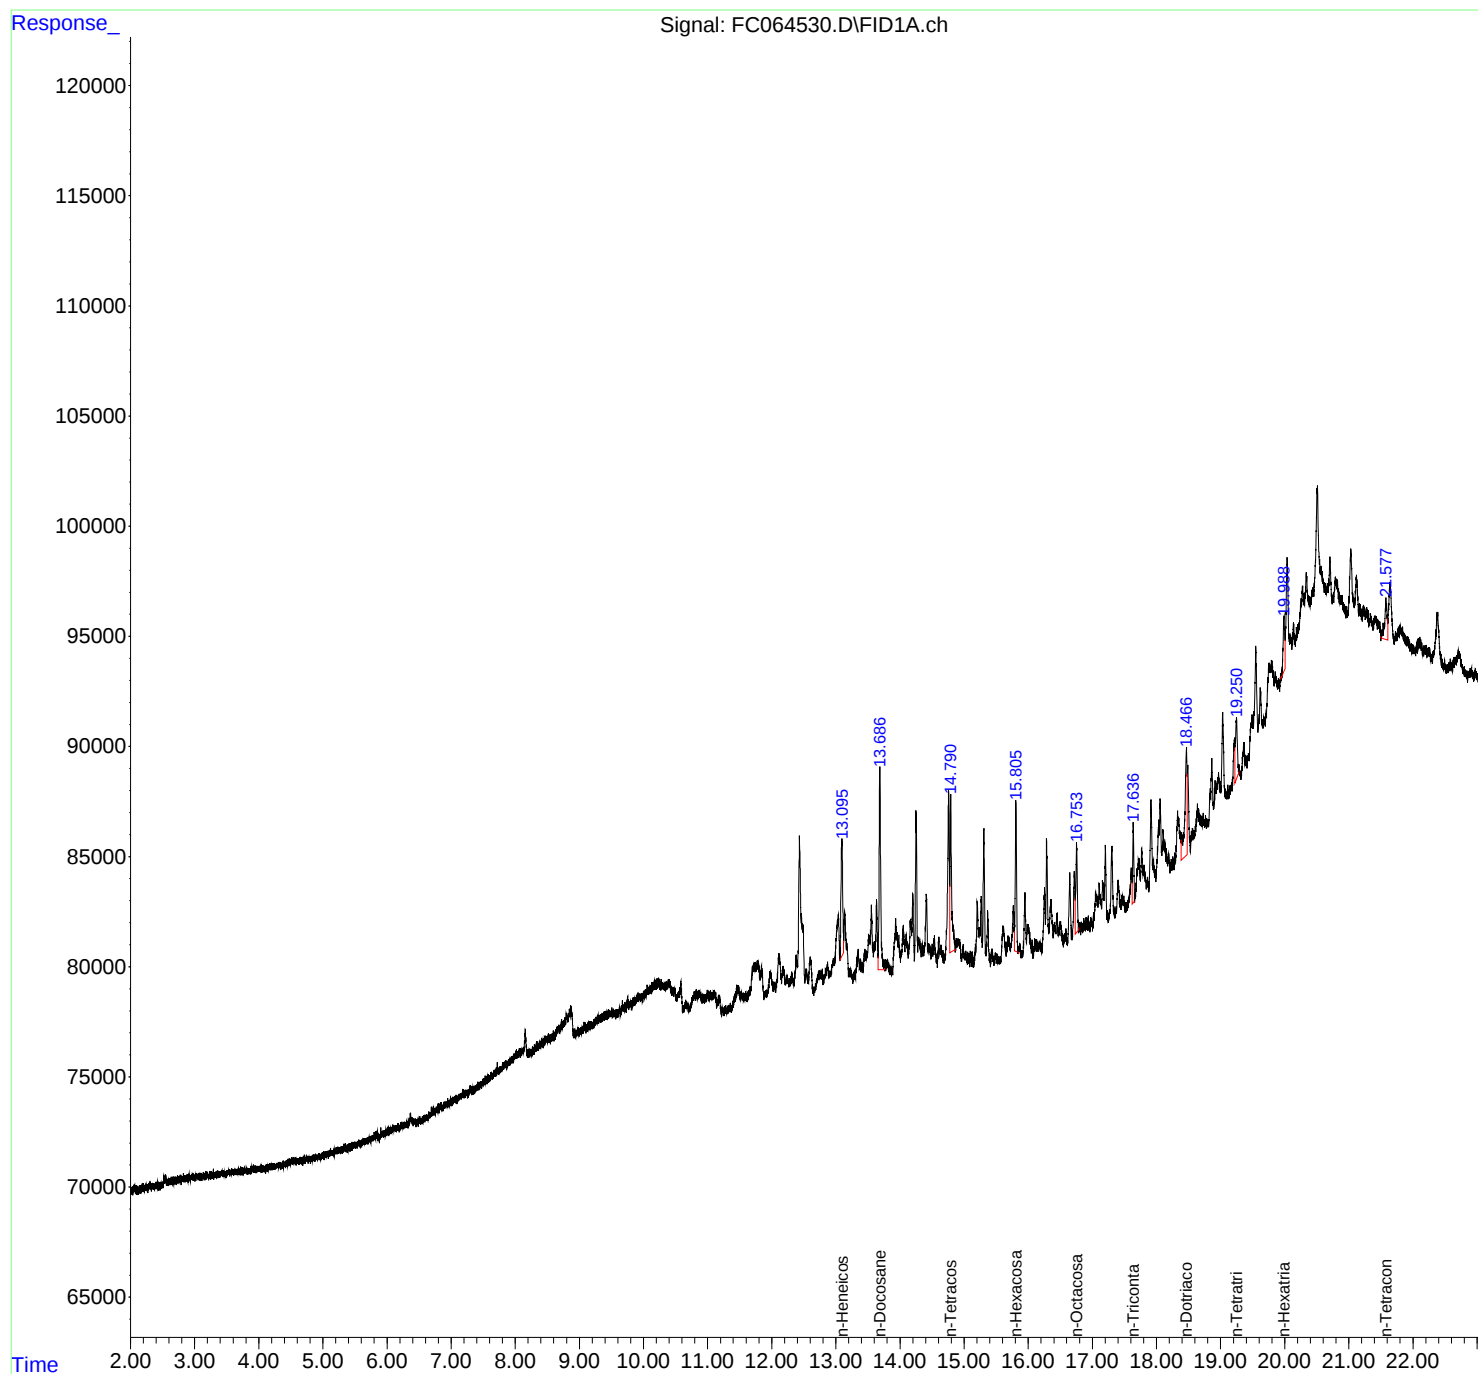


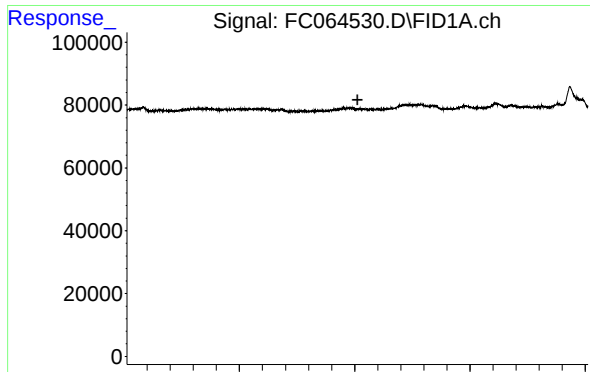

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.512 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

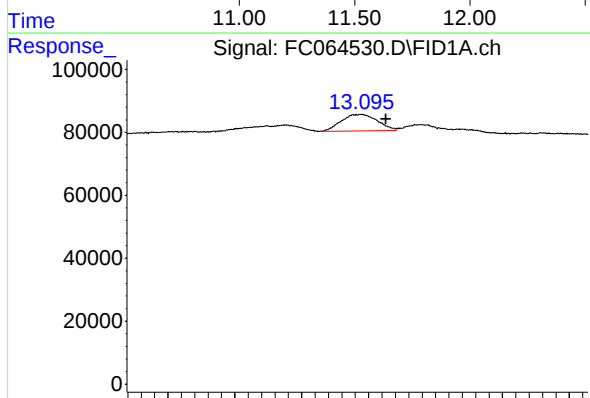


#11 n-Heneicosane (C21)

R.T.: 13.095 min
Delta R.T.: -0.018 min
Response: 98027
Conc: 0.59 ug/ml

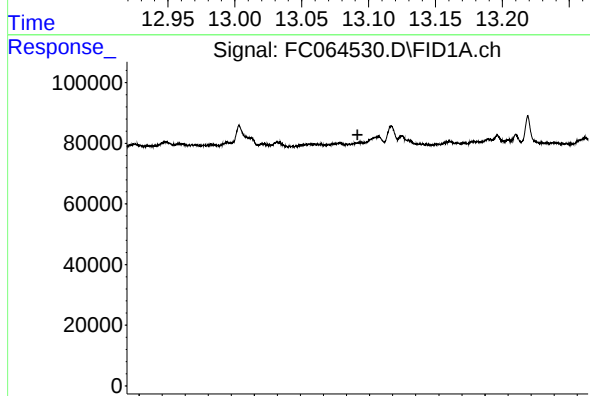


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.947 min
Response: 0
Conc: N.D.

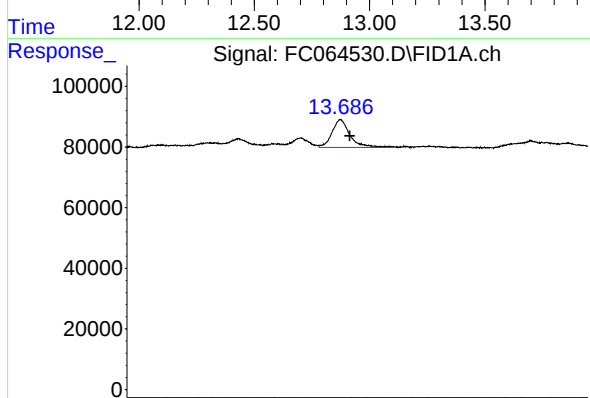

#13 n-Docosane (C22)


R.T.: 13.686 min
Delta R.T.: -0.013 min
Response: 150390
Conc: 0.92 ug/ml

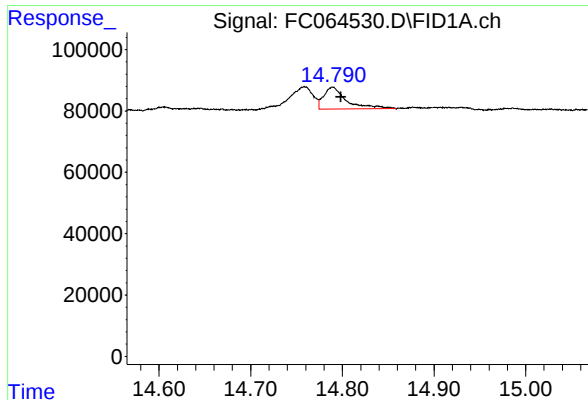

#14 n-Tetracosane (C24)


R.T.: 14.790 min
Delta R.T.: -0.009 min
Response: 122399
Conc: 0.77 ug/ml

Instrument :
FID_C
ClientSampleId :

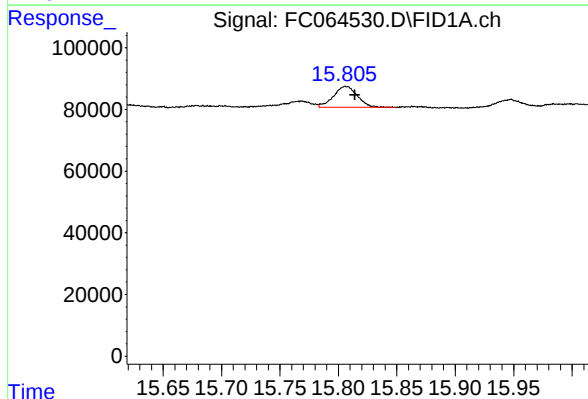


#15 n-Hexacosane (C26)

R.T.: 15.807 min
Delta R.T.: -0.007 min
Response: 96327
Conc: 0.62 ug/ml

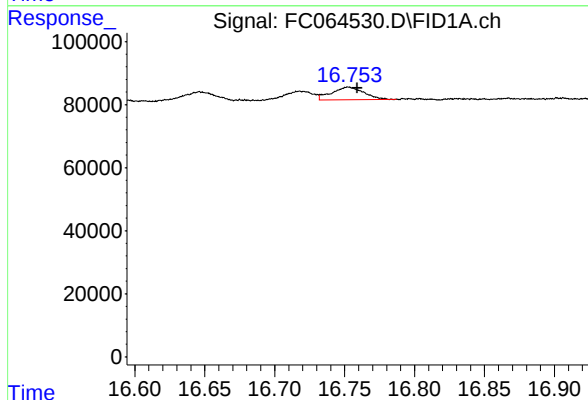


#16 n-Octacosane (C28)

R.T.: 16.753 min
Delta R.T.: -0.006 min
Response: 64227
Conc: 0.43 ug/ml

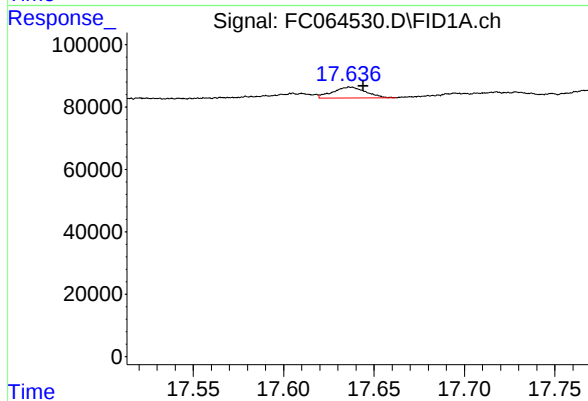

#17 n-Tricontane (C30)


R.T.: 17.637 min
Delta R.T.: -0.007 min
Response: 43924
Conc: 0.30 ug/ml

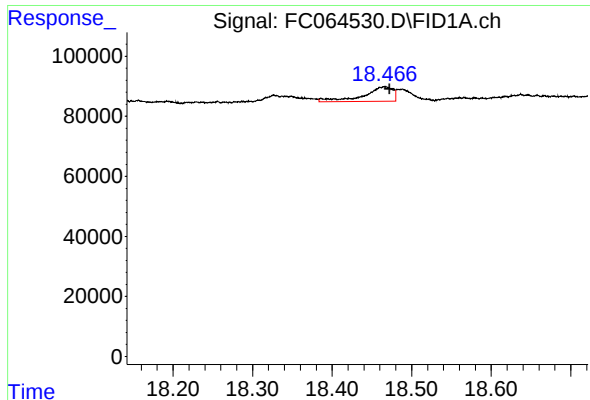

#18 n-Dotriacontane (C32)


R.T.: 18.466 min
Delta R.T.: -0.006 min
Response: 122983
Conc: 0.87 ug/ml

Instrument :
FID_C
ClientSampleId :

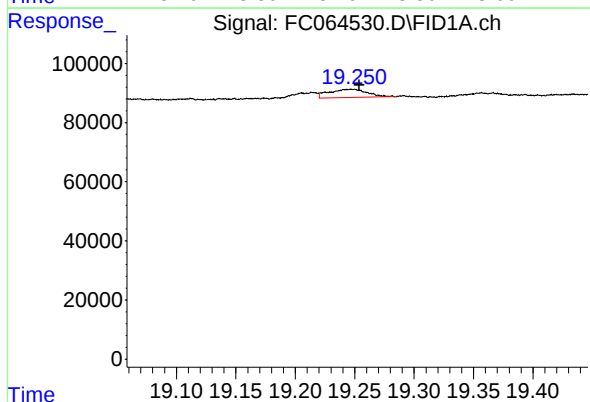


#19 n-Tetratriacontane (C34)

R.T.: 19.247 min
Delta R.T.: -0.006 min
Response: 61579
Conc: 0.46 ug/ml

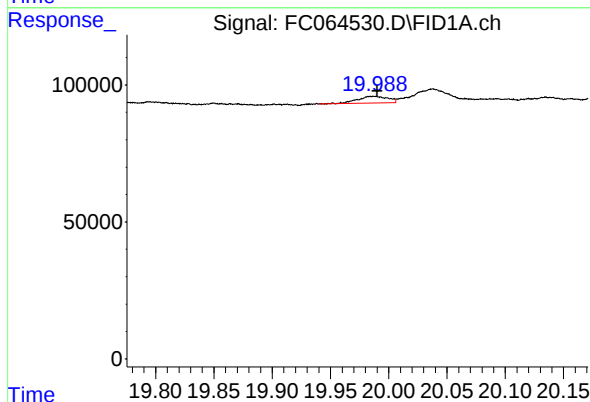

#20 n-Hexatriacontane (C36)

R.T.: 19.987 min
Delta R.T.: -0.003 min
Response: 43945
Conc: 0.34 ug/ml

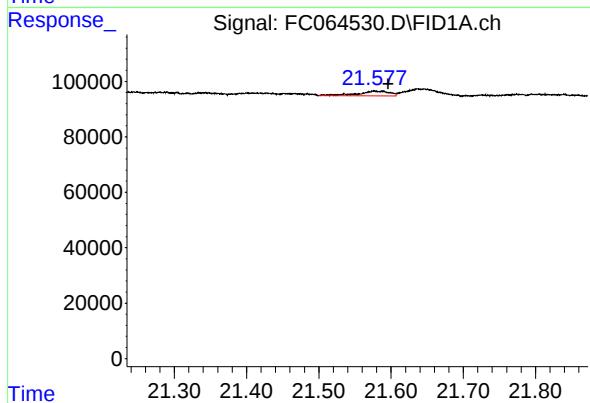

#22 n-Tetracontane (C40)

R.T.: 21.577 min
Delta R.T.: -0.019 min
Response: 49822
Conc: 0.43 ug/ml