

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC091422AL\
Data File : FC061502.D
Signal(s) : FID1A.ch
Acq On : 14 Sep 2022 08:51
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 14 12:58:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 082222.M
Quant Title : GC Extractables
QLast Update : Wed Aug 31 11:58:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.555	247579	2.256 ug/ml
21) T	n-Octatriacontane (C38)	20.809	523947	11.294 ug/ml
22) T	n-Tetracontane (C40)	21.721	301309	7.184 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC091422AL\
Data File : FC061502.D
Signal(s) : FID1A.ch
Acq On : 14 Sep 2022 08:51
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 14 12:58:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 082222.M
Quant Title : GC Extractables
QLast Update : Wed Aug 31 11:58:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

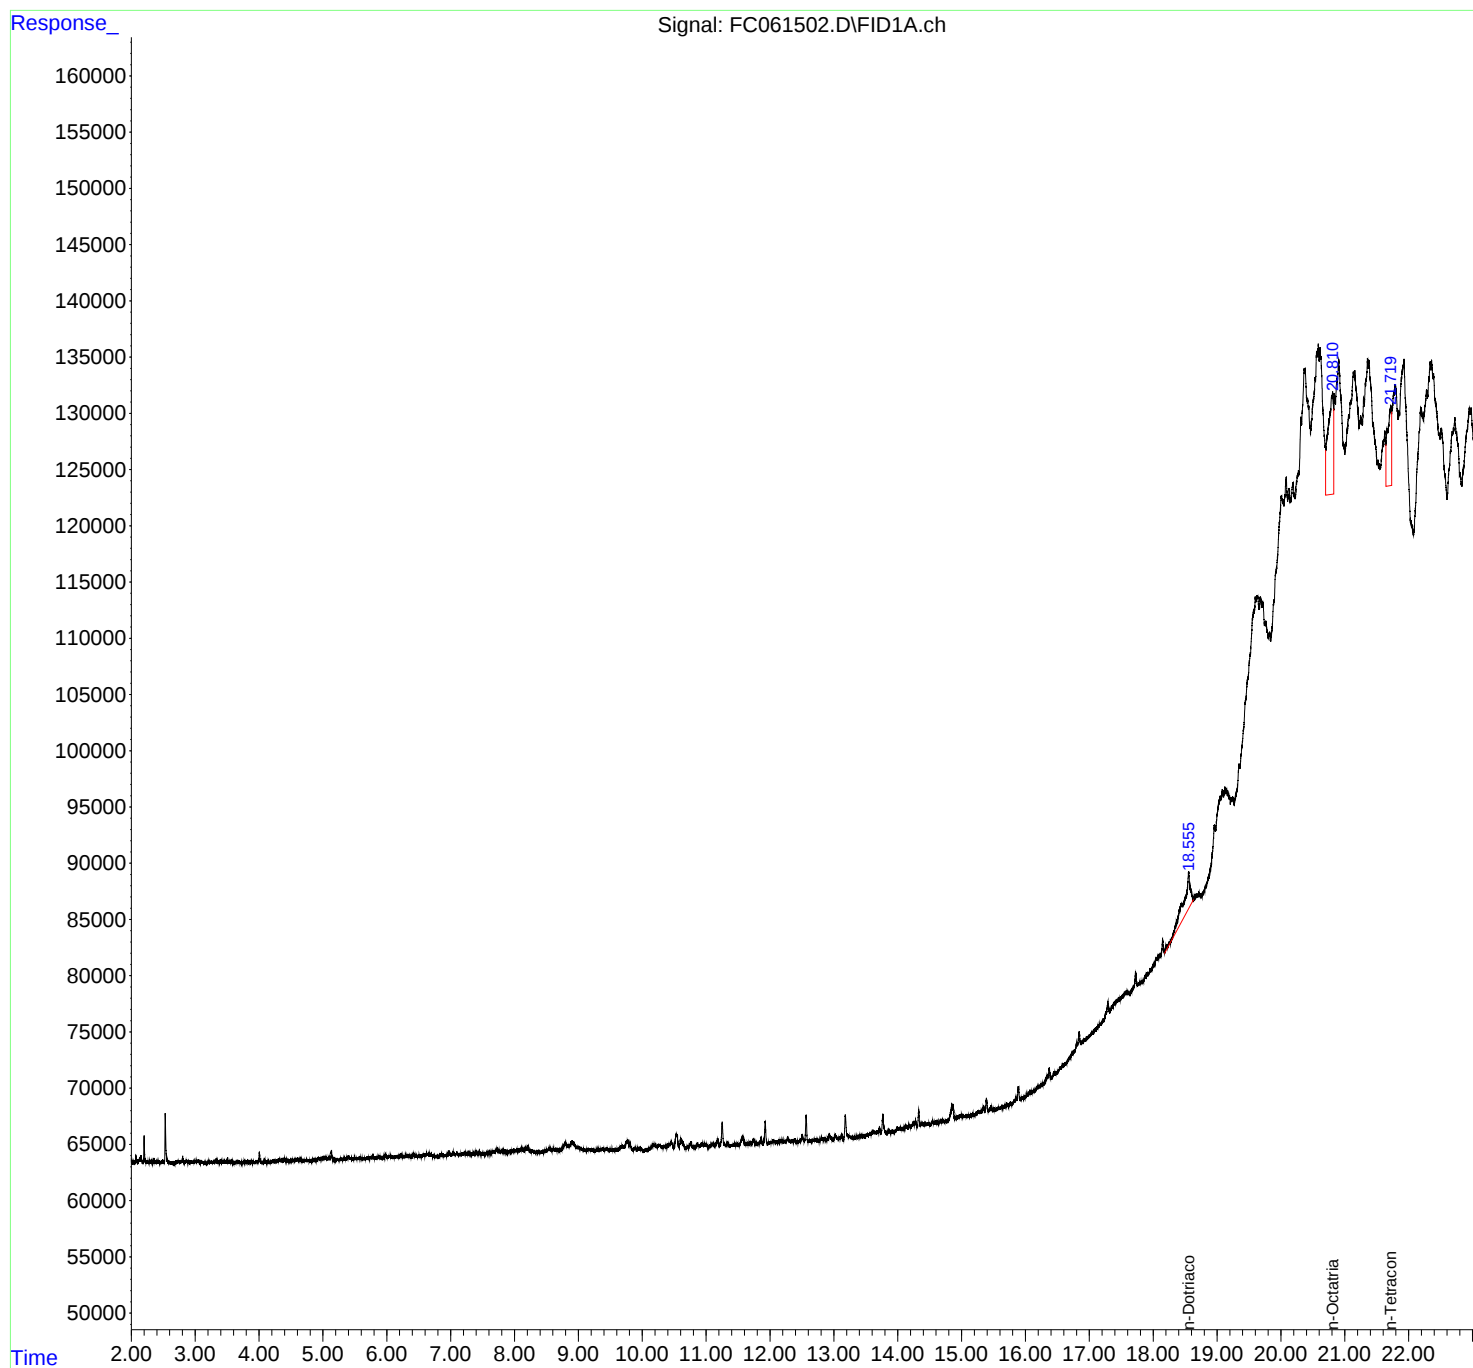


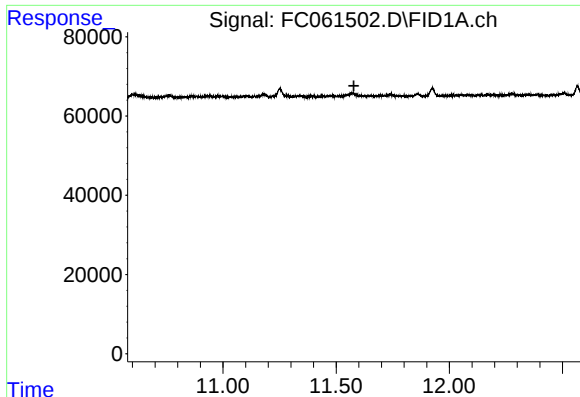

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.578 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

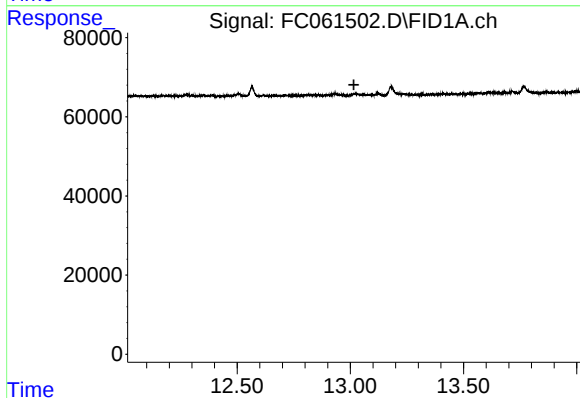


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.016 min
Response: 0
Conc: N.D.

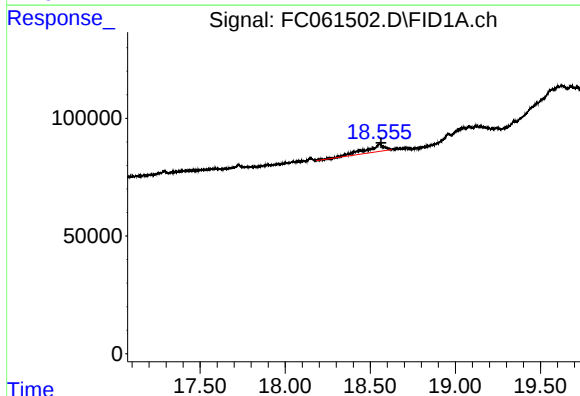


#18 n-Dotriacontane (C32)

R.T.: 18.555 min
Delta R.T.: -0.007 min
Response: 247579
Conc: 2.26 ug/ml

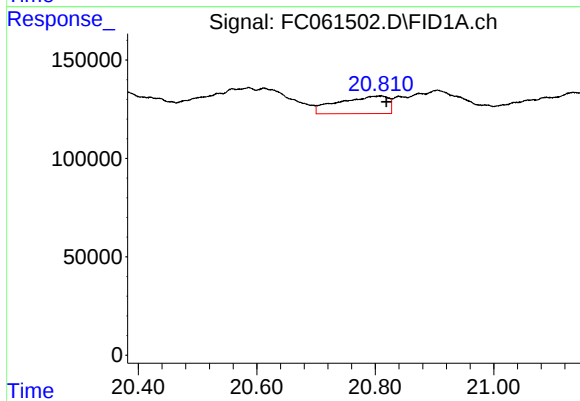

#21 n-Octatriacontane (C38)

R.T.: 20.809 min
Delta R.T.: -0.010 min
Response: 523947
Conc: 11.29 ug/ml

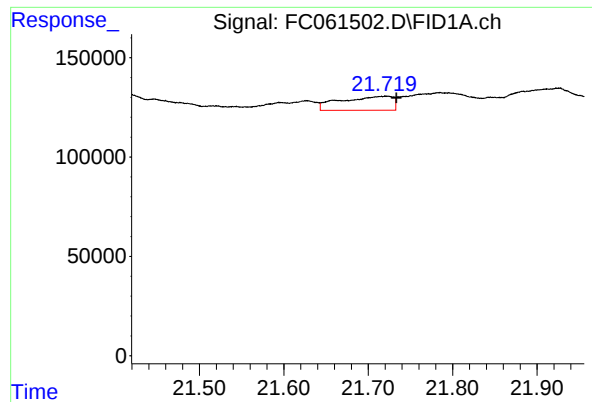

#22 n-Tetracontane (C40)

R.T.: 21.721 min
Delta R.T.: -0.012 min
Response: 301309
Conc: 7.18 ug/ml

Instrument :

FID_C

ClientSampleId :